

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050366.D
 Acq On : 1 Oct 2021 21:50
 Operator : CG/JU
 Sample : PB139404BS
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050366.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.641	22	26	29	rBV	12530	21602	1.03%	0.035%
2	3.676	29	32	39	rVB	28990	45031	2.14%	0.072%
3	4.076	93	100	118	rBV2	244989	692307	32.86%	1.108%
4	4.411	153	157	161	rVB4	4620	7241	0.34%	0.012%
5	4.622	190	193	201	rVV4	2704	4995	0.24%	0.008%
6	7.401	655	666	679	rBV2	467825	1236060	58.67%	1.979%
7	7.589	690	698	707	rBV	164170	292698	13.89%	0.469%
8	7.677	707	713	721	rVB	185312	303462	14.40%	0.486%
9	7.795	725	733	736	rBV	222740	418033	19.84%	0.669%
10	7.830	736	739	745	rVB	229378	350995	16.66%	0.562%
11	8.271	807	814	822	rVB	122411	210060	9.97%	0.336%
12	8.694	879	886	895	rVB	292614	516596	24.52%	0.827%
13	8.788	895	902	910	rBV2	164950	411419	19.53%	0.659%
14	8.847	910	912	917	rVB2	5643	6654	0.32%	0.011%
15	8.964	924	932	937	rBV	258724	472045	22.40%	0.756%
16	9.023	937	942	947	rVV	267749	515681	24.48%	0.826%
17	9.087	947	953	962	rVB2	346253	894893	42.47%	1.433%
18	9.364	993	1000	1007	rBV	199797	364437	17.30%	0.583%
19	9.440	1007	1013	1017	rVV	208788	406537	19.30%	0.651%
20	9.481	1017	1020	1030	rVB	224240	378324	17.96%	0.606%
21	10.010	1102	1110	1117	rBV	309339	550269	26.12%	0.881%
22	10.169	1128	1137	1139	rBV	176955	328816	15.61%	0.526%
23	10.198	1139	1142	1145	rVV	185443	318152	15.10%	0.509%
24	10.239	1145	1149	1158	rVV	303449	536215	25.45%	0.858%
25	10.310	1158	1161	1166	rVV3	3739	6073	0.29%	0.010%
26	10.486	1184	1191	1200	rVB	224529	380593	18.06%	0.609%
27	10.703	1220	1228	1230	rBV	282296	503783	23.91%	0.807%
28	11.097	1286	1295	1299	rBV	163199	313931	14.90%	0.503%
29	11.144	1299	1303	1310	rVV	369249	679321	32.24%	1.088%
30	11.238	1310	1319	1330	rVB2	313974	945289	44.87%	1.513%
31	11.420	1343	1350	1358	rBV	282867	493155	23.41%	0.790%
32	12.008	1442	1450	1454	rBV2	105971	222669	10.57%	0.356%
33	12.337	1499	1506	1517	rBV	313914	537716	25.52%	0.861%
34	12.607	1544	1552	1558	rBV5	14396	38443	1.82%	0.062%
35	12.660	1558	1561	1565	rVB2	4592	5811	0.28%	0.009%
36	12.730	1565	1573	1580	rBV	472644	799171	37.93%	1.279%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050366.D
 Acq On : 1 Oct 2021 21:50
 Operator : CG/JU
 Sample : PB139404BS
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	12.848	1586	1593	1600	rBV3	10913	17760	0.84%	0.028%
38	12.948	1602	1610	1623	rVV	452384	777882	36.92%	1.245%
39	13.089	1623	1634	1643	rVB2	417474	991478	47.06%	1.587%
40	13.324	1665	1674	1680	rBV	344471	545640	25.90%	0.874%
41	13.394	1680	1686	1694	rVV	324413	538867	25.58%	0.863%
42	13.694	1729	1737	1739	rBV	410194	687048	32.61%	1.100%
43	13.723	1739	1742	1746	rVV	556321	846940	40.20%	1.356%
44	13.770	1746	1750	1758	rVB	445566	719199	34.14%	1.151%
45	13.964	1774	1783	1791	rBV	274505	455766	21.63%	0.730%
46	14.187	1817	1821	1826	rVB3	6076	8547	0.41%	0.014%
47	14.281	1830	1837	1841	rVV	453764	684545	32.49%	1.096%
48	14.328	1841	1845	1853	rVB	473905	672891	31.94%	1.077%
49	14.452	1860	1866	1873	rBV	324789	487019	23.12%	0.780%
50	14.587	1881	1889	1891	rBV	505237	879444	41.74%	1.408%
51	14.610	1891	1893	1904	rVB	475136	668045	31.71%	1.070%
52	14.781	1915	1922	1931	rBV	283029	441417	20.95%	0.707%
53	14.887	1933	1940	1945	rBV	263033	409630	19.44%	0.656%
54	14.951	1945	1951	1962	rVV2	585214	1164378	55.27%	1.864%
55	15.063	1962	1970	1982	rVV2	405811	849396	40.32%	1.360%
56	15.198	1985	1993	1996	rVV	438893	703415	33.39%	1.126%
57	15.233	1996	1999	2003	rVV	316864	472503	22.43%	0.756%
58	15.280	2003	2007	2016	rVB	515340	815155	38.69%	1.305%
59	15.498	2037	2044	2055	rBV	369984	576758	27.37%	0.923%
60	15.686	2069	2076	2085	rVB	537284	757179	35.94%	1.212%
61	15.874	2100	2108	2112	rBV	650285	1035050	49.13%	1.657%
62	15.926	2112	2117	2123	rVV3	967693	2106882	100.00%	3.373%
63	15.985	2123	2127	2137	rVB3	340179	642724	30.51%	1.029%
64	16.126	2145	2151	2158	rBV	638450	954444	45.30%	1.528%
65	16.179	2158	2160	2165	rVB3	4550	5377	0.26%	0.009%
66	16.514	2213	2217	2221	rBV3	5236	6385	0.30%	0.010%
67	16.814	2261	2268	2274	rBV	486721	727964	34.55%	1.165%
68	16.931	2281	2288	2294	rBV	448152	703224	33.38%	1.126%
69	17.066	2304	2311	2317	rBV	543973	749840	35.59%	1.200%
70	17.266	2339	2345	2359	rVV	354915	549990	26.10%	0.881%
71	17.425	2367	2372	2377	rBV2	17414	23243	1.10%	0.037%
72	17.630	2401	2407	2410	rBV	327371	513745	24.38%	0.823%
73	17.671	2410	2414	2419	rVV	741094	1151593	54.66%	1.844%
74	17.730	2419	2424	2427	rVV	686332	1121182	53.22%	1.795%
75	17.765	2427	2430	2441	rVB	730297	1039506	49.34%	1.664%
76	18.030	2468	2475	2481	rBV	674161	1024544	48.63%	1.640%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050366.D
 Acq On : 1 Oct 2021 21:50
 Operator : CG/JU
 Sample : PB139404BS
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SLCS404

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

77	18.570	2561	2567	2573	rVV	752198	957853	45.46%	1.534%
78	18.829	2607	2611	2616	rVB5	4229	7823	0.37%	0.013%
79	19.416	2706	2711	2715	rVV8	4590	8269	0.39%	0.013%
80	19.569	2730	2737	2741	rBV4	8174	15200	0.72%	0.024%
81	19.669	2743	2754	2761	rVB	930879	1364402	64.76%	2.184%
82	19.898	2788	2793	2801	rVB3	60525	94736	4.50%	0.152%
83	20.004	2803	2811	2813	rBV	919762	1413568	67.09%	2.263%
84	20.033	2813	2816	2823	rVB	912689	1239090	58.81%	1.984%
85	20.133	2828	2833	2841	rVV	80037	111138	5.27%	0.178%
86	20.574	2906	2908	2910	rBV3	4692	4070	0.19%	0.007%
87	20.903	2959	2964	2970	rBV	819632	973680	46.21%	1.559%
88	21.150	3001	3006	3012	rBV2	40572	62057	2.95%	0.099%
89	21.796	3110	3116	3127	rBV2	913243	2023752	96.05%	3.240%
90	21.914	3129	3136	3143	rVV2	814528	1878743	89.17%	3.008%
91	21.984	3143	3148	3155	rVB	775727	1326094	62.94%	2.123%
92	23.018	3319	3324	3329	rBV	74544	138349	6.57%	0.221%
93	23.083	3329	3335	3343	rVB	670446	1172321	55.64%	1.877%
94	24.258	3525	3535	3541	rBV	525582	1359304	64.52%	2.176%
95	24.334	3541	3548	3559	rVB	538761	1349970	64.07%	2.161%
96	25.122	3671	3682	3688	rBV2	401048	1235884	58.66%	1.979%
97	25.192	3688	3694	3705	rVB	423575	1197031	56.82%	1.916%
98	25.357	3713	3722	3736	rVB	179366	568908	27.00%	0.911%
99	29.287	4376	4391	4395	rBV4	252517	1022107	48.51%	1.636%
100	30.515	4585	4600	4618	rVB2	239068	1201613	57.03%	1.924%

Sum of corrected areas: 62461034

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050366.D
Acq On : 1 Oct 2021 21:50
Operator : CG/JU
Sample : PB139404BS
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS404










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 4-Chloroaniline, N-isopropy... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.607	2.45 ng/ul	38443	Naphthalene-d8	11.097

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		4-Chloroaniline, N-isopropylidene	167	C9H10ClN	040938-43-0	50
2		6-Chloroanthranilonitrile	152	C7H5ClN2	006575-11-7	38
3		7-Chloro-1H-indazole	152	C7H5ClN2	037435-12-4	27
4		Benzofuran, 7-chloro-	152	C8H5ClO	024410-55-7	27
5		Biphenylene	152	C12H8	000259-79-0	27

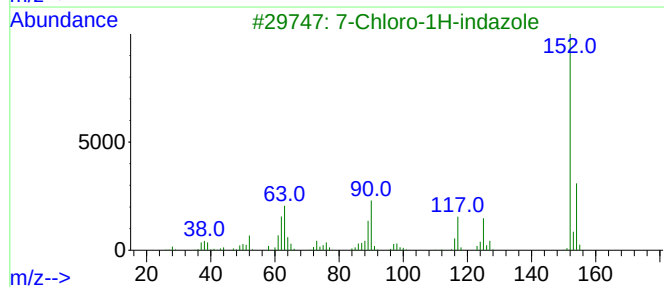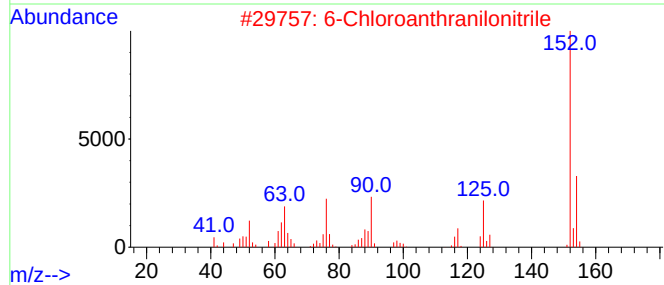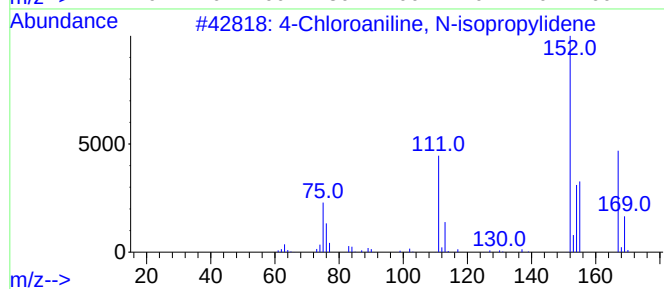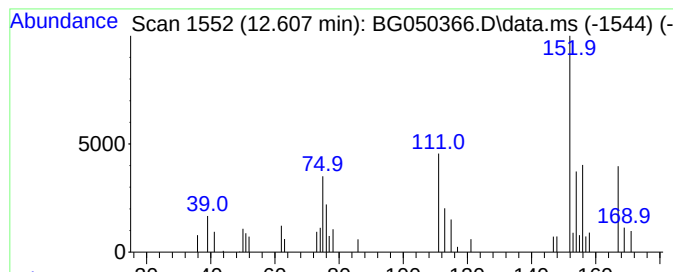

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050366.D
Acq On : 1 Oct 2021 21:50
Operator : CG/JU
Sample : PB139404BS
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SLCS404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
4-Chloroaniline...	12.607	2.4	ng/ul	38443	2	11.097	313931	20.0