

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050380.D
 Acq On : 2 Oct 2021 8:03
 Operator : CG/JU
 Sample : PB139462BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.554	9	11	14	rVB4	1925	1815	0.15%	0.013%
2	3.637	21	25	32	rVB2	14164	24328	1.97%	0.180%
3	4.060	92	97	114	rBV	164390	320997	25.96%	2.376%
4	4.283	133	135	138	rBV2	1498	1358	0.11%	0.010%
5	4.400	151	155	163	rVB5	4172	8279	0.67%	0.061%
6	4.694	203	205	208	rBV3	1259	1551	0.13%	0.011%
7	5.106	273	275	278	rBV3	1047	1273	0.10%	0.009%
8	5.364	318	319	323	rBV3	1180	1511	0.12%	0.011%
9	5.570	349	354	356	rVB2	1246	1612	0.13%	0.012%
10	6.046	432	435	436	rBV2	1261	1330	0.11%	0.010%
11	6.175	453	457	460	rVV4	887	1389	0.11%	0.010%
12	6.427	497	500	502	rBV2	1245	1513	0.12%	0.011%
13	6.480	505	509	511	rBV4	917	1488	0.12%	0.011%
14	7.397	658	665	675	rVV	215837	384488	31.09%	2.846%
15	7.585	687	697	706	rVB	159119	275639	22.29%	2.040%
16	7.791	726	732	740	rBV	205318	357302	28.89%	2.644%
17	7.967	760	762	764	rVB2	1270	1267	0.10%	0.009%
18	8.267	807	813	821	rBV	177225	314722	25.45%	2.329%
19	8.784	898	901	903	rBV2	1053	1262	0.10%	0.009%
20	8.954	923	930	941	rVB	247268	440752	35.64%	3.262%
21	9.436	1004	1012	1020	rBV	197659	361217	29.21%	2.673%
22	10.164	1129	1136	1144	rBV	161187	288992	23.37%	2.139%
23	10.699	1219	1227	1237	rBV	241334	432383	34.97%	3.200%
24	11.093	1285	1294	1302	rBV	237950	444632	35.96%	3.291%
25	11.222	1308	1316	1325	rVB	238288	445844	36.05%	3.300%
26	12.391	1510	1515	1517	rBV2	948	1278	0.10%	0.009%
27	12.655	1556	1560	1565	rBV5	3997	7433	0.60%	0.055%
28	14.277	1830	1836	1845	rVB	445718	644409	52.11%	4.769%
29	14.583	1879	1888	1895	rBV	462911	754038	60.98%	5.581%
30	14.882	1932	1939	1948	rBV	379383	605257	48.94%	4.480%
31	15.047	1959	1967	1978	rBV	223884	368371	29.79%	2.726%
32	15.869	2101	2107	2116	rVB	590866	941836	76.16%	6.971%
33	15.975	2119	2125	2132	rBV	165576	260204	21.04%	1.926%
34	16.110	2144	2148	2153	rBV4	6186	8339	0.67%	0.062%
35	16.151	2153	2155	2160	rVB2	1062	1669	0.13%	0.012%
36	16.903	2282	2283	2289	rVB2	1027	1818	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050380.D
 Acq On : 2 Oct 2021 8:03
 Operator : CG/JU
 Sample : PB139462BL
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK462

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	17.409	2366	2369	2375	rVV3	1892	3320	0.27%	0.025%
38	17.626	2400	2406	2415	rVB	471166	736408	59.55%	5.450%
39	17.726	2416	2423	2431	rVV	678900	1040579	84.15%	7.701%
40	17.979	2463	2466	2468	rBV4	1445	1907	0.15%	0.014%
41	18.443	2542	2545	2546	rBV2	1830	1453	0.12%	0.011%
42	18.460	2546	2548	2551	rVV4	1263	1361	0.11%	0.010%
43	18.537	2559	2561	2564	rBV4	1248	1351	0.11%	0.010%
44	18.666	2581	2583	2588	rVB5	1126	1420	0.11%	0.011%
45	18.707	2588	2590	2593	rBV2	1226	1589	0.13%	0.012%
46	18.784	2598	2603	2606	rBV5	1460	2393	0.19%	0.018%
47	19.095	2654	2656	2659	rBV3	1807	2466	0.20%	0.018%
48	19.130	2661	2662	2666	rBV4	1785	2002	0.16%	0.015%
49	19.189	2671	2672	2675	rBV2	1565	1512	0.12%	0.011%
50	19.218	2675	2677	2679	rBV3	1262	1252	0.10%	0.009%
51	19.259	2682	2684	2685	rVB	2975	1574	0.13%	0.012%
52	19.277	2685	2687	2689	rBV3	3197	3386	0.27%	0.025%
53	19.301	2689	2691	2692	rBV2	1751	1480	0.12%	0.011%
54	19.312	2692	2693	2697	rBV4	1462	1749	0.14%	0.013%
55	19.430	2710	2713	2715	rBV3	1852	1798	0.15%	0.013%
56	19.483	2721	2722	2724	rBV2	1792	1479	0.12%	0.011%
57	19.571	2733	2737	2744	rBV7	6646	11015	0.89%	0.082%
58	19.636	2744	2748	2753	rBV	8538	12362	1.00%	0.091%
59	19.894	2790	2792	2794	rVB2	2442	1860	0.15%	0.014%
60	20.000	2803	2810	2817	rBV	852509	1236611	100.00%	9.152%
61	20.153	2834	2836	2838	rBV3	2109	1551	0.13%	0.011%
62	20.200	2842	2844	2845	rBV2	2195	1671	0.14%	0.012%
63	20.305	2860	2862	2864	rBV2	2932	2648	0.21%	0.020%
64	20.476	2887	2891	2892	rBV4	4203	3858	0.31%	0.029%
65	21.927	3132	3138	3146	rVB	458224	791802	64.03%	5.860%
66	25.111	3670	3680	3693	rVB3	370852	1114841	90.15%	8.251%
67	25.352	3711	3721	3735	rVB2	246561	806521	65.22%	5.969%
68	28.267	4215	4217	4219	rBV2	6588	4839	0.39%	0.036%




Sum of corrected areas: 13511654

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050380.D
Acq On : 2 Oct 2021 8:03
Operator : CG/JU
Sample : PB139462BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

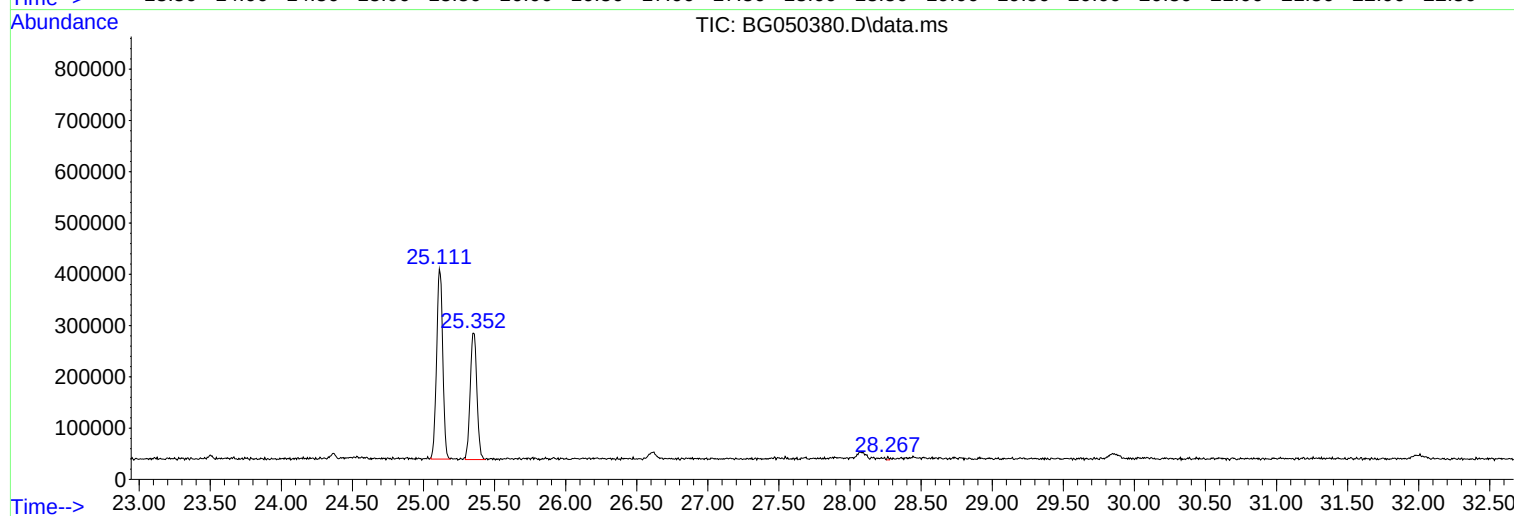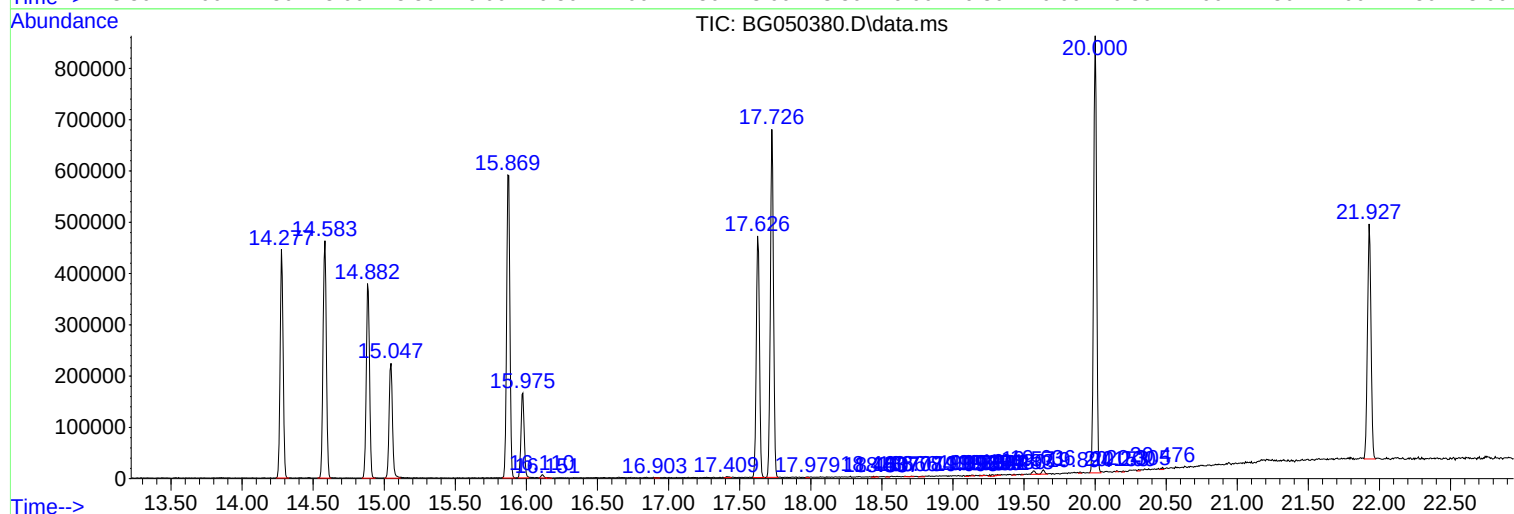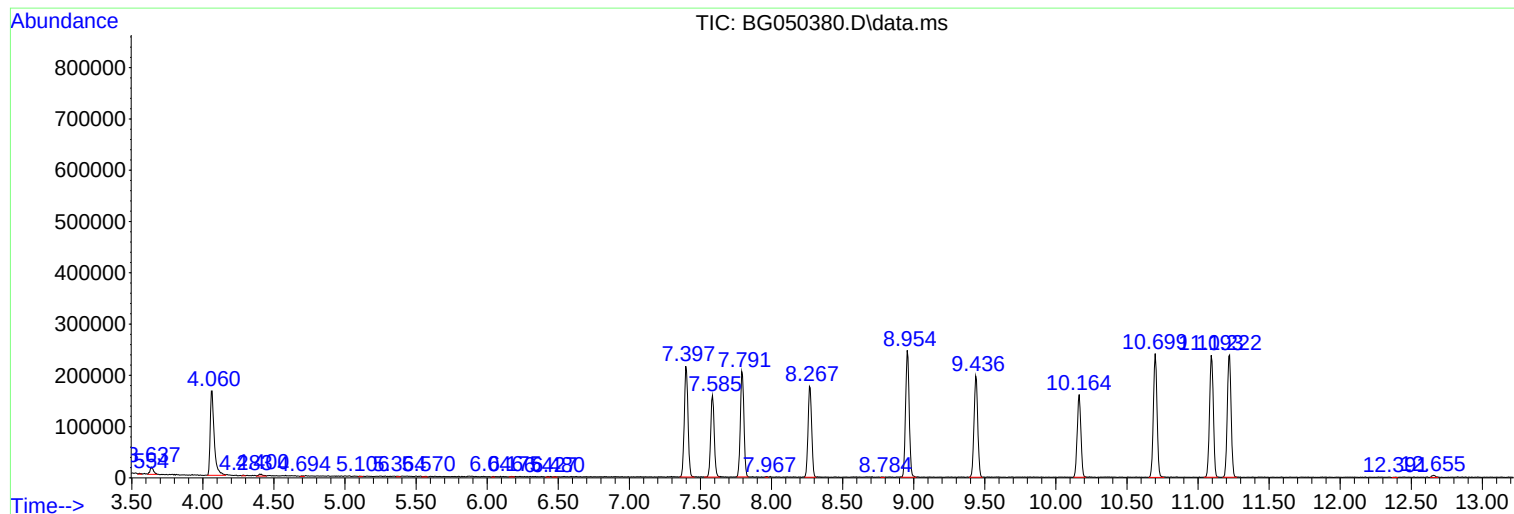

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050380.D
Acq On : 2 Oct 2021 8:03
Operator : CG/JU
Sample : PB139462BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050380.D
Acq On : 2 Oct 2021 8:03
Operator : CG/JU
Sample : PB139462BL
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK462

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
