

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050394.D
 Acq On : 2 Oct 2021 18:19
 Operator : CG/JU
 Sample : PB139405BL
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK405

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.637	22	25	31	rVB2	15466	24177	1.84%	0.170%
2	4.066	92	98	116	rBV	180313	351359	26.81%	2.467%
3	4.401	152	155	160	rBV5	3102	4454	0.34%	0.031%
4	4.748	213	214	217	rBV2	1791	2015	0.15%	0.014%
5	5.653	366	368	372	rVB4	1599	1595	0.12%	0.011%
6	7.403	656	666	676	rBV	234123	422500	32.23%	2.967%
7	7.586	690	697	706	rVV	179838	304810	23.25%	2.140%
8	7.797	726	733	740	rBV	221365	388669	29.65%	2.729%
9	8.273	806	814	822	rBV	168819	293989	22.43%	2.064%
10	8.955	923	930	941	rVB	282464	493316	37.64%	3.464%
11	9.442	1004	1013	1020	rBV	222581	407539	31.09%	2.862%
12	10.165	1129	1136	1144	rBV2	183172	332128	25.34%	2.332%
13	10.700	1220	1227	1236	rBV	274716	487254	37.17%	3.421%
14	11.093	1287	1294	1303	rBV	228392	418166	31.90%	2.936%
15	11.222	1307	1316	1326	rVB	270751	503509	38.41%	3.536%
16	12.527	1534	1538	1540	rBV3	1103	1318	0.10%	0.009%
17	12.662	1556	1561	1566	rVB4	4234	7425	0.57%	0.052%
18	13.208	1648	1654	1658	rBV2	847	1821	0.14%	0.013%
19	13.866	1762	1766	1769	rVB3	1150	1418	0.11%	0.010%
20	14.278	1829	1836	1844	rBV	478399	715698	54.60%	5.026%
21	14.583	1881	1888	1895	rBV	536320	859545	65.58%	6.036%
22	14.883	1932	1939	1950	rVB	349502	569964	43.48%	4.002%
23	15.047	1960	1967	1975	rBV	256705	408248	31.15%	2.867%
24	15.876	2101	2108	2115	rBV	685823	1059218	80.81%	7.438%
25	15.976	2118	2125	2136	rBV2	195043	301090	22.97%	2.114%
26	16.117	2141	2149	2152	rVV4	7571	11045	0.84%	0.078%
27	16.593	2228	2230	2233	rVB2	1325	1442	0.11%	0.010%
28	17.039	2302	2306	2308	rVB2	1000	1372	0.10%	0.010%
29	17.415	2365	2370	2373	rBV5	1846	3218	0.25%	0.023%
30	17.627	2399	2406	2413	rBV	437324	685593	52.31%	4.814%
31	17.727	2416	2423	2430	rBV	722792	1132079	86.37%	7.949%
32	17.873	2444	2448	2453	rBV3	1318	2076	0.16%	0.015%
33	18.473	2546	2550	2552	rVB4	1772	2528	0.19%	0.018%
34	18.502	2552	2555	2559	rBV5	1924	3685	0.28%	0.026%
35	18.702	2586	2589	2591	rBV4	1136	1356	0.10%	0.010%
36	19.037	2644	2646	2649	rBV2	2011	1613	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
 Data File : BG050394.D
 Acq On : 2 Oct 2021 18:19
 Operator : CG/JU
 Sample : PB139405BL
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK405

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	19.383	2703	2705	2707	rBV3	1298	1375	0.10%	0.010%
38	19.442	2712	2715	2717	rBV4	1841	1735	0.13%	0.012%
39	19.536	2728	2731	2732	rBV3	2130	2434	0.19%	0.017%
40	19.566	2732	2736	2742	rVB3	8201	13073	1.00%	0.092%
41	19.636	2742	2748	2755	rBV3	11482	20205	1.54%	0.142%
42	19.842	2780	2783	2784	rVV3	2668	1925	0.15%	0.014%
43	19.924	2795	2797	2798	rVB2	2408	1459	0.11%	0.010%
44	20.000	2804	2810	2817	rVB	876089	1310741	100.00%	9.204%
45	20.265	2853	2855	2857	rBV3	2355	2333	0.18%	0.016%
46	20.300	2859	2861	2864	rBV4	3754	4803	0.37%	0.034%
47	20.400	2876	2878	2879	rBV2	2775	1503	0.11%	0.011%
48	20.635	2915	2918	2920	rBV3	4048	5083	0.39%	0.036%
49	20.799	2944	2946	2948	rBV3	4885	3374	0.26%	0.024%
50	21.928	3132	3138	3145	rVB2	414030	716226	54.64%	5.029%
51	25.118	3670	3681	3693	rVB2	400741	1196049	91.25%	8.399%
52	25.353	3711	3721	3734	rVB2	236357	751525	57.34%	5.277%




Sum of corrected areas: 14241075

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050394.D
Acq On : 2 Oct 2021 18:19
Operator : CG/JU
Sample : PB139405BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

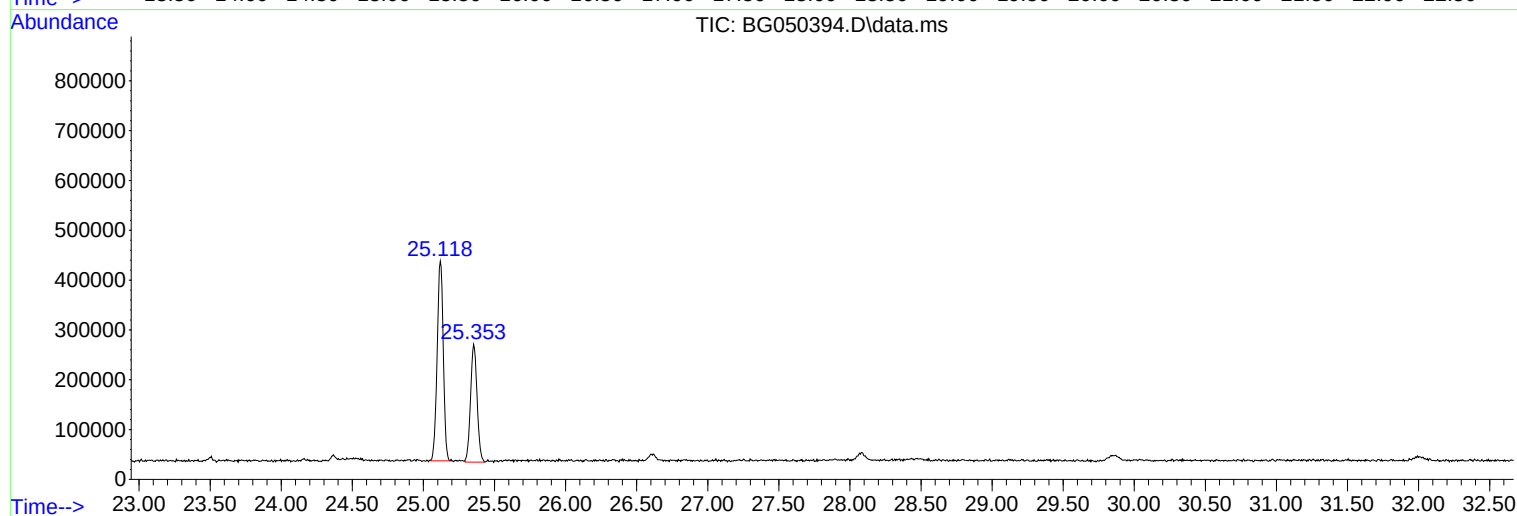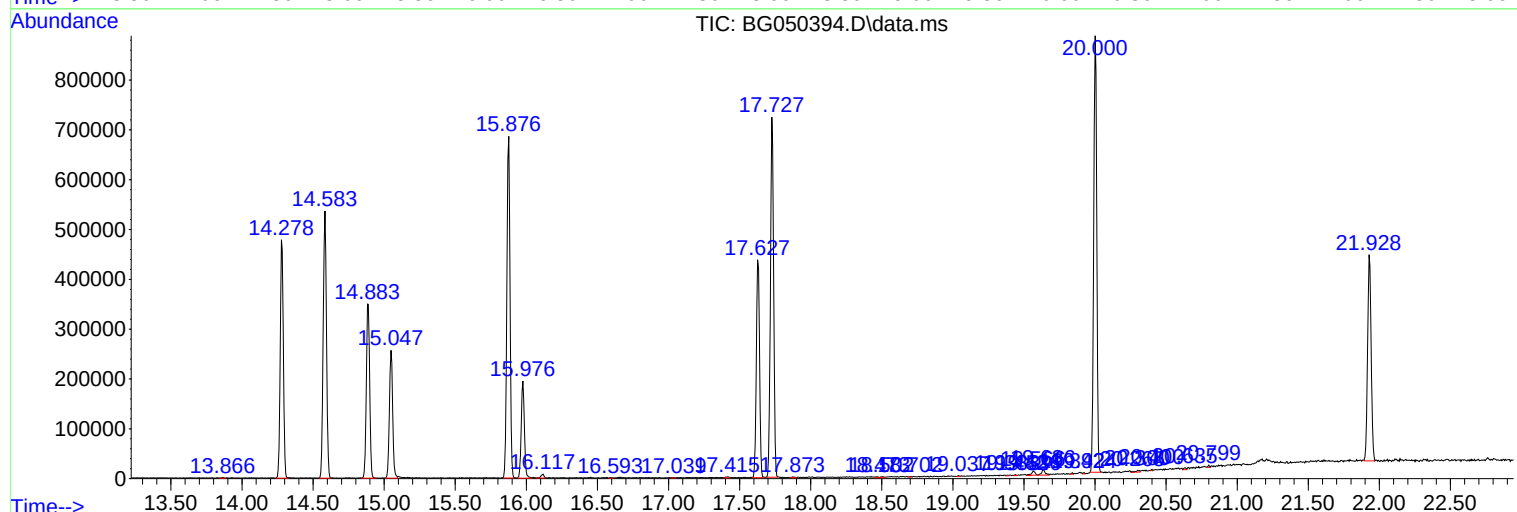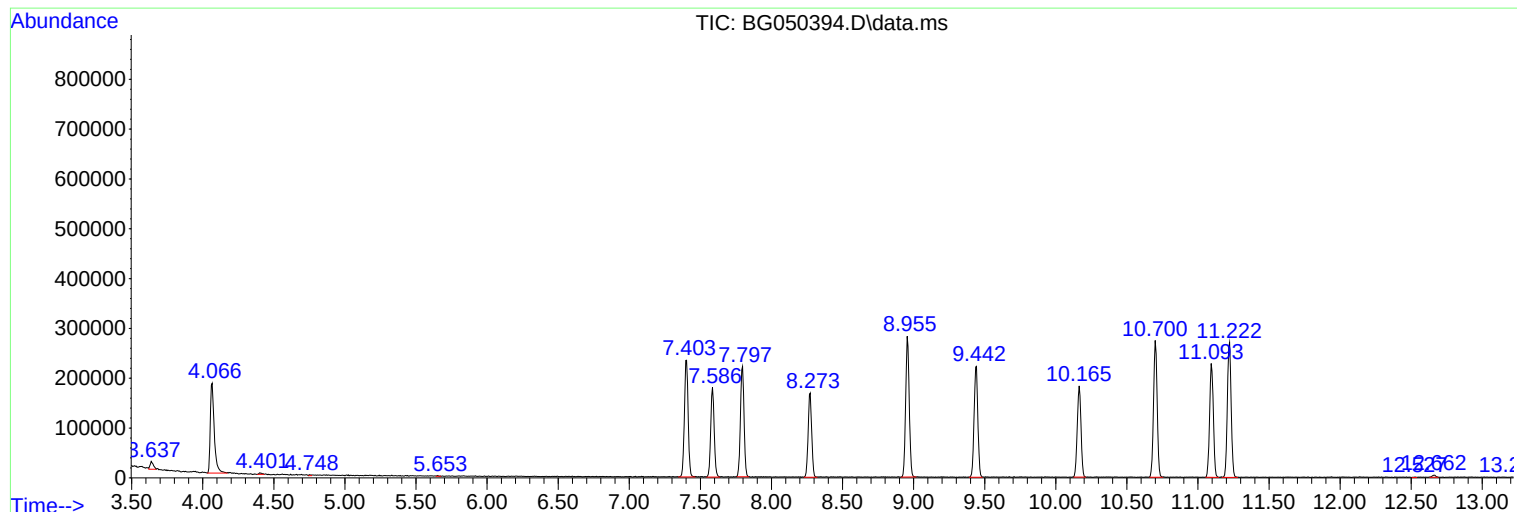

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050394.D
Acq On : 2 Oct 2021 18:19
Operator : CG/JU
Sample : PB139405BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093021\
Data File : BG050394.D
Acq On : 2 Oct 2021 18:19
Operator : CG/JU
Sample : PB139405BL
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK405

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
