
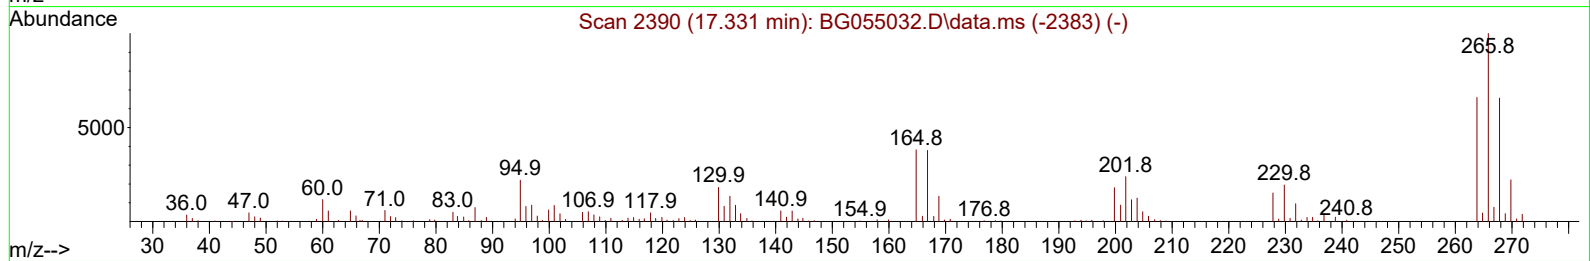
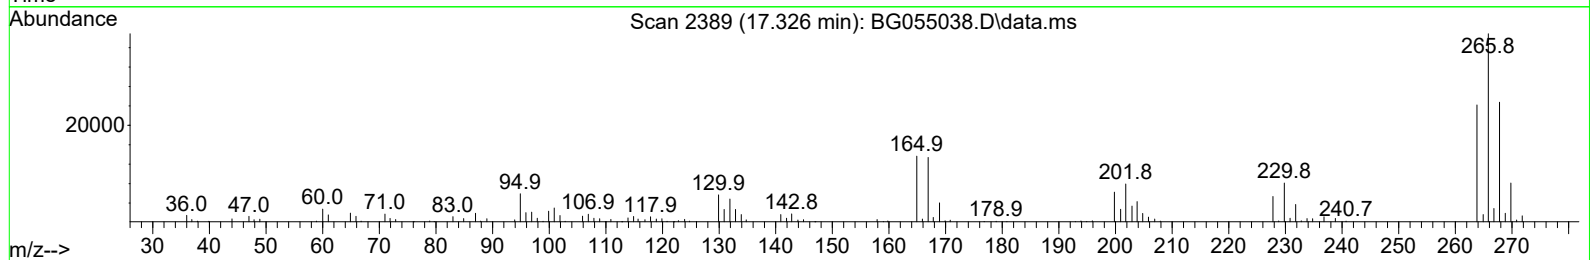


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093022\
Data File : BG055038.D
Acq On : 30 Sep 2022 11:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 02:57:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

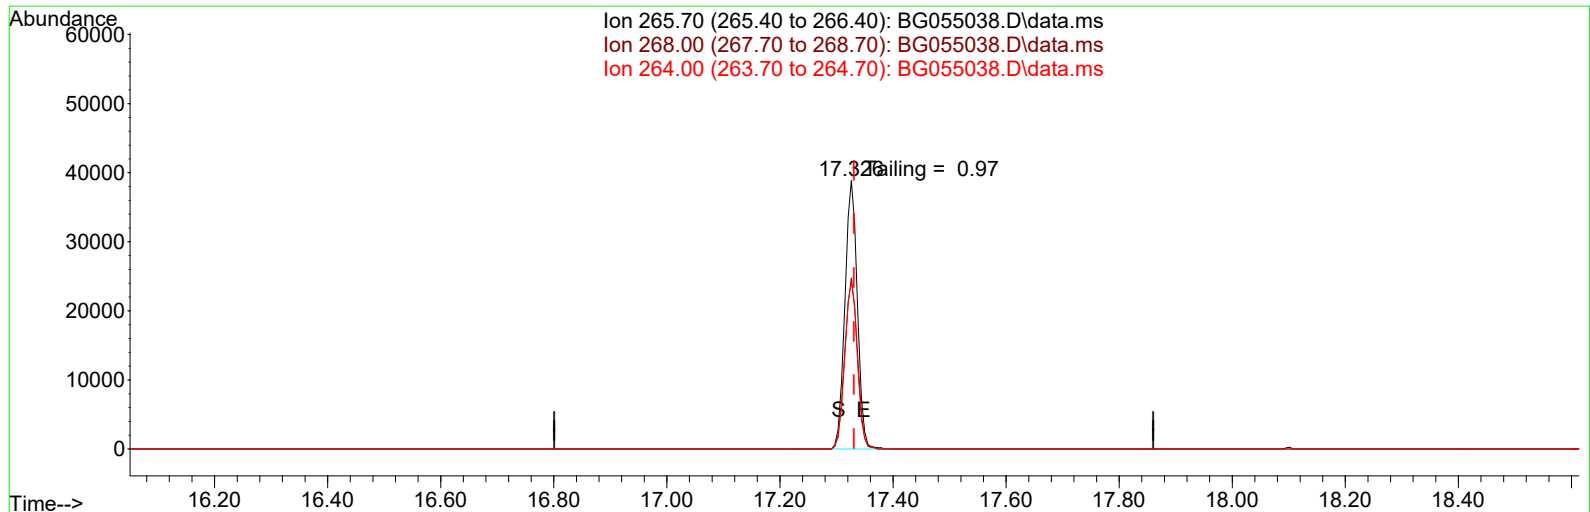

TIC: BG055038.D\data.ms

(70) Pentachlorophenol (C)




17.326min (-0.004) 22227.63 ng

response 59388

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.74
264.00	61.70	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093022\
Data File : BG055038.D
Acq On : 30 Sep 2022 11:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 01 02:57:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

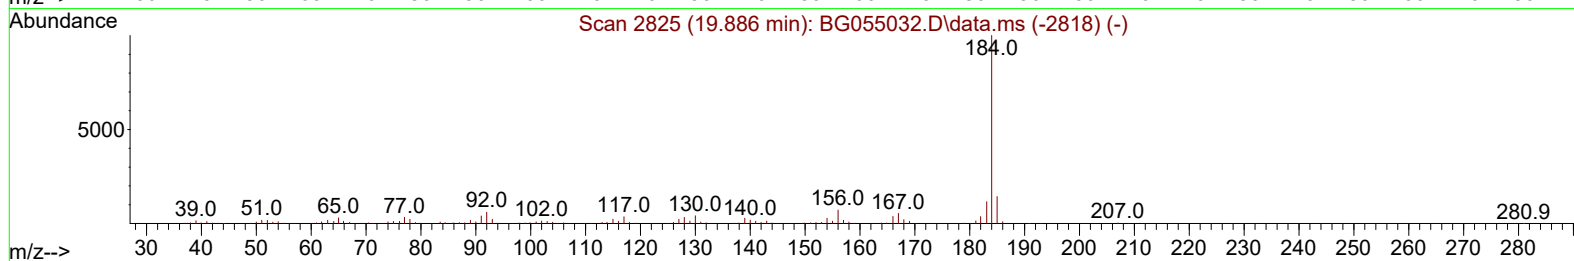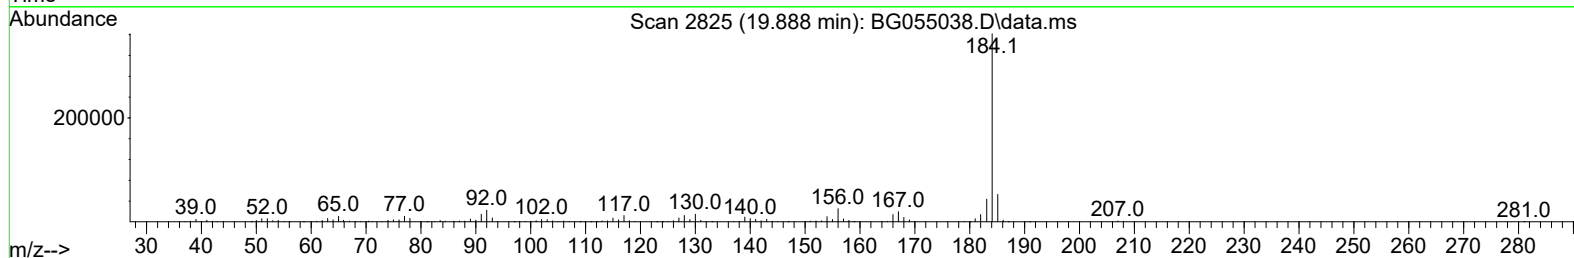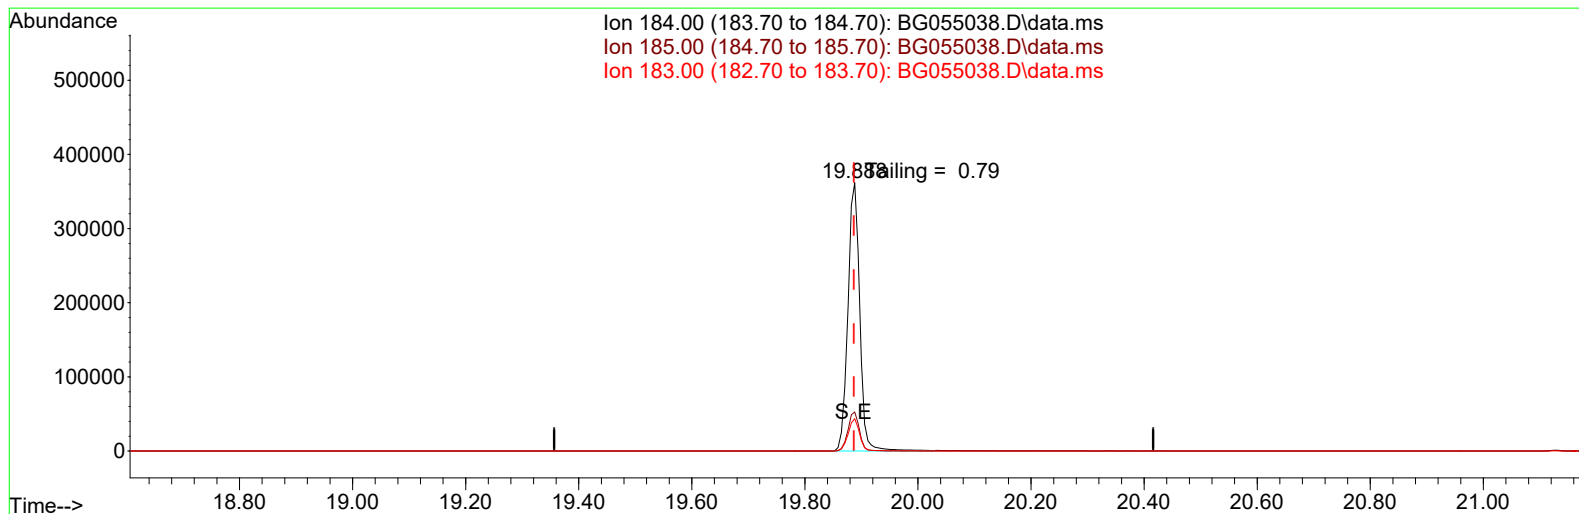

TIC: BG055038.D\data.ms

(77) Benzidine

19.888min (+ 0.002) 0.00 ng

response 525609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.56
183.00	12.30	12.07
0.00	0.00	0.00