
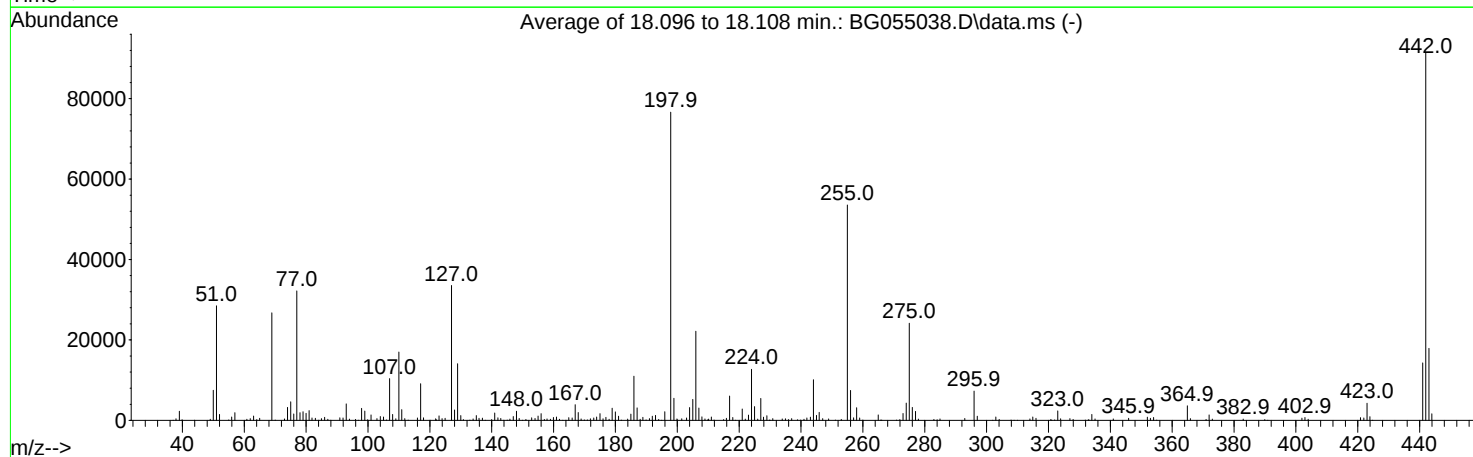


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093022\
 Data File : BG055038.D
 Acq On : 30 Sep 2022 11:49
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 15:43:39 2022

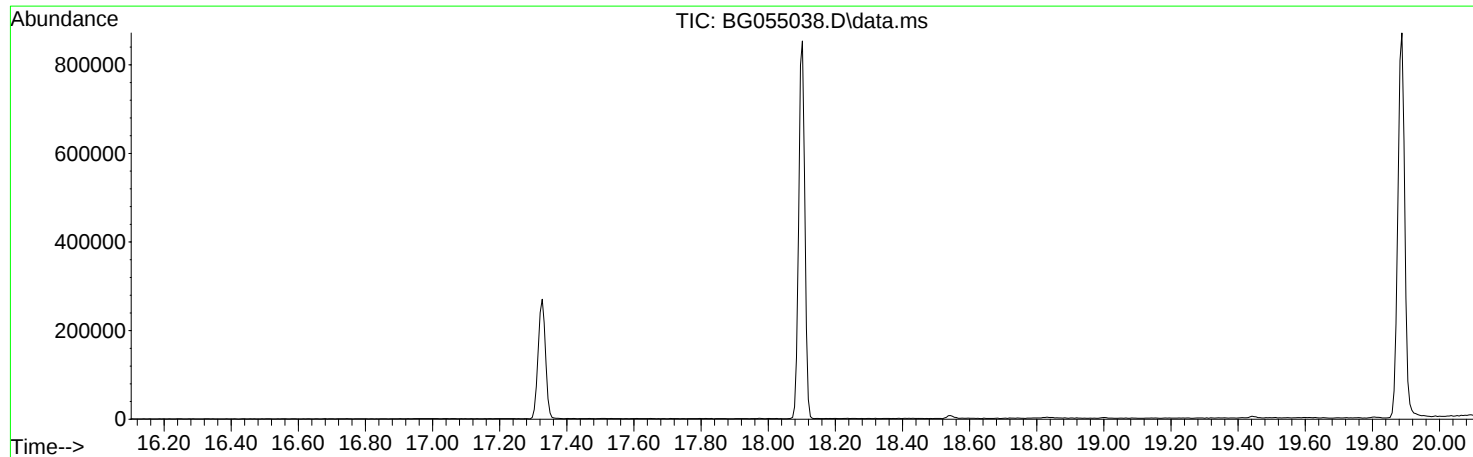




AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	28480	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.9	26752	PASS
70	69	0.00	2	0.3	81	PASS
127	198	10	80	43.8	33563	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76645	PASS
199	198	5	9	7.1	5479	PASS
275	198	10	60	31.5	24141	PASS
365	198	1	100	4.7	3623	PASS
441	198	0.01	100	18.6	14273	PASS
442	442	50	100	100.0	91480	PASS
443	442	15	24	19.6	17919	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093022\
Data File : BG055038.D
Acq On : 30 Sep 2022 11:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 01 02:57:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

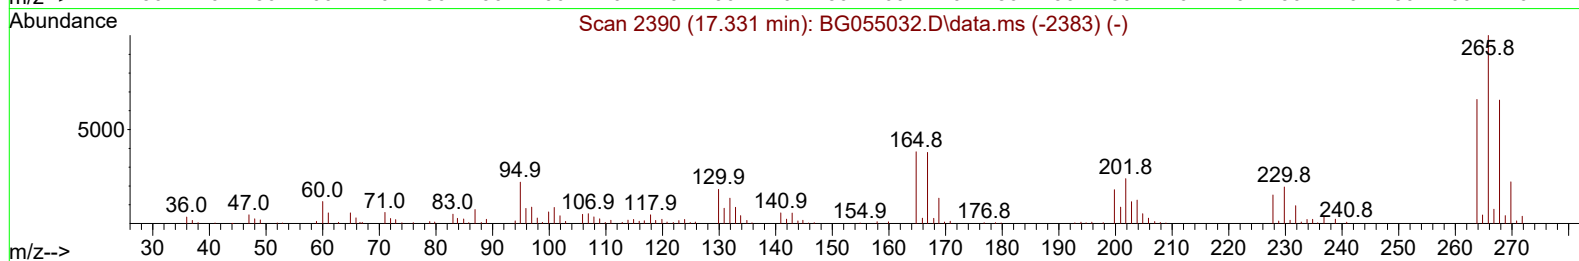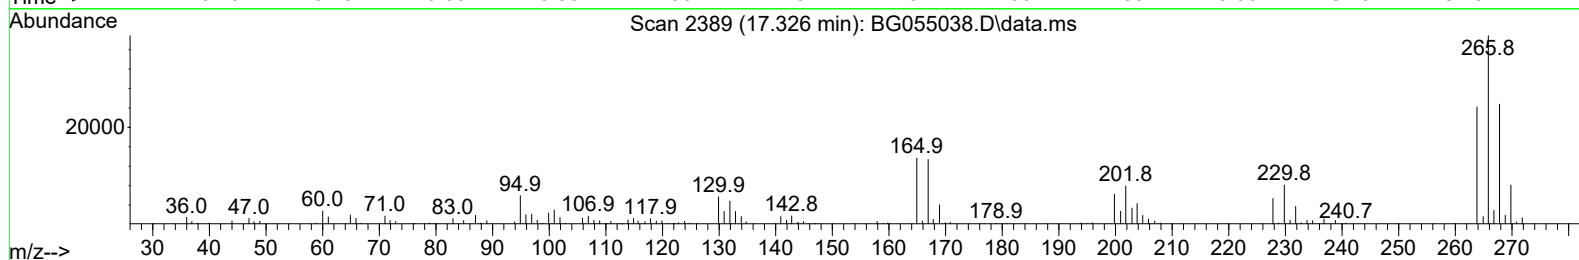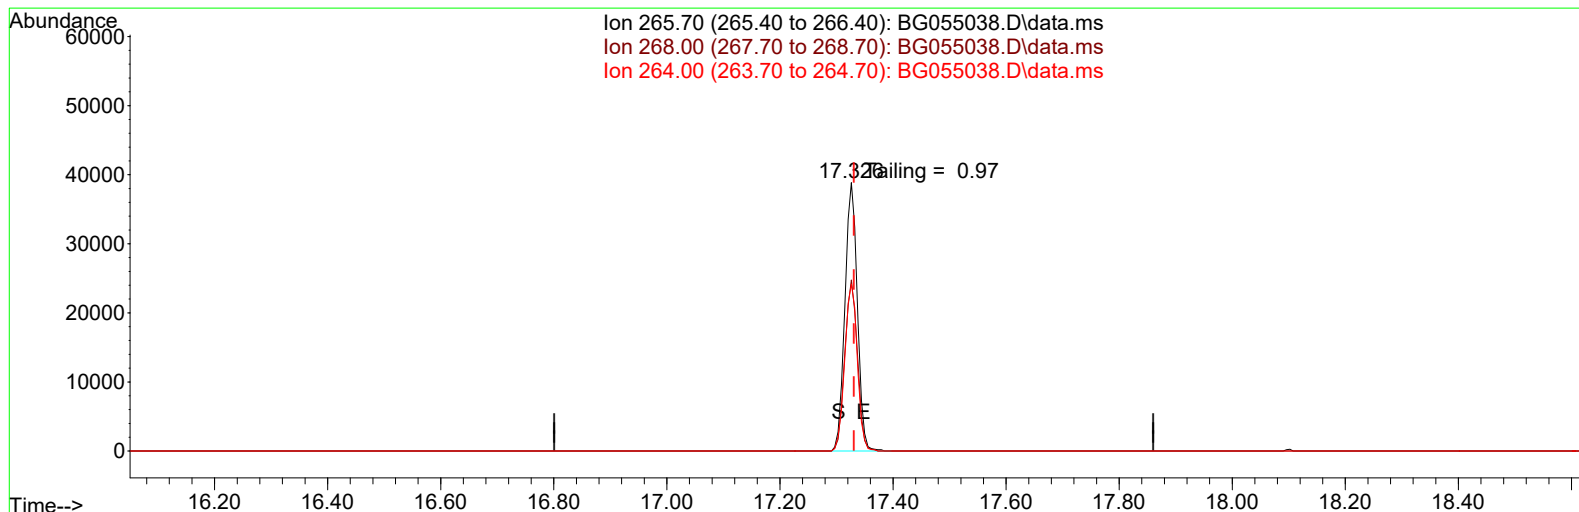

TIC: BG055038.D\data.ms

(70) Pentachlorophenol (C)

17.326min (-0.004) 22227.63 ng




response 59388

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.00	63.74
264.00	61.70	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG093022\
Data File : BG055038.D
Acq On : 30 Sep 2022 11:49
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 01 02:57:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG092822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 15:43:39 2022
Response via : Initial Calibration

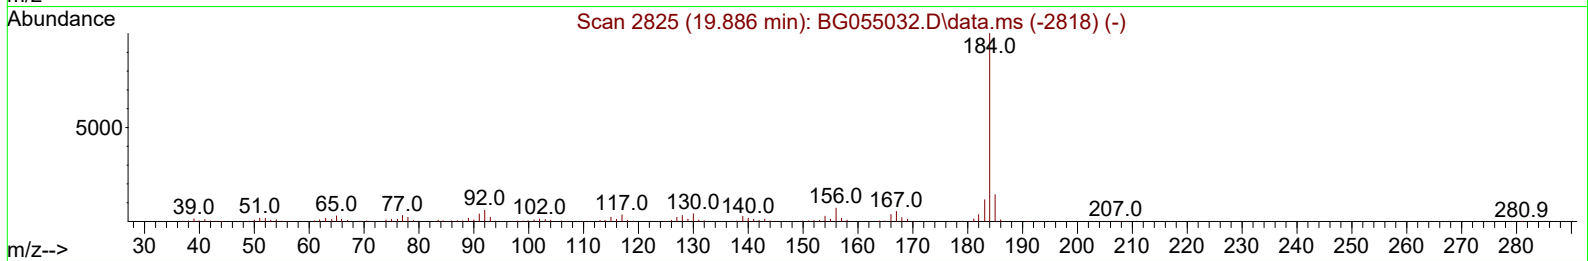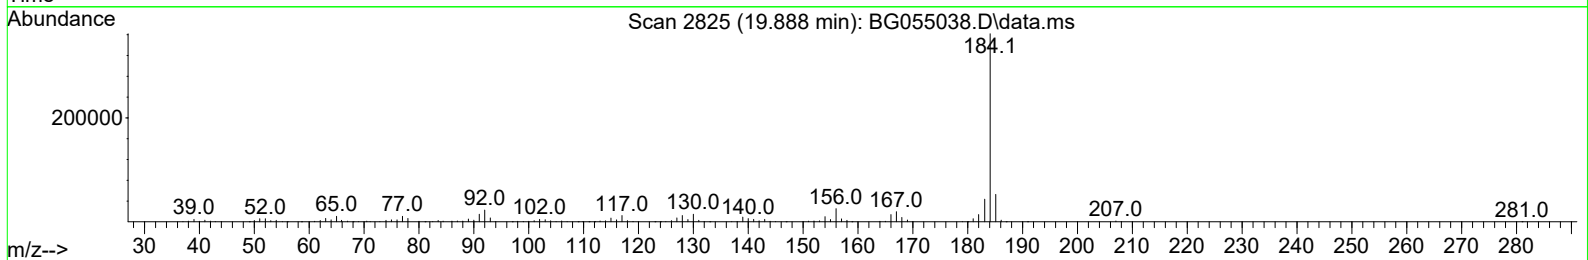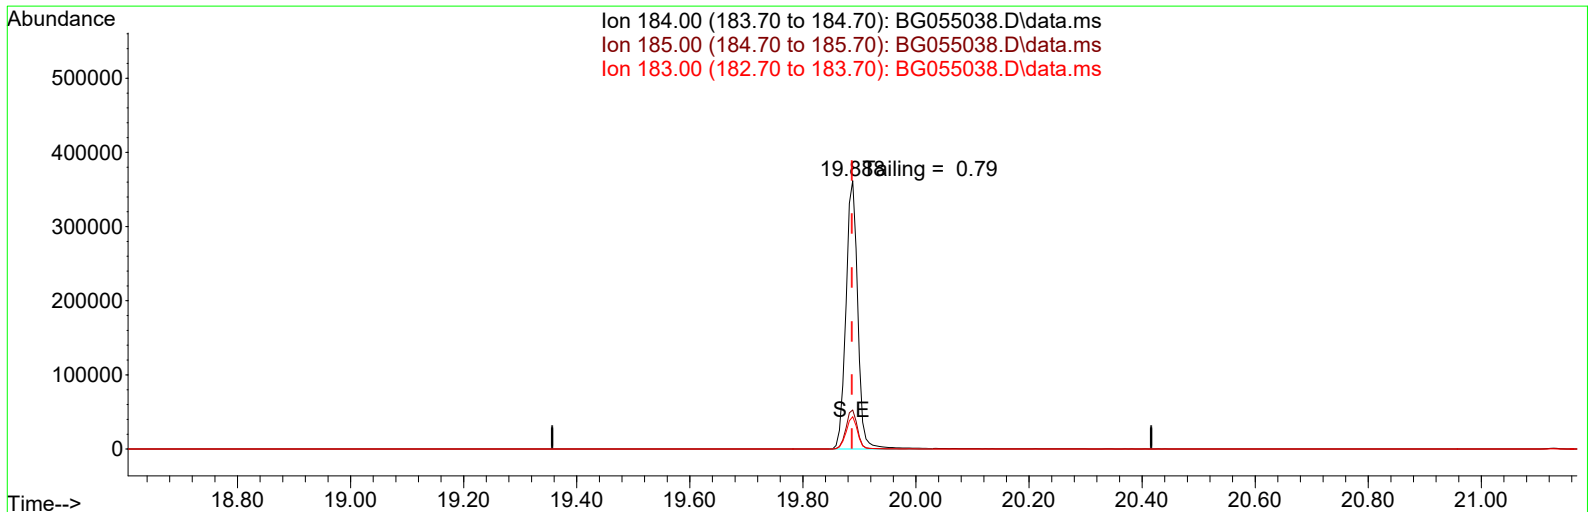

TIC: BG055038.D\data.ms

(77) Benzidine

19.888min (+ 0.002) 0.00 ng

response 525609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.56
183.00	12.30	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/30/2022	BNA_G	BG055038.D
Compound Name	Response	Retention Time
DDT	185882	21.128
DDD	1508	20.728
DDE	0	19.09
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1508	187390	0.80

Instrument :
BNA_G
ClientSampleId :
DFTPP