

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100115\
 Data File : BG018976.D
 Acq On : 30 Sep 2015 17:16
 Operator : UM/NP
 Sample : G3803-04RX
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E43J4

Quant Time: Oct 01 04:22:37 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 01 04:12:22 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	50772	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	224222	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.62	164	169361	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.35	188	503522	20.00	ng/ul	0.00
78) Chrysene-d12	21.61	240	565064	20.00	ng/ul	0.00
86) Perylene-d12	24.79	264	569862	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	1799	1.70	ng/uL	0.00
5) Phenol-d5	7.16	99	39597	9.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	57706	23.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	76748	24.31	ng/ul	0.00
13) 4-Methylphenol-d8	8.69	113	62934	18.60	ng/ul	0.00
19) Nitrobenzene-d5	9.14	128	44750	26.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	49651	29.07	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.41	165	93044	25.87	ng/ul	0.00
29) 4-Chloroaniline-d4	10.93	131	6222	1.49	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	366941	26.92	ng/ul	0.00
47) Acenaphthylene-d8	14.30	160	428378	26.52	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	22953	8.77	ng/ul	0.00
58) Fluorene-d10	15.60	176	336893	28.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	59270	24.87	ng/ul	0.00
71) Anthracene-d10	17.45	188	570752	25.75	ng/ul	0.00
79) Pyrene-d10	19.74	212	706377	27.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.57	264	742377	26.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.06	163	33198	2.51	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100115\
Data File : BG018976.D
Acq On : 30 Sep 2015 17:16
Operator : UM/NP
Sample : G3803-04RX
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E43J4

Quant Time: Oct 01 04:22:37 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 01 04:12:22 2015
Response via : Initial Calibration

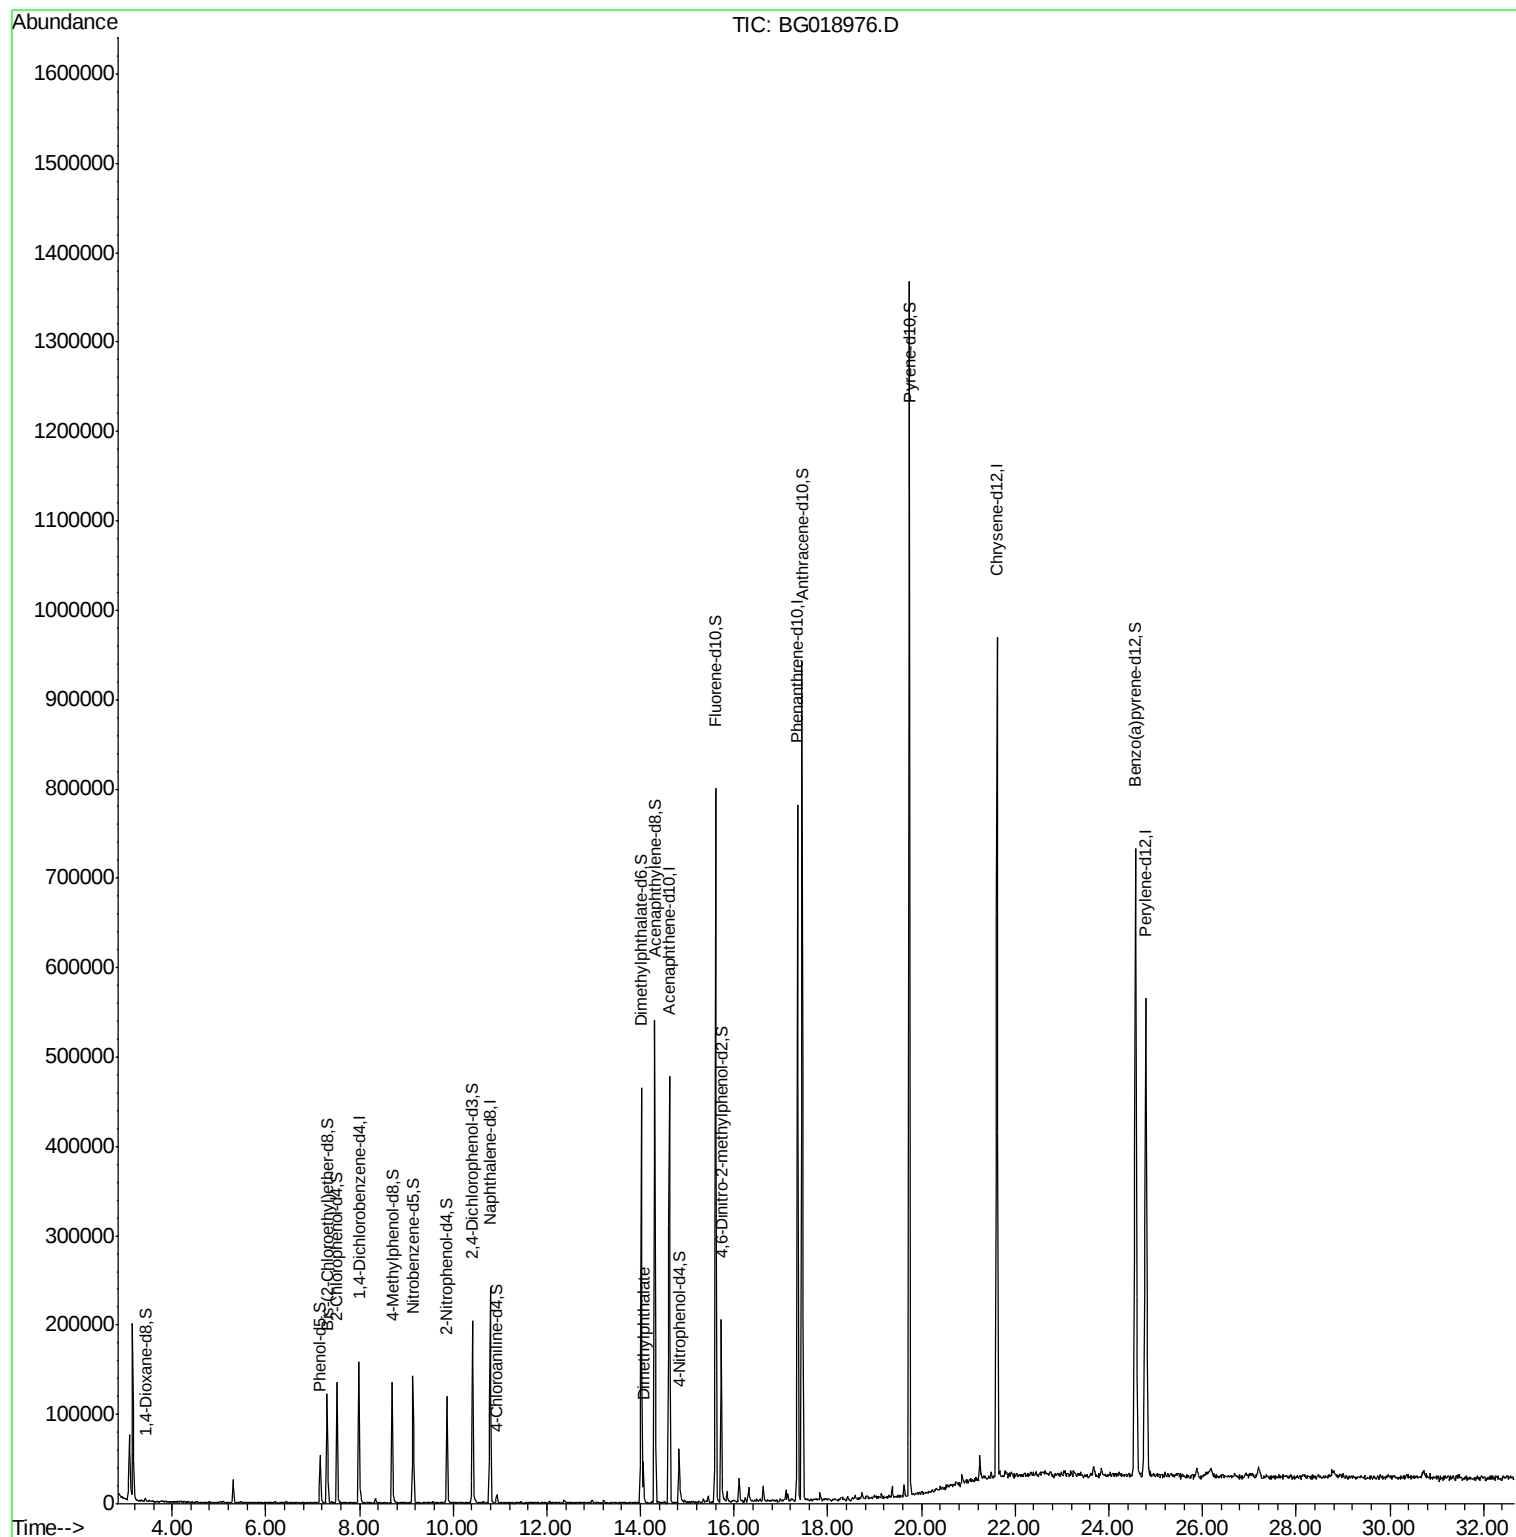

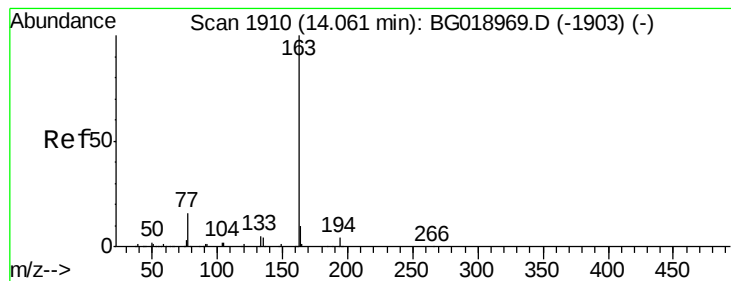

#45

Dimethylphthalate

Concen: 2.51 ng/ul

RT: 14.06 min Scan# 1909

Delta R.T. -0.00 min

Lab File: BG018976.D

Acq: 30 Sep 2015 17:16

Instrument :

BNA_G

ClientSampleId :

E43J4

Tgt Ion:163 Resp: 33198

Ion Ratio Lower Upper

163 100

194 3.0 2.9 4.3

164 11.4 7.7 11.5

