

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100115\
 Data File : BG018980.D
 Acq On : 30 Sep 2015 19:49
 Operator : UM/NP
 Sample : G3800-18
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C03H0

Quant Time: Oct 01 04:23:49 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 01 04:12:22 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.99	152	62433	20.00	ng/ul	0.00
18) Naphthalene-d8	10.79	136	271050	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.61	164	201854	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.36	188	568092	20.00	ng/ul	0.00
78) Chrysene-d12	21.61	240	589623	20.00	ng/ul	0.00
86) Perylene-d12	24.79	264	585551	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.42	96	810	0.62	ng/uL	0.00
5) Phenol-d5	7.16	99	20770	4.05	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.31	67	40627	13.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	53927	13.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.70	113	38267	9.20	ng/ul	0.00
19) Nitrobenzene-d5	9.15	128	33536	16.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	36120	17.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.41	165	70365	16.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.92	131	75634	14.95	ng/ul	0.00
44) Dimethylphthalate-d6	14.02	166	258420	15.91	ng/ul	0.00
47) Acenaphthylene-d8	14.31	160	297483	15.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	9088	2.92	ng/ul	0.00
58) Fluorene-d10	15.60	176	237394	16.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	28996	10.78	ng/ul	0.00
71) Anthracene-d10	17.45	188	397751	15.90	ng/ul	0.00
79) Pyrene-d10	19.74	212	446302	16.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.57	264	446138	15.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.06	163	18447	1.17	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100115\
Data File : BG018980.D
Acq On : 30 Sep 2015 19:49
Operator : UM/NP
Sample : G3800-18
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C03H0

Quant Time: Oct 01 04:23:49 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 01 04:12:22 2015
Response via : Initial Calibration

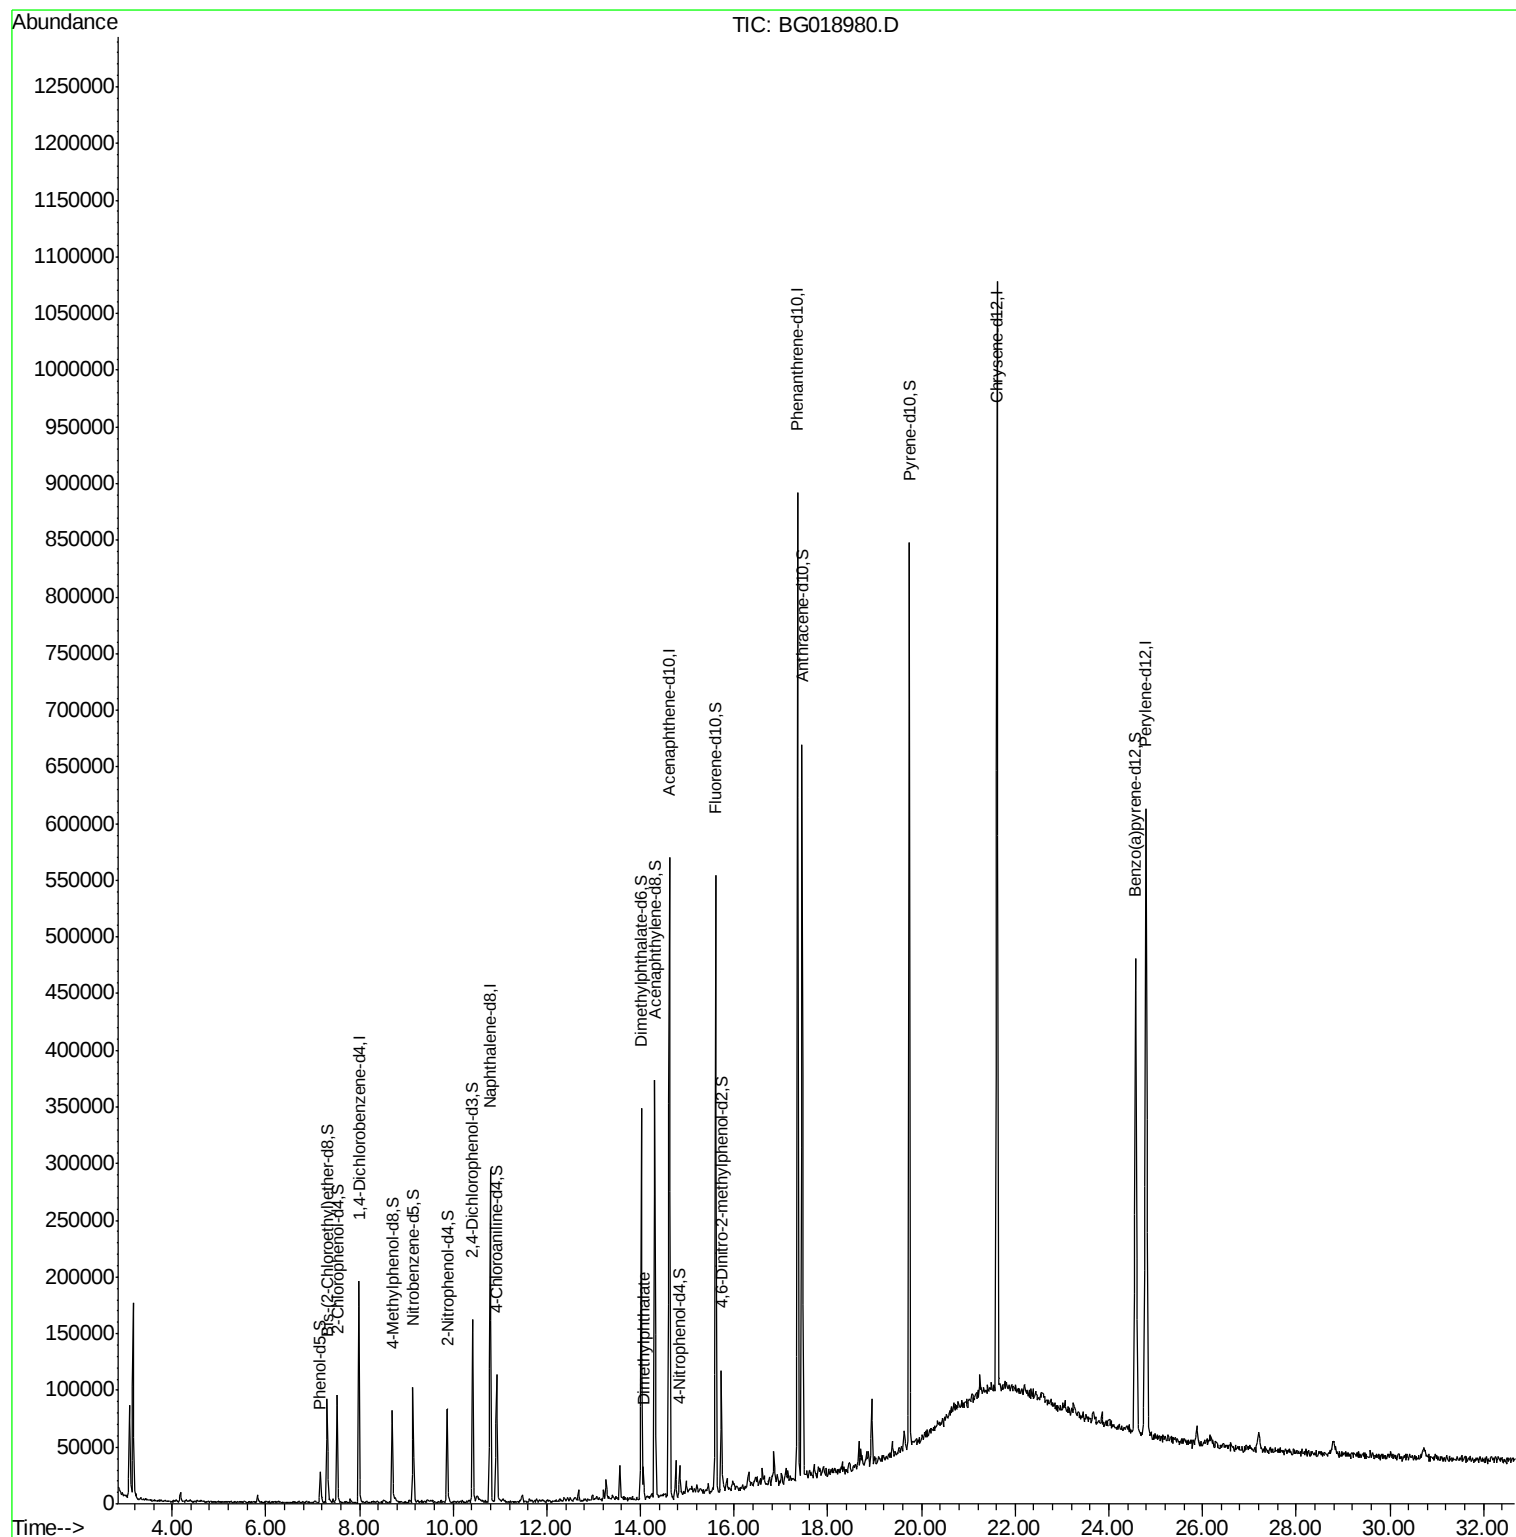

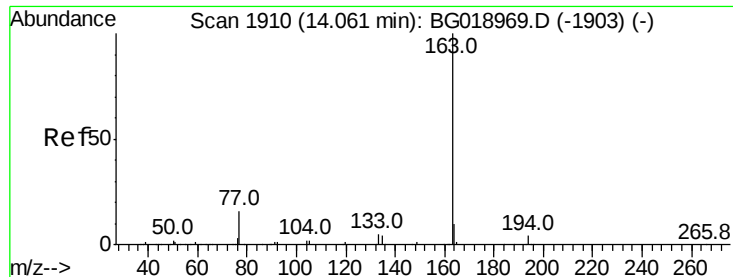

#45

Dimethylphthalate

Concen: 1.17 ng/ul

RT: 14.06 min Scan# 1910

Delta R.T. 0.00 min

Lab File: BG018980.D

Acq: 30 Sep 2015 19:49

Instrument :

BNA_G

ClientSampleId :

C03H0


Tot Ion:163 Resp: 18447

Ion Ratio Lower Upper

163 100

194 6.0 2.9 4.3#

164 11.9 7.7 11.5#

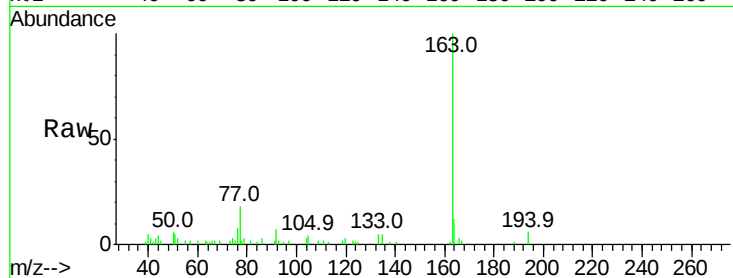

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

