

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100215\
 Data File : BG018986.D
 Acq On : 1 Oct 2015 19:31
 Operator : UM/NP
 Sample : G3831-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AP6

Quant Time: Oct 02 04:37:56 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 04:39:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	53185	20.00	ng/ul	0.00
18) Naphthalene-d8	10.78	136	211081	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	144892	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.35	188	372340	20.00	ng/ul	0.00
78) Chrysene-d12	21.60	240	471452	20.00	ng/ul	0.00
86) Perylene-d12	24.77	264	463298	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	1088	0.98	ng/uL	0.00
5) Phenol-d5	7.18	99	4733	1.08	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.30	67	60978	24.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.53	132	60808	18.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	15563	4.39	ng/ul	0.04
19) Nitrobenzene-d5	9.15	128	43122	26.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.87	143	47367	29.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.44	165	25920	7.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	1606	0.41	ng/ul	0.05
44) Dimethylphthalate-d6	14.00	166	346083	29.68	ng/ul	0.00
47) Acenaphthylene-d8	14.30	160	423870	30.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.94	143	2416	1.08	ng/ul	0.05
58) Fluorene-d10	15.60	176	314014	30.80	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	34372	19.50	ng/ul	0.00
71) Anthracene-d10	17.45	188	514213	31.37	ng/ul	0.00
79) Pyrene-d10	19.73	212	641286	29.57	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	714183	31.67	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
2) 1,4-Dioxane	3.44	88	5002	4.18	ng/uL#	78
11) 2-Methylphenol	8.32	108	7466	2.15	ng/ul	99
30) 4-Chloroaniline	10.94	127	5145	1.26	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100215\
Data File : BG018986.D
Acq On : 1 Oct 2015 19:31
Operator : UM/NP
Sample : G3831-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AP6

Quant Time: Oct 02 04:37:56 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 04:39:32 2015
Response via : Initial Calibration

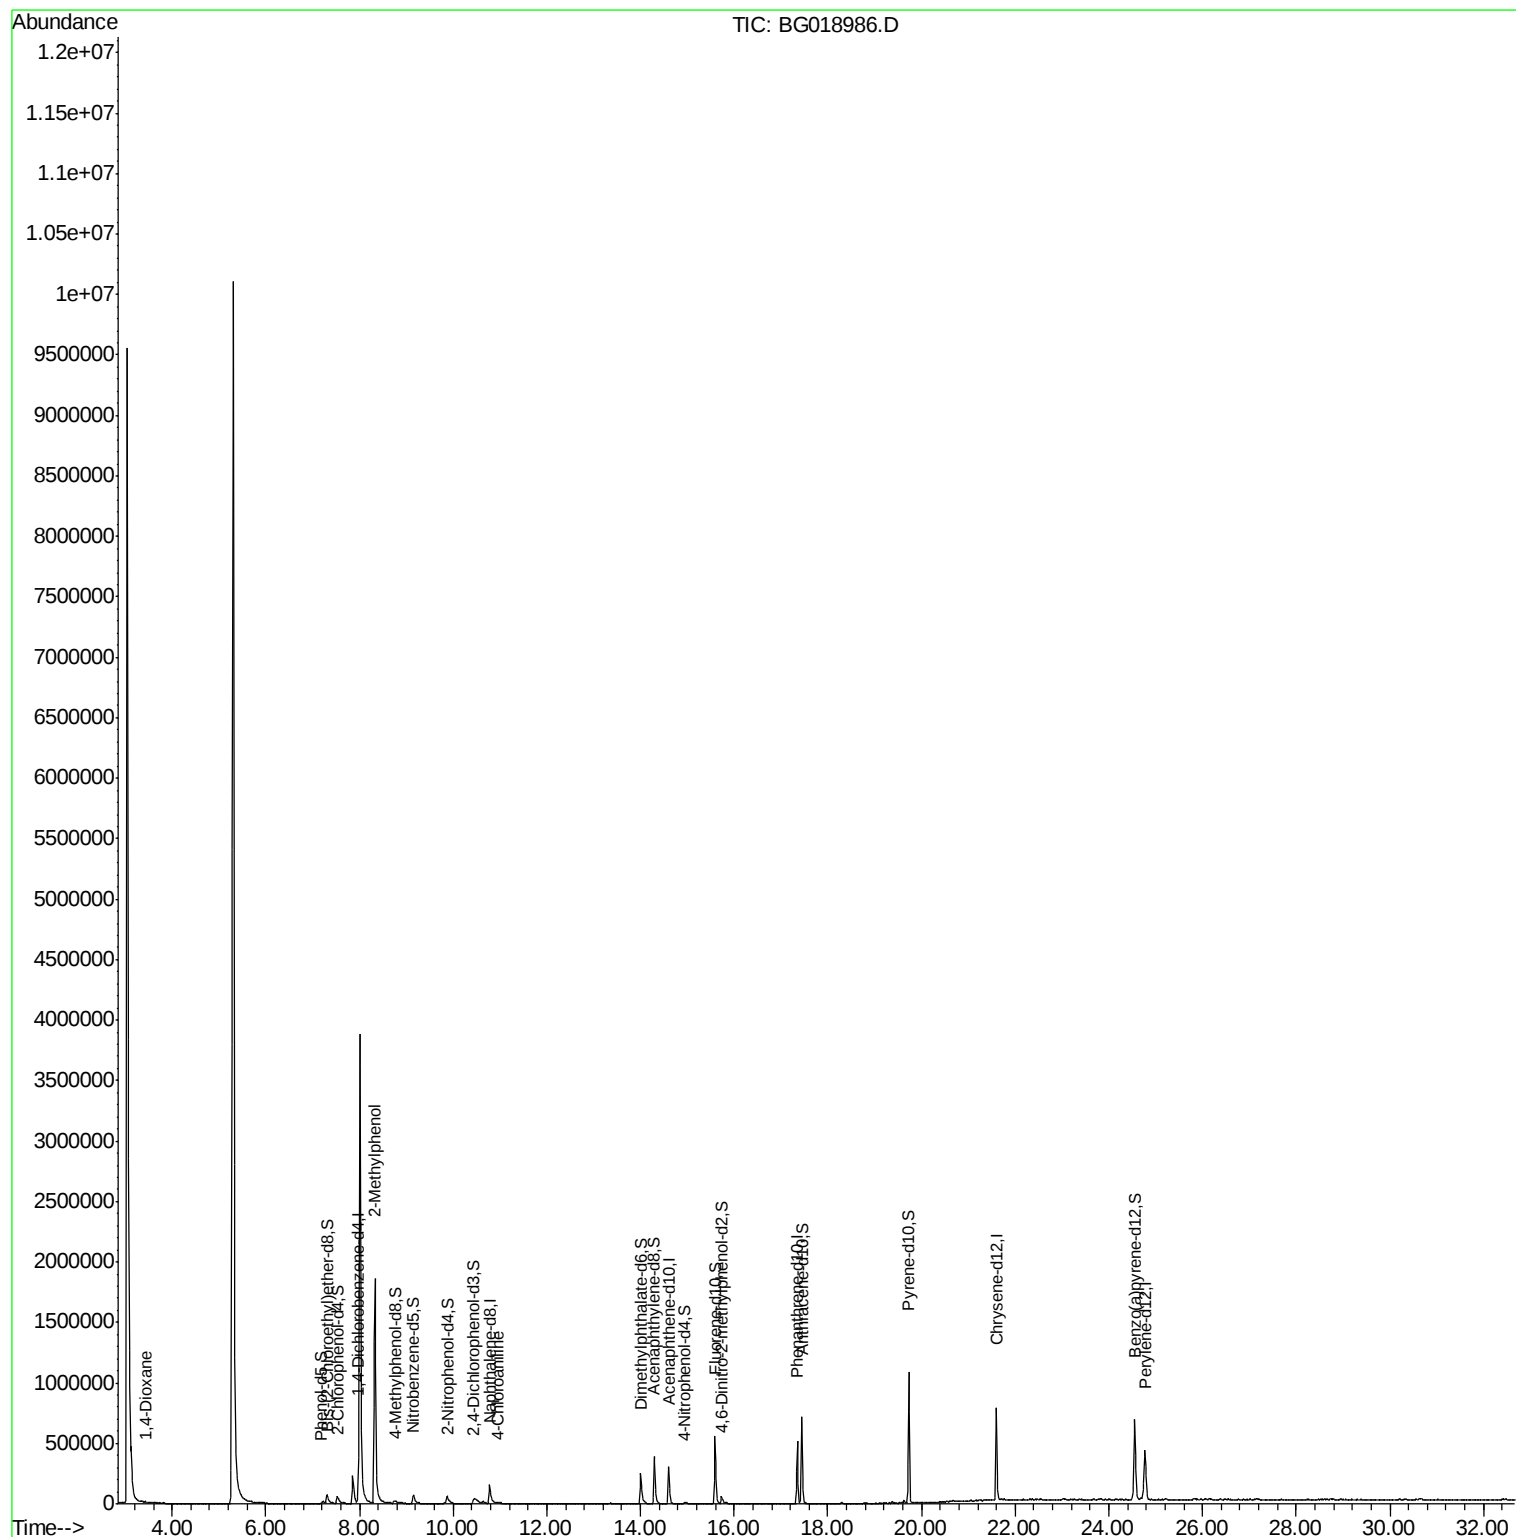

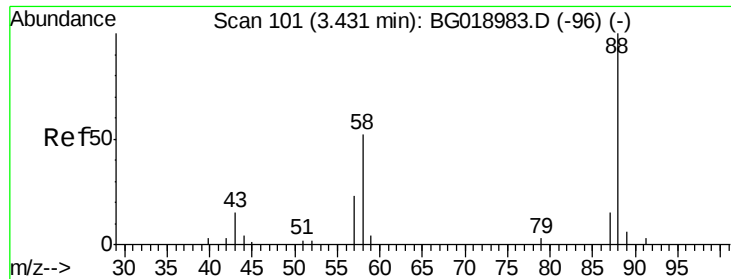

#2

1,4-Dioxane

Concen: 4.18 ng/uL

RT: 3.44 min Scan# 102

Delta R.T. 0.01 min

Lab File: BG018986.D

Acq: 1 Oct 2015 19:31

Instrument :

BNA_G

ClientSampleId :

C0AP6


Tot Ion: 88 Resp: 5002

Ion Ratio Lower Upper




88 100

43 33.1 33.0 49.4

58 66.3 73.4 110.0#

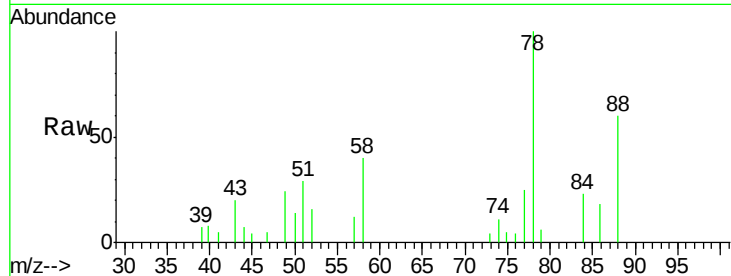

Abundance Ion 88.00 (87.70 to 88.70): BGC
Ion 43.00 (42.70 to 43.70): BGC
Ion 58.00 (57.70 to 58.70): BGC

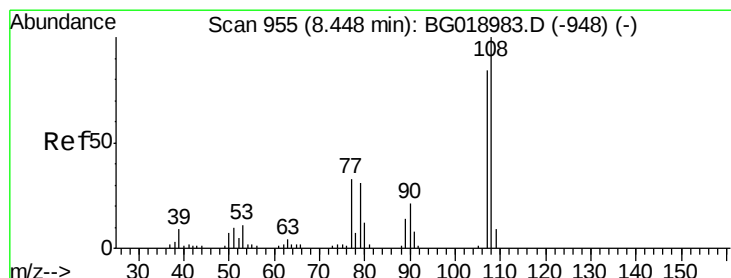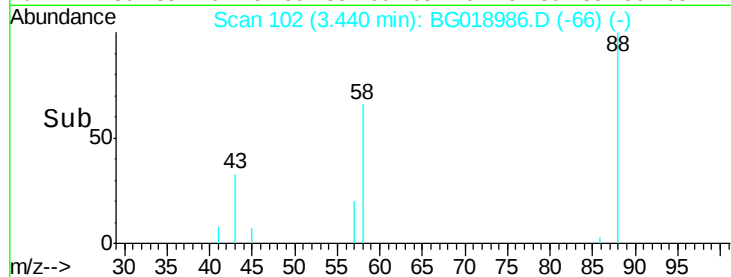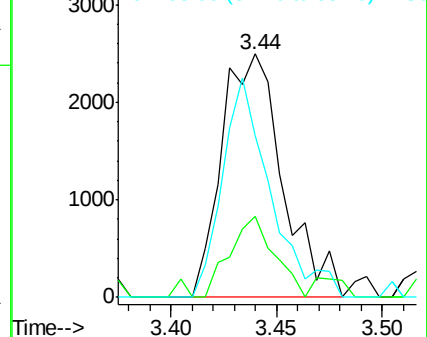

#11

2-Methylphenol

Concen: 2.15 ng/uL

RT: 8.32 min Scan# 933

Delta R.T. -0.13 min

Lab File: BG018986.D


Acq: 1 Oct 2015 19:31

Tgt Ion: 108 Resp: 7466



Ion Ratio Lower Upper


108 100

107 89.2 72.1 108.1

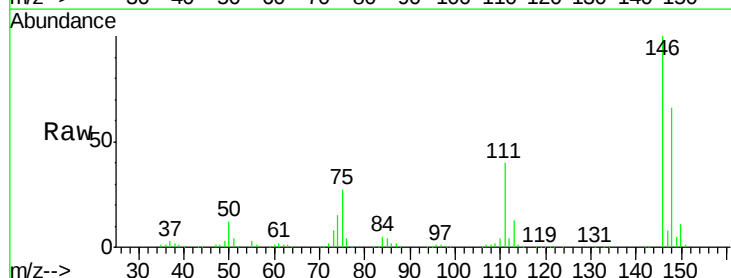

Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E

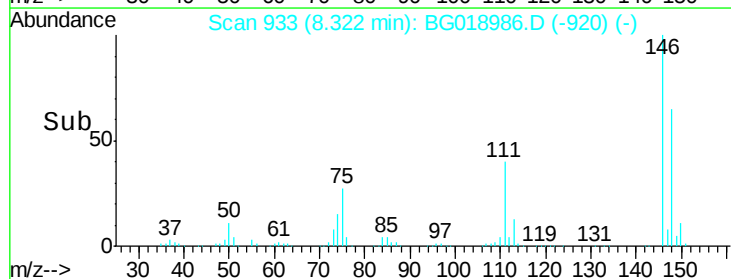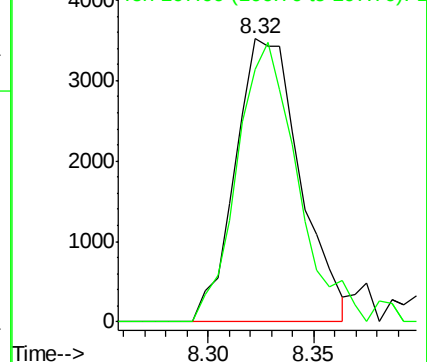

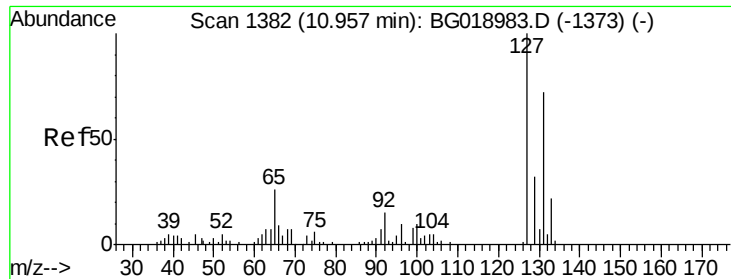

#30
 4-Chloroaniline
 Concen: 1.26 ng/ul
 RT: 10.94 min Scan# 1378
 Delta R.T. -0.02 min
 Lab File: BG018986.D
 Acq: 1 Oct 2015 19:31

Instrument :
 BNA_G
 ClientSampleId :
 C0AP6

Tot Ion:127 Resp: 5145
 Ion Ratio Lower Upper
 127 100
 129 29.6 26.7 40.1

