

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100215\
 Data File : BG018990.D
 Acq On : 1 Oct 2015 22:03
 Operator : UM/NP
 Sample : G3865-18
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5MZ4

Quant Time: Oct 02 04:39:00 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 04:39:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.98	152	49952	20.00	ng/ul	0.00
18) Naphthalene-d8	10.78	136	240649	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	157937	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.35	188	411409	20.00	ng/ul	0.00
78) Chrysene-d12	21.60	240	493325	20.00	ng/ul	0.00
86) Perylene-d12	24.77	264	496882	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	2167	2.09	ng/uL	0.00
5) Phenol-d5	7.22	99	10819	2.64	ng/ul	0.03
7) Bis-(2-Chloroethyl)ether-d	7.32	67	18797	7.91	ng/ul	0.01
9) 2-Chlorophenol-d4	7.53	132	29330	9.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	3380	1.02	ng/ul	0.02
19) Nitrobenzene-d5	9.16	128	18710	10.26	ng/ul	0.02
22) 2-Nitrophenol-d4	9.88	143	10999	6.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	9224	2.39	ng/ul	0.03
29) 4-Chloroaniline-d4	10.97	131	14755	3.29	ng/ul	0.03
44) Dimethylphthalate-d6	14.16	166	681	0.05	ng/ul	0.16
47) Acenaphthylene-d8	14.30	160	187437	12.44	ng/ul	0.00
52) 4-Nitrophenol-d4	14.93	143	4037	1.65	ng/ul	0.04
58) Fluorene-d10	15.60	176	145835	13.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.74	200	6869	3.53	ng/ul	0.01
71) Anthracene-d10	17.45	188	234576	12.95	ng/ul	0.00
79) Pyrene-d10	19.73	212	277358	12.22	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	292545	12.10	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.06	163	81467	6.61	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100215\
Data File : BG018990.D
Acq On : 1 Oct 2015 22:03
Operator : UM/NP
Sample : G3865-18
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5MZ4

Quant Time: Oct 02 04:39:00 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 04:39:32 2015
Response via : Initial Calibration

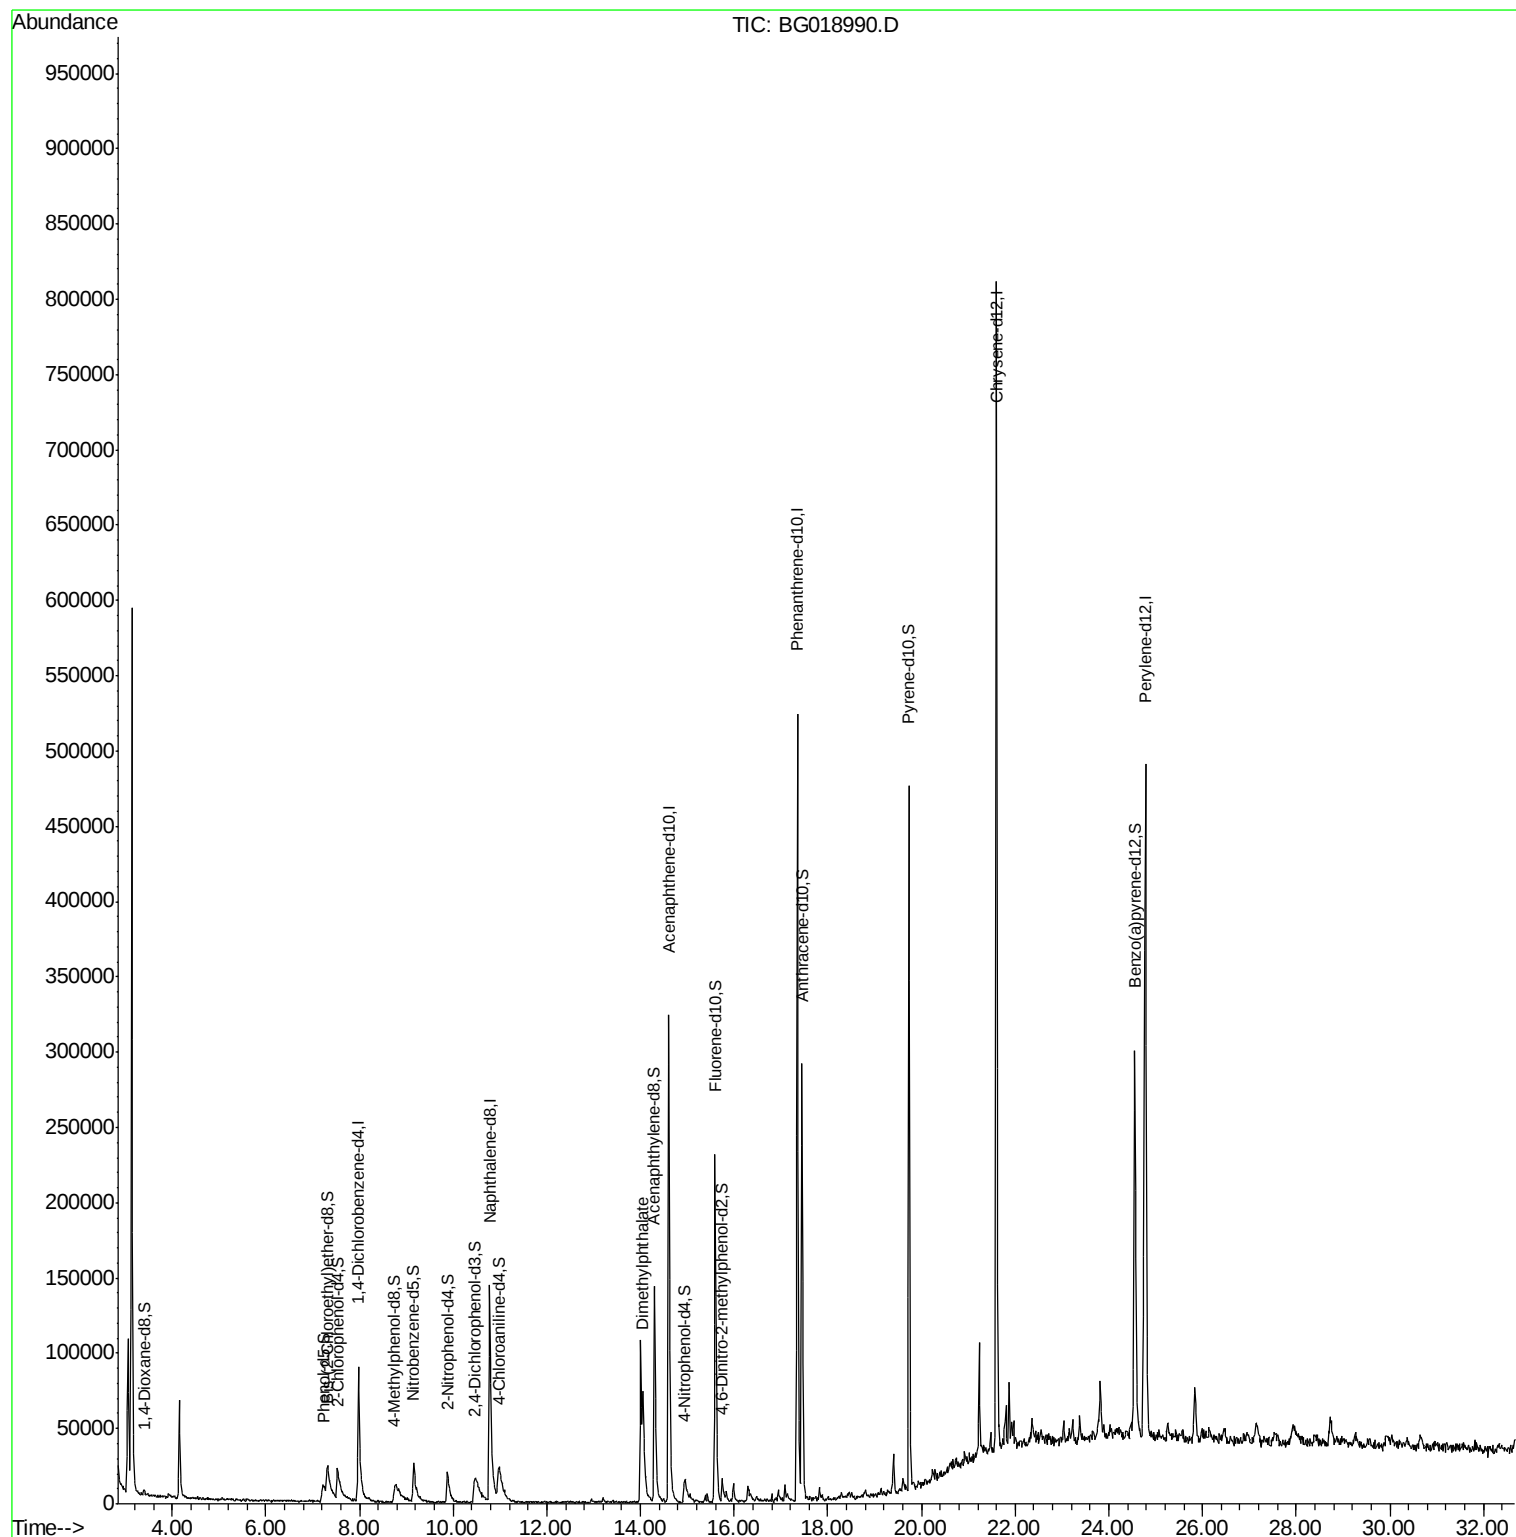

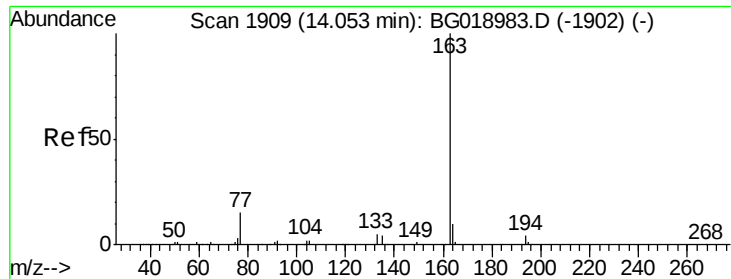

#45

Dimethylphthalate

Concen: 6.61 ng/ul

RT: 14.06 min Scan# 1909

Delta R.T. 0.00 min

Lab File: BG018990.D

Acq: 1 Oct 2015 22:03

Instrument :

BNA_G

ClientSampleId :

E5MZ4


Tot Ion:163 Resp: 81467

Ion Ratio Lower Upper

163 100

194 4.1 2.9 4.3

164 9.7 7.7 11.5

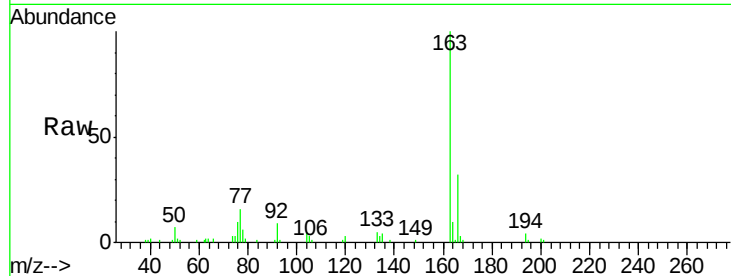

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

