

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100215\
 Data File : BG018995.D
 Acq On : 2 Oct 2015 1:12
 Operator : UM/NP
 Sample : G3865-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5MY3

Quant Time: Oct 02 04:39:47 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 04:39:32 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.97	152	46921	20.00	ng/ul	0.00
18) Naphthalene-d8	10.78	136	206656	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.60	164	144292	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.35	188	376256	20.00	ng/ul	0.00
78) Chrysene-d12	21.60	240	469860	20.00	ng/ul	0.00
86) Perylene-d12	24.77	264	469199	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.40	96	5930	6.08	ng/uL	0.00
5) Phenol-d5	7.20	99	29753	7.72	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.30	67	61572	27.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.52	132	84283	28.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	37725	12.07	ng/ul	0.03
19) Nitrobenzene-d5	9.15	128	40268	25.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.86	143	50175	31.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.45	165	67446	20.34	ng/ul	0.02
29) 4-Chloroaniline-d4	10.97	131	68460	17.75	ng/ul	0.03
44) Dimethylphthalate-d6	14.01	166	369078	31.78	ng/ul	0.00
47) Acenaphthylene-d8	14.29	160	460572	33.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	16545	7.42	ng/ul	0.02
58) Fluorene-d10	15.59	176	344267	33.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.73	200	33936	19.05	ng/ul	0.00
71) Anthracene-d10	17.45	188	556399	33.59	ng/ul	0.00
79) Pyrene-d10	19.73	212	688282	31.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.56	264	757448	33.17	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.05	163	198750	17.66	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100215\
Data File : BG018995.D
Acq On : 2 Oct 2015 1:12
Operator : UM/NP
Sample : G3865-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5MY3

Quant Time: Oct 02 04:39:47 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG091015.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 04:39:32 2015
Response via : Initial Calibration

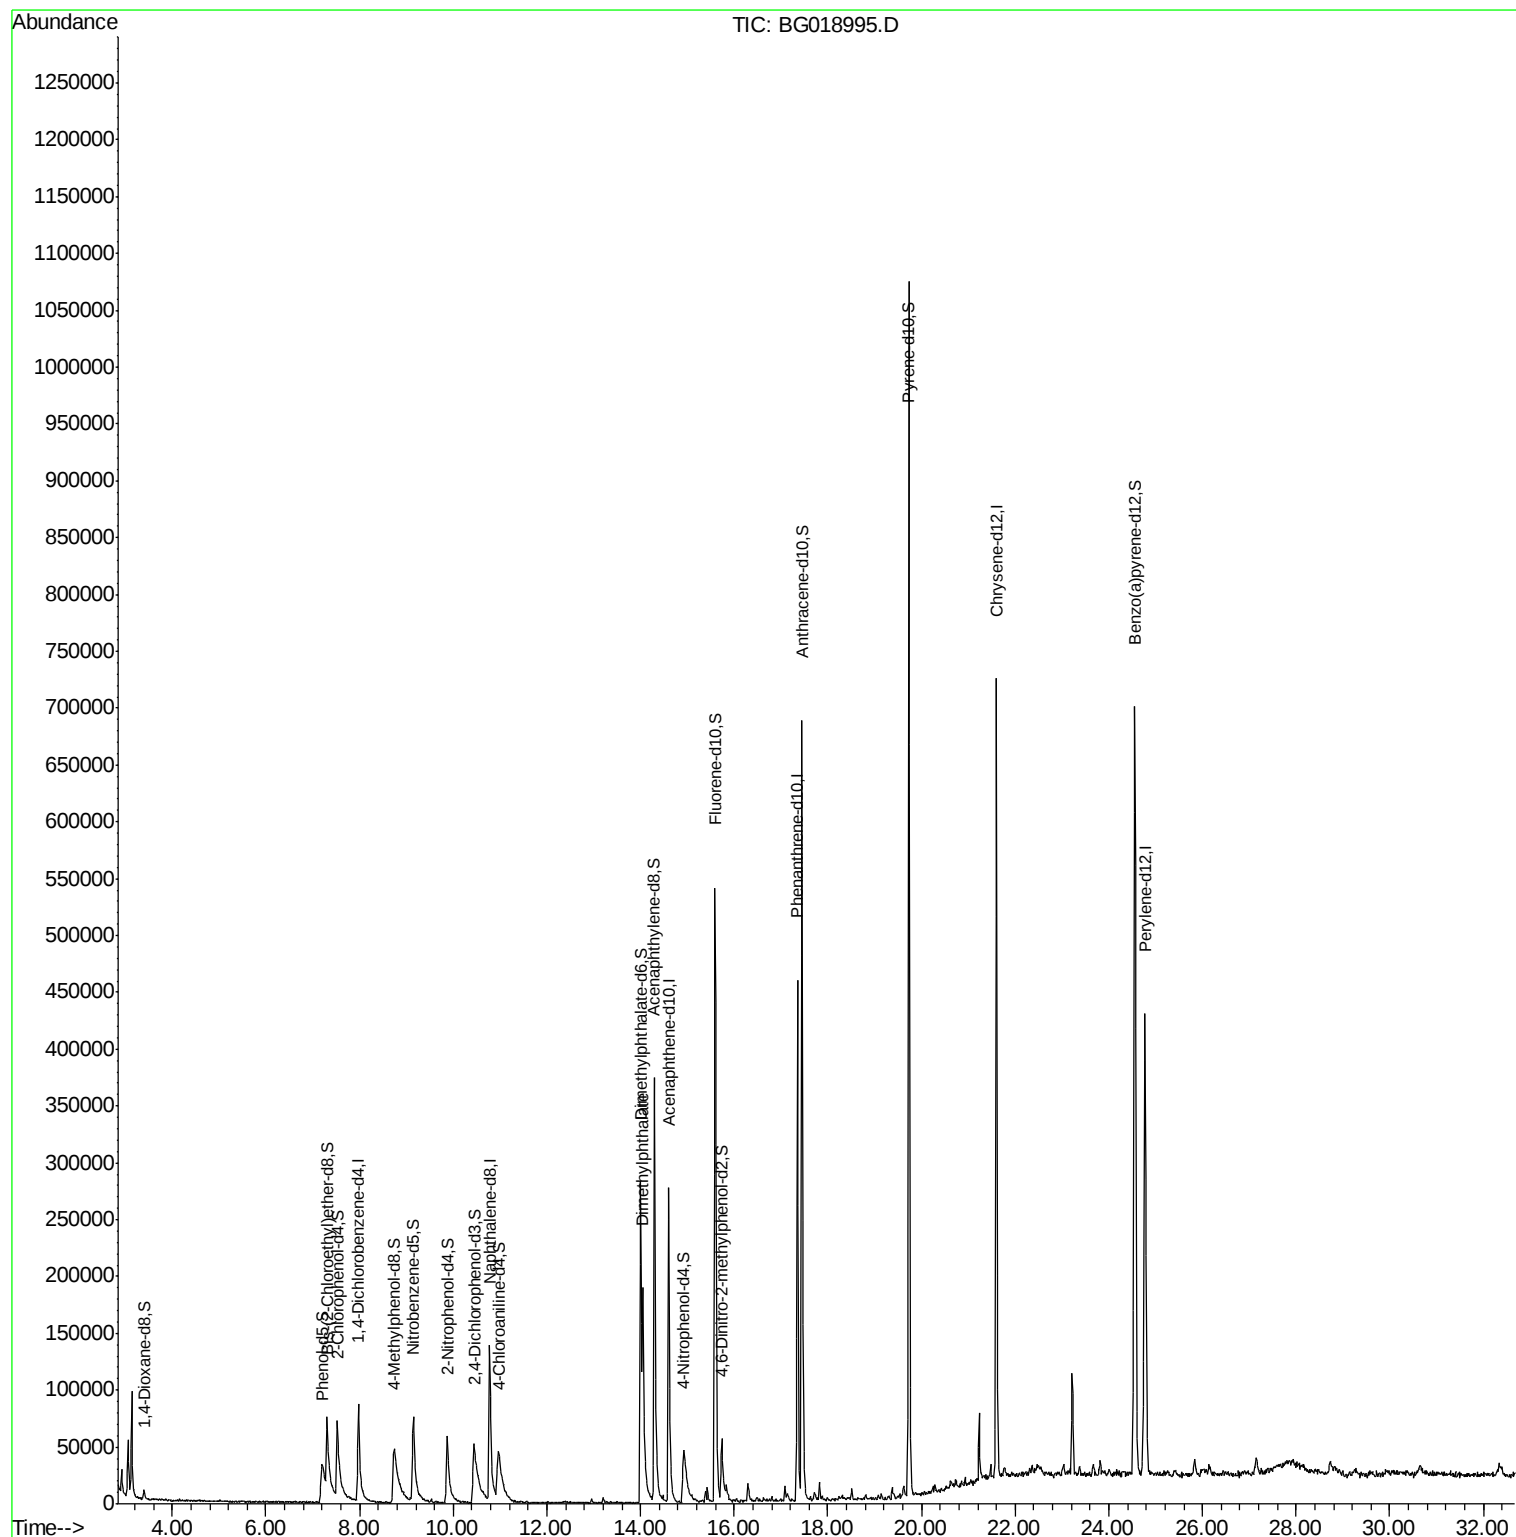


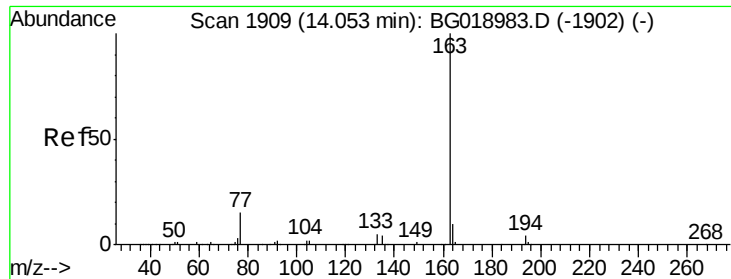

#45
 Dimethylphthalate
 Concen: 17.66 ng/ul
 RT: 14.05 min Scan# 1908
 Delta R.T. -0.01 min
 Lab File: BG018995.D
 Acq: 2 Oct 2015 1:12

Instrument :
 BNA_G
 ClientSampleId :
 E5MY3

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.1	2.9	4.3
164	8.9	7.7	11.5

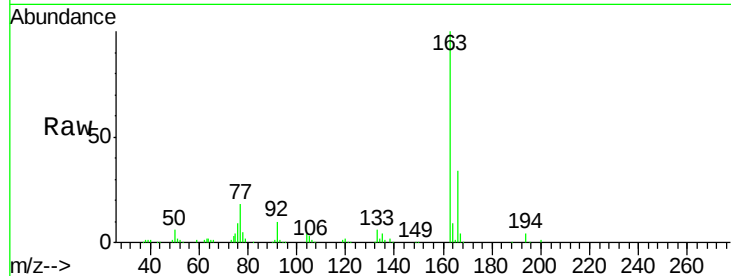

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

