

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100218\
 Data File : BG037113.D
 Acq On : 2 Oct 2018 20:34
 Operator : JU/SJ
 Sample : J5200-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1


Quant Time: Oct 03 01:57:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	55576	20.00	ng	0.00
21) Naphthalene-d8	10.84	136	219841	20.00	ng	-0.02
38) Acenaphthene-d10	14.67	164	129925	20.00	ng	0.00
63) Phenanthrene-d10	17.41	188	318290	20.00	ng	0.00
75) Chrysene-d12	21.67	240	318904	20.00	ng	-0.02
86) Perylene-d12	24.88	264	307681	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.62	112	361636	124.79	ng	0.00
7) Phenol-d6	7.20	99	427729	95.40	ng	0.00
23) Nitrobenzene-d5	9.20	82	367347	89.48	ng	0.00
41) 2,4,6-Tribromophenol	16.15	330	175982	113.21	ng	-0.02
44) 2-Fluorobiphenyl	13.28	172	736829	84.47	ng	-0.02
78) Terphenyl-d14	20.02	244	1192499	98.33	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.20	70	49157	13.179	ng	# 72
50) 2,6-Dinitrotoluene	14.67	165	16490	7.227	ng	# 21
56) 2,4-Dinitrotoluene	14.67	165	16490	5.179	ng	# 19
66) 4-Bromophenyl-phenylether	16.15	248	12197	3.369	ng	# 1
76) Benzidine	20.02	184	19961	2.071	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG100218\
Data File : BG037113.D
Acq On : 2 Oct 2018 20:34
Operator : JU/SJ
Sample : J5200-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Oct 03 01:57:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

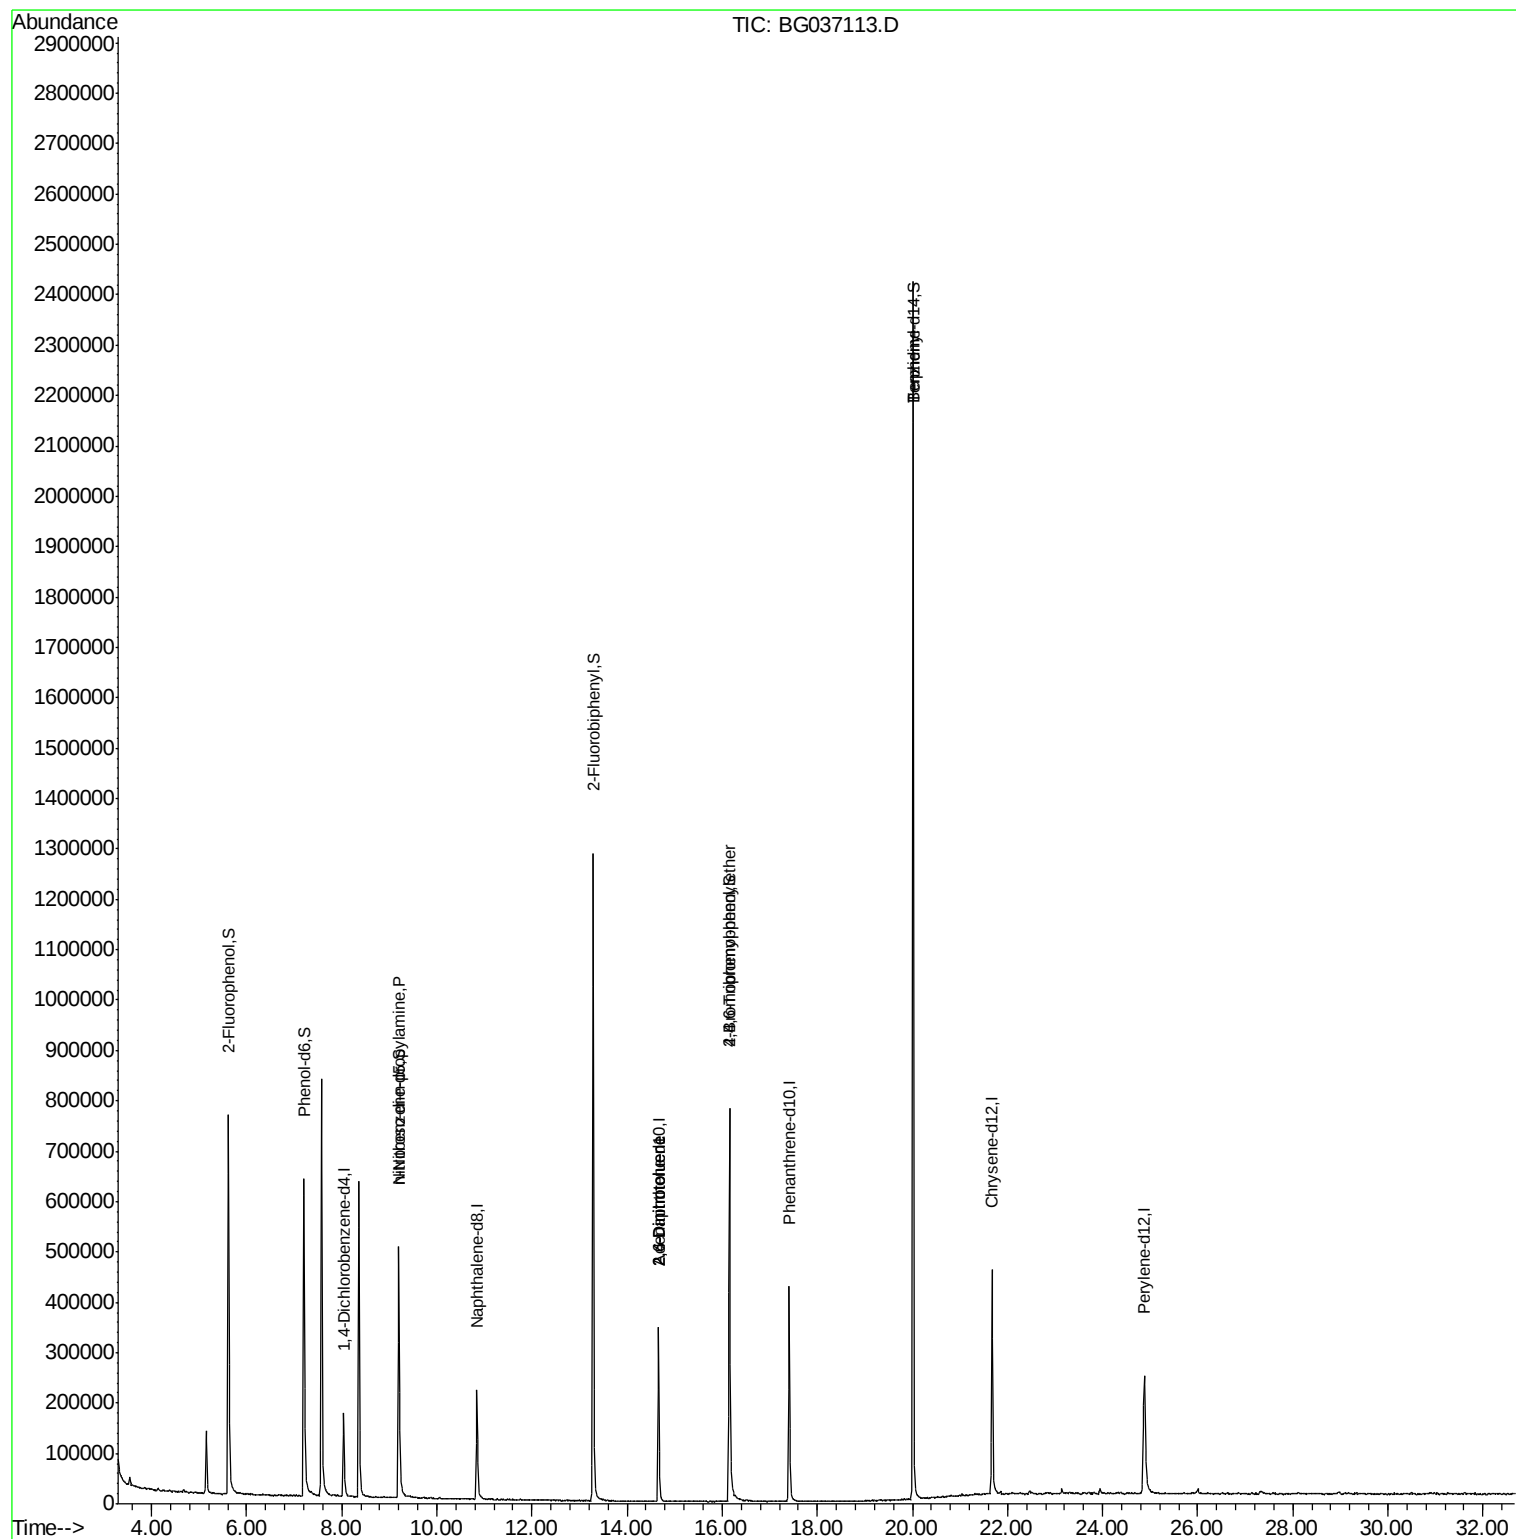


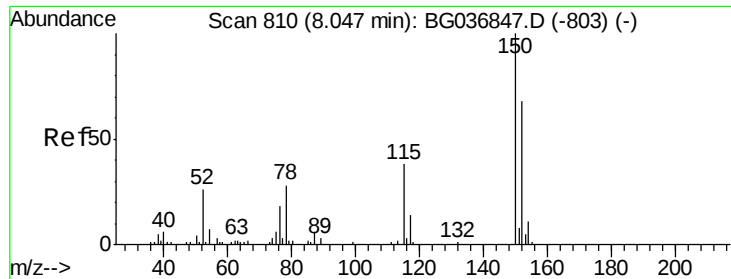




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 809
Delta R.T. -0.00 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion:152 Resp: 55576
Ion Ratio Lower Upper
152 100
150 151.0 119.5 179.3
115 60.9 44.5 66.7

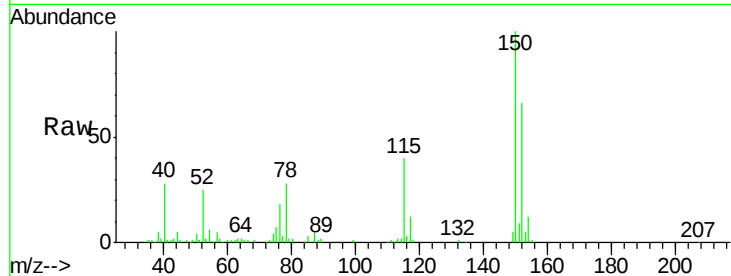


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

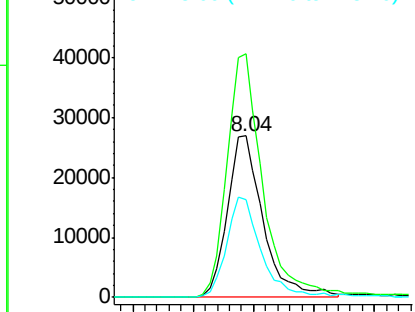



#5

2-Fluorophenol
Concen: 124.791 ng
RT: 5.62 min Scan# 396
Delta R.T. -0.00 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion:112 Resp: 361636
Ion Ratio Lower Upper
112 100
64 71.4 57.2 85.8
63 37.6 30.8 46.2



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

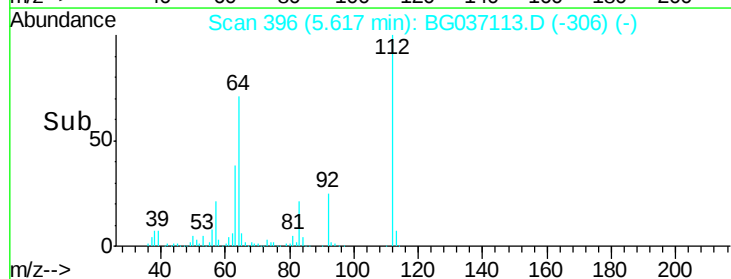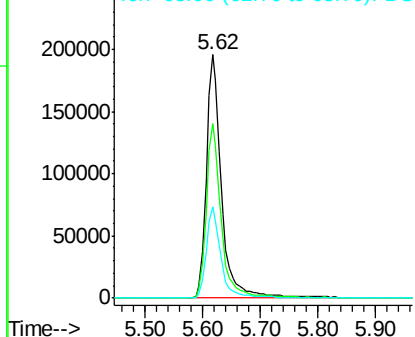



#7

Phenol-d6

Concen: 95.399 ng

RT: 7.20 min Scan# 666

Delta R.T. -0.01 min

Lab File: BG037113.D

Acq: 2 Oct 2018 20:34


Tgt Ion: 99 Resp: 427729

Ion Ratio Lower Upper




99 100

42 21.7 16.5 24.7

71 36.4 29.4 44.2

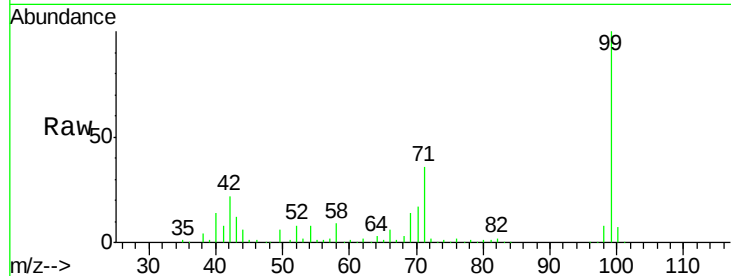

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

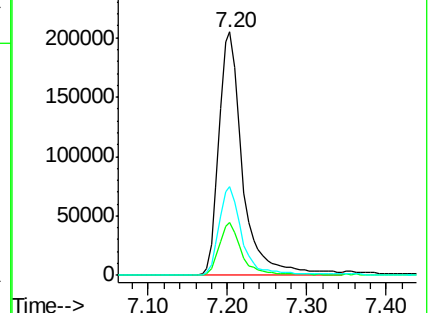

#19

n-Nitroso-di-n-propylamine

Concen: 13.179 ng

RT: 9.20 min Scan# 1006

Delta R.T. 0.35 min

Lab File: BG037113.D

Acq: 2 Oct 2018 20:34

Tgt Ion: 70 Resp: 49157


Ion Ratio Lower Upper

70 100



42 49.8 56.2 84.4#

101 0.0 7.8 11.6#

130 2.3 16.2 24.2#




Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

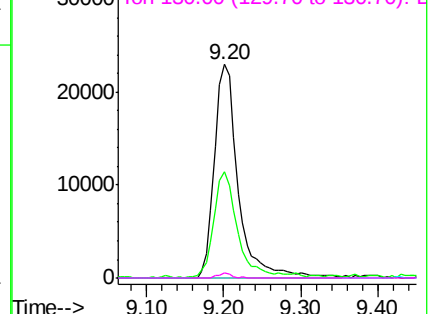






#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.84 min Scan# 1285
Delta R.T. -0.02 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion:	136	Resp:	219841
Ion	Ratio	Lower	Upper
136	100		
137	11.5	8.8	13.2
54	10.3	9.2	13.8
68	7.7	5.8	8.6

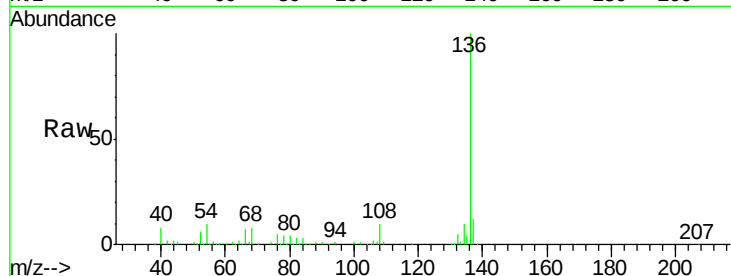


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

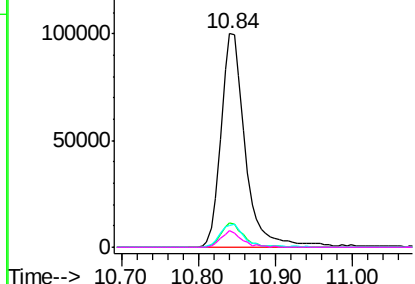




#23
Nitrobenzene-d5
Concen: 89.482 ng
RT: 9.20 min Scan# 1006
Delta R.T. -0.01 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion:	82	Resp:	367347
Ion	Ratio	Lower	Upper
82	100		
128	40.2	33.3	49.9
54	55.5	45.1	67.7




Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

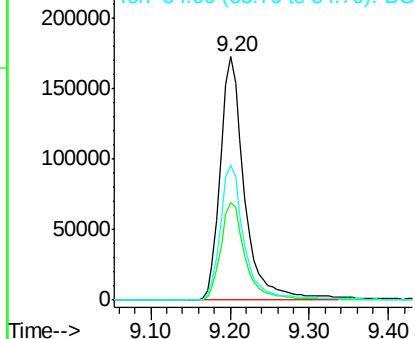



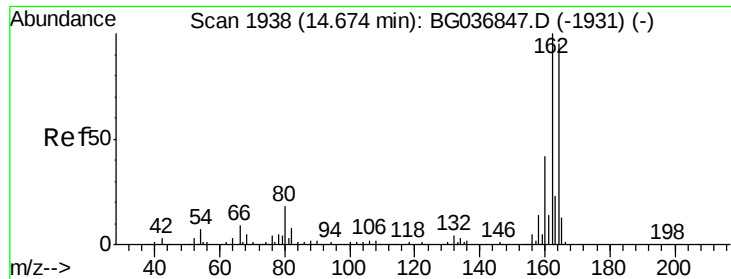


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.67 min Scan# 1936
Delta R.T. -0.01 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion	Ratio	Lower	Upper
164	100		
162	106.2	80.7	121.1
160	45.7	35.3	52.9

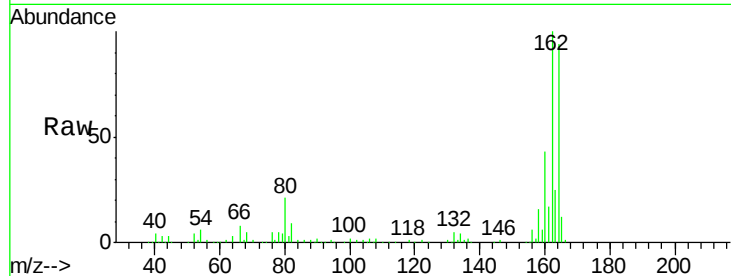


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E


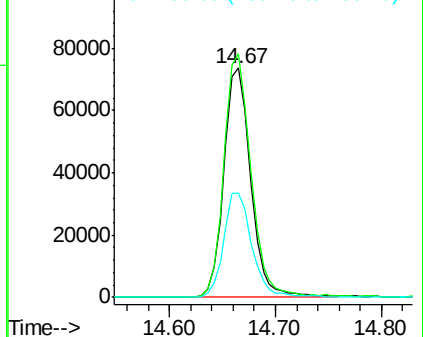


#41
2,4,6-Tribromophenol
Concen: 113.210 ng
RT: 16.15 min Scan# 2189
Delta R.T. -0.02 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.6	75.4	113.2
141	38.6	30.7	46.1

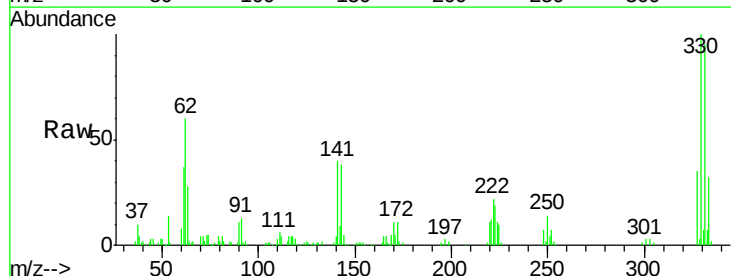


Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

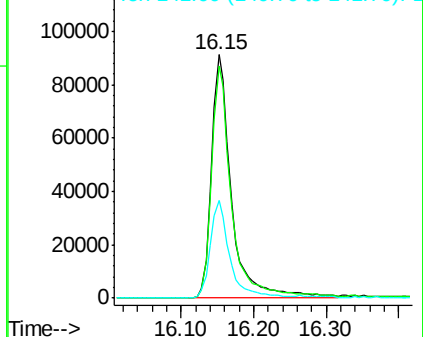






#44
 2-Fluorobiphenyl
 Concen: 84.466 ng
 RT: 13.28 min Scan# 1701
 Delta R.T. -0.02 min
 Lab File: BG037113.D
 Acq: 2 Oct 2018 20:34

Tgt Ion:	172	Resp:	736829
Ion	Ratio	Lower	Upper
172	100		
171	36.8	31.3	46.9
170	24.9	21.0	31.6

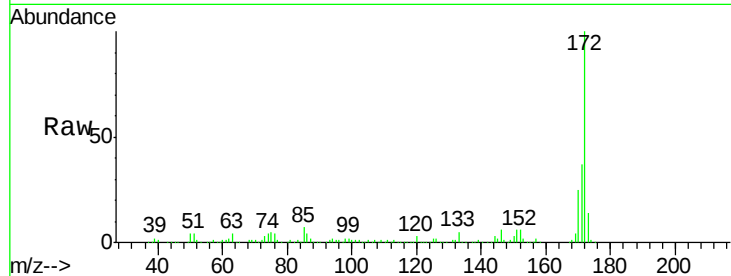


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

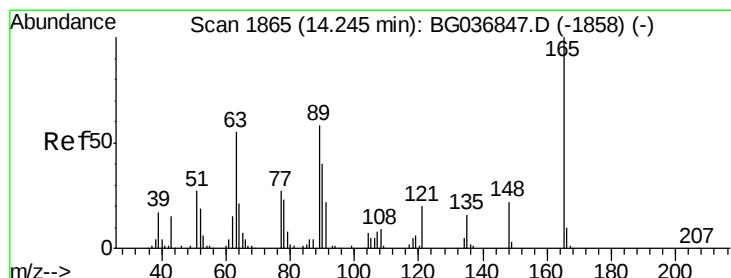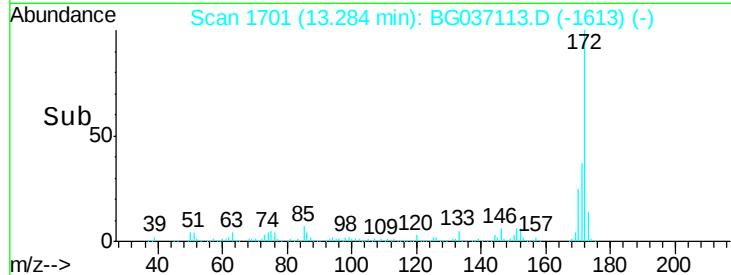
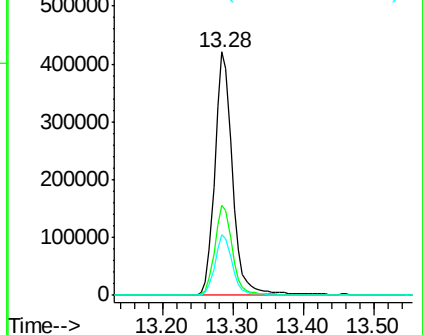


#50
 2,6-Dinitrotoluene
 Concen: 7.227 ng
 RT: 14.67 min Scan# 1936
 Delta R.T. 0.42 min
 Lab File: BG037113.D
 Acq: 2 Oct 2018 20:34

Tgt Ion:	165	Resp:	16490
Ion	Ratio	Lower	Upper
165	100		
63	0.0	50.1	75.1#
89	1.9	47.8	71.6#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BG0
 Ion 89.00 (88.70 to 89.70): BG0

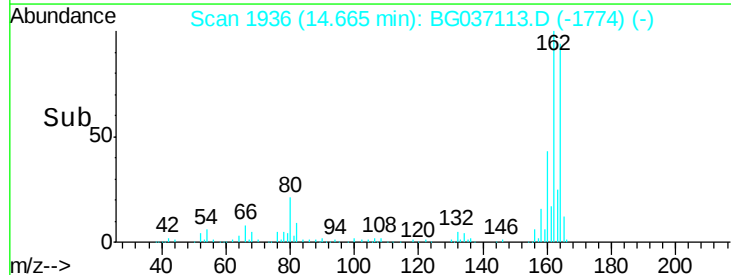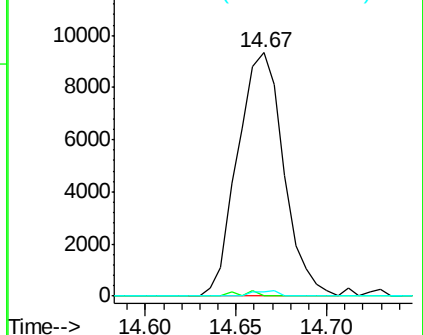



#56
 2,4-Dinitrotoluene
 Concen: 5.179 ng
 RT: 14.67 min Scan# 1936
 Delta R.T. -0.37 min
 Lab File: BG037113.D
 Acq: 2 Oct 2018 20:34

Tgt Ion:	165	Resp:	16490
Ion	Ratio	Lower	Upper
165	100		
63	0.0	40.1	60.1#
89	1.9	63.7	95.5#
182	0.0	2.5	3.7#


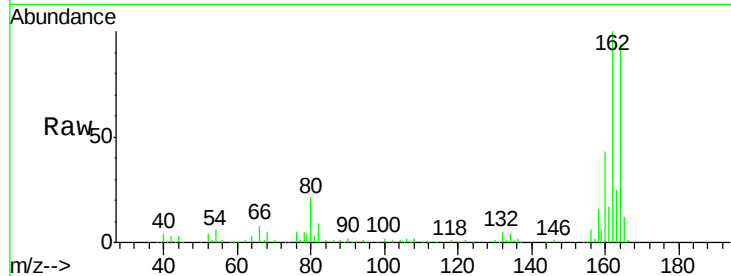


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BGC

Ion 89.00 (88.70 to 89.70): BGC

Ion 182.00 (181.70 to 182.70): E

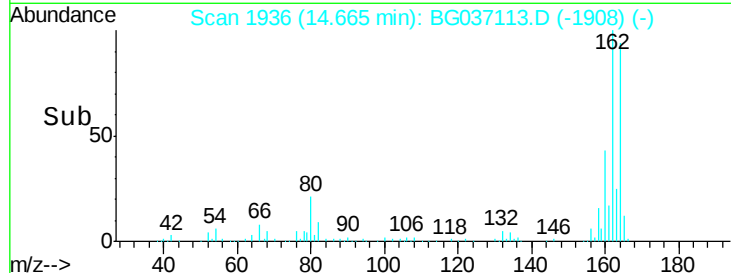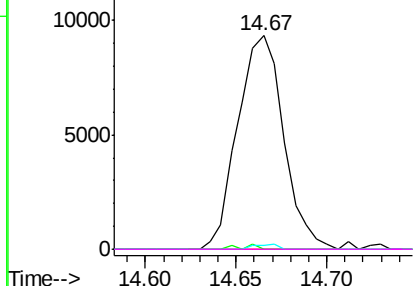




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.41 min Scan# 2403
 Delta R.T. -0.01 min
 Lab File: BG037113.D
 Acq: 2 Oct 2018 20:34

Tgt Ion:	188	Resp:	318290
Ion	Ratio	Lower	Upper
188	100		
94	9.1	6.7	10.1
80	10.1	8.1	12.1

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC


Ion 80.00 (79.70 to 80.70): BGC

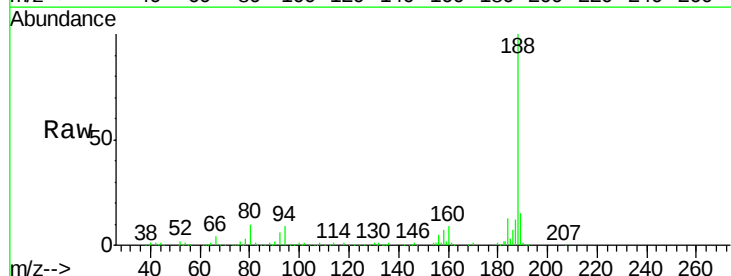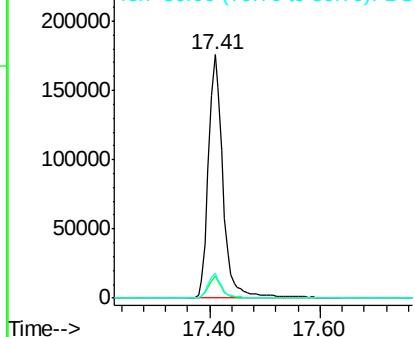






#66
 4-Bromophenyl-phenylether
 Concen: 3.369 ng
 RT: 16.15 min Scan# 2189
 Delta R.T. -0.46 min
 Lab File: BG037113.D
 Acq: 2 Oct 2018 20:34

Tgt Ion:248 Resp: 12197
 Ion Ratio Lower Upper
 248 100
 250 216.0 78.1 117.1#
 141 601.1 53.7 80.5#

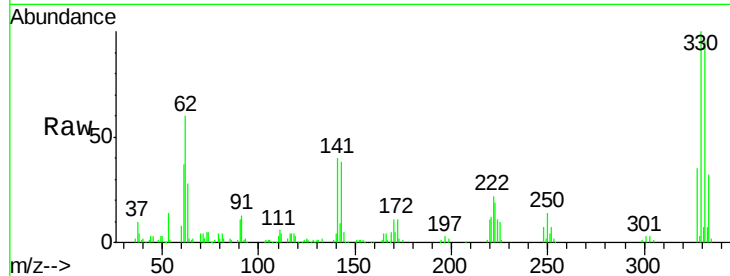


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

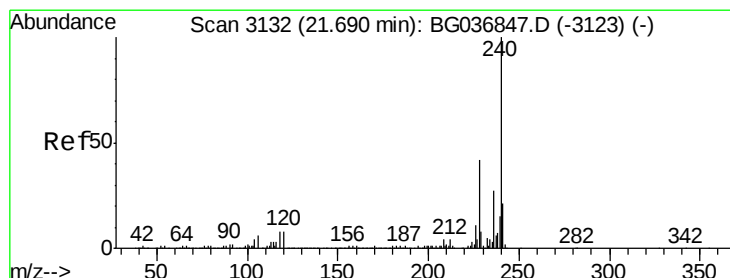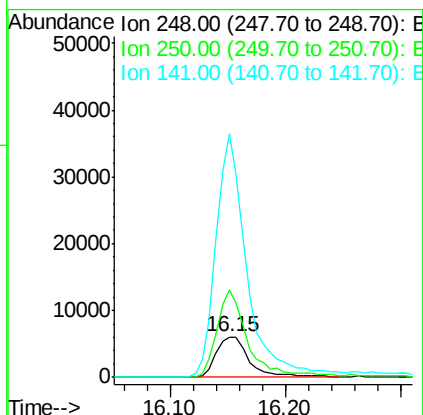
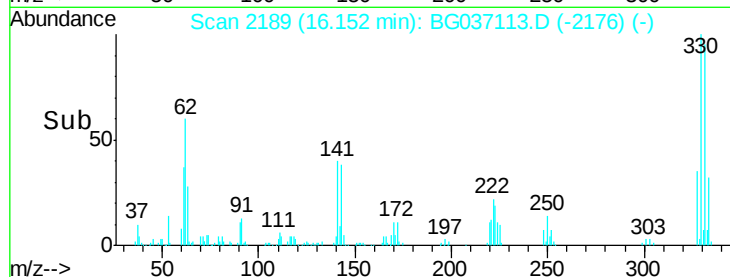


#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.67 min Scan# 3129
 Delta R.T. -0.02 min
 Lab File: BG037113.D
 Acq: 2 Oct 2018 20:34

Tgt Ion:240 Resp: 318904
 Ion Ratio Lower Upper
 240 100
 120 8.9 6.9 10.3
 236 26.2 21.2 31.8

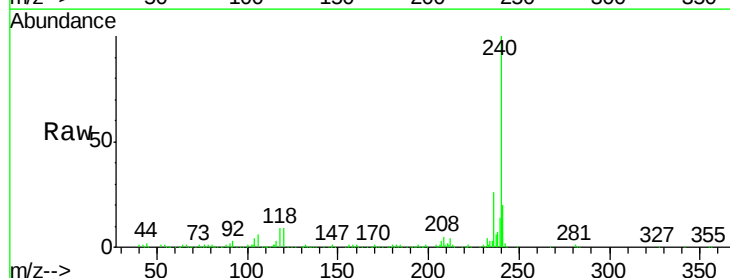





Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

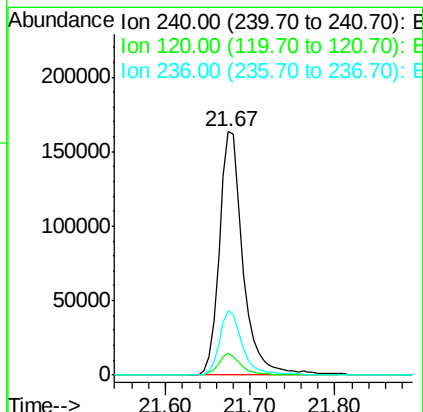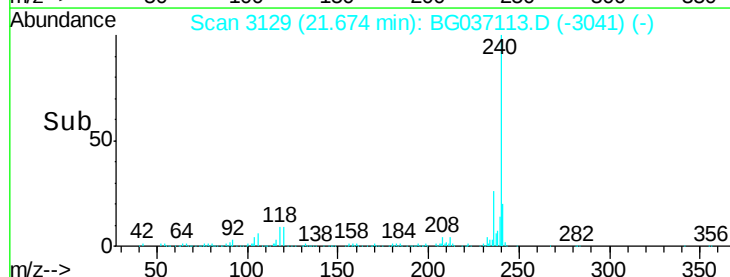






#76
Benzidine
Concen: 2.071 ng
RT: 20.02 min Scan# 2847
Delta R.T. 0.37 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34


Tgt Ion:184 Resp: 19961
Ion Ratio Lower Upper
184 100
185 17.0 12.6 18.8
183 9.3 10.9 16.3#

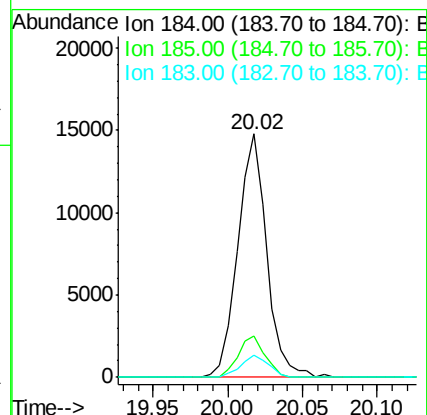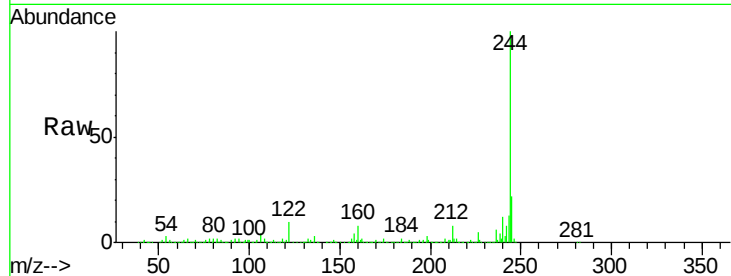

#78
Terphenyl-d14
Concen: 98.326 ng
RT: 20.02 min Scan# 2847
Delta R.T. -0.01 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion:244 Resp: 1192499
Ion Ratio Lower Upper
244 100
212 8.4 7.0 10.6
122 9.5 7.1 10.7

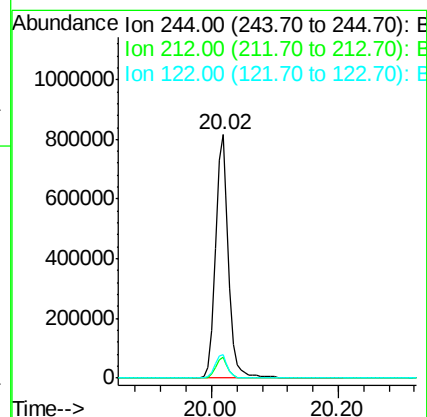

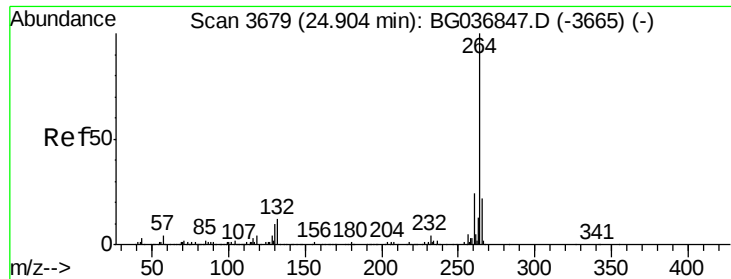

#86
Perylene-d12
Concen: 20.000 ng
RT: 24.88 min Scan# 3674
Delta R.T. -0.03 min
Lab File: BG037113.D
Acq: 2 Oct 2018 20:34

Tgt Ion:	264	Resp:	307681
Ion	Ratio	Lower	Upper
264	100		
260	23.7	19.6	29.4
265	22.2	17.4	26.0

