


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100218\
 Data File : BG037106.D
 Acq On : 2 Oct 2018 16:02
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

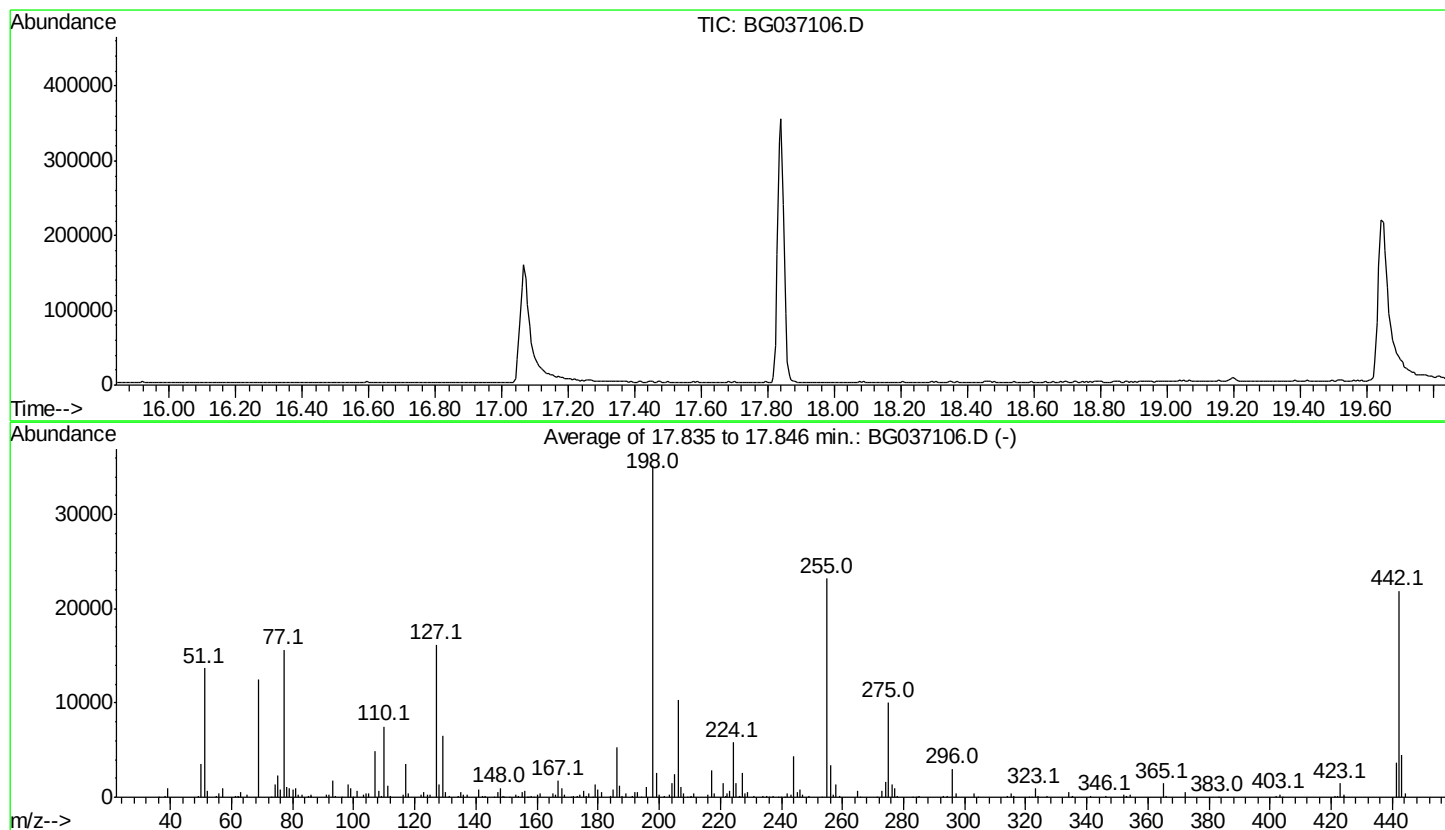

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.9	13681	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.4	12458	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	16201	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35176	PASS
199	198	5	9	7.5	2623	PASS
275	198	10	60	28.5	10036	PASS
365	198	1	100	4.1	1432	PASS
441	198	0.01	100	10.4	3659	PASS
442	198	50	100	62.2	21893	PASS
443	442	15	24	20.5	4485	PASS