

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100220\
 Data File : BG046754.D
 Acq On : 3 Oct 2020 3:06
 Operator : CG/JU
 Sample : L4151-17
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7L8

Quant Time: Oct 03 04:00:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 03:57:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	78930	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	323163	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	231986	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	553278	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	558441	20.00	ng/ul	0.00
86) Perylene-d12	25.02	264	570897	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.54	96	5448	3.39	ng/uL	0.00
5) Phenol-d5	7.25	99	114002	16.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	72453	17.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	88270	17.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	84427	15.98	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	45113	18.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	53040	21.58	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	101745	17.59	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	76499	11.13	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	334856	18.89	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	379705	18.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	56058	18.55	ng/ul	0.00
58) Fluorene-d10	15.72	176	294982	18.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	48962	17.71	ng/ul	0.00
71) Anthracene-d10	17.57	188	433289	17.07	ng/ul	0.00
79) Pyrene-d10	19.85	212	510853	17.63	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.80	264	496669	16.14	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	14.18	163	27866	1.553	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100220\
Data File : BG046754.D
Acq On : 3 Oct 2020 3:06
Operator : CG/JU
Sample : L4151-17
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7L8

Quant Time: Oct 03 04:00:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 03:57:33 2020
Response via : Initial Calibration

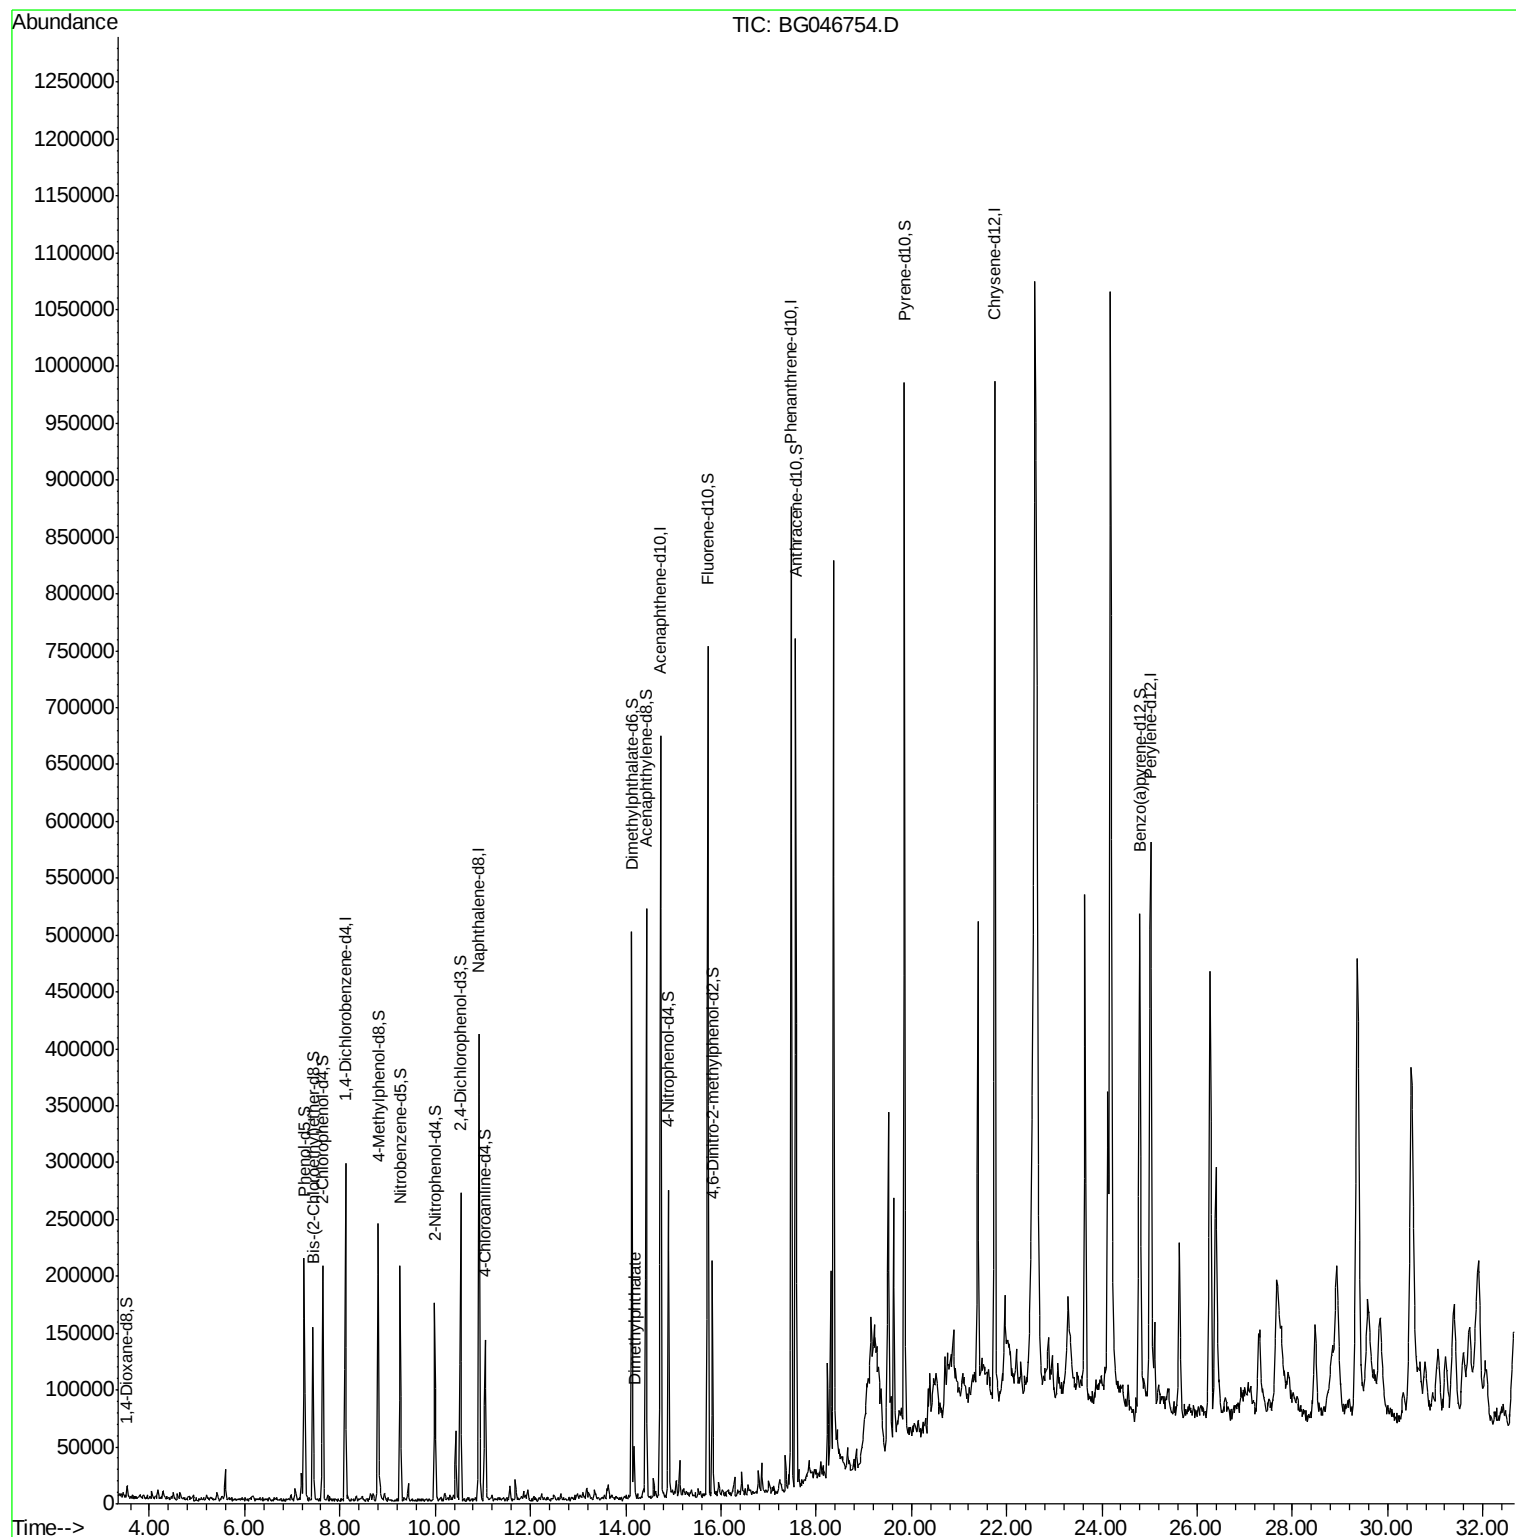


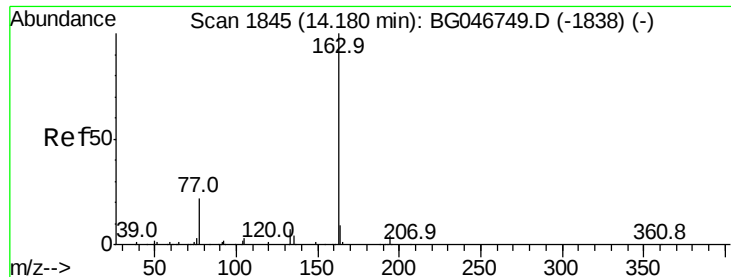

#45
 Dimethylphthalate
 Concen: 1.553 ng/ul
 RT: 14.18 min Scan# 1845
 Delta R.T. -0.01 min
 Lab File: BG046754.D
 Acq: 3 Oct 2020 3:06

Instrument :
 BNA_G
 ClientSampleId :
 CB7L8

Tot Ion	Ratio	Lower	Upper
163	100		
194	5.4	3.6	5.4
164	10.0	7.4	11.0

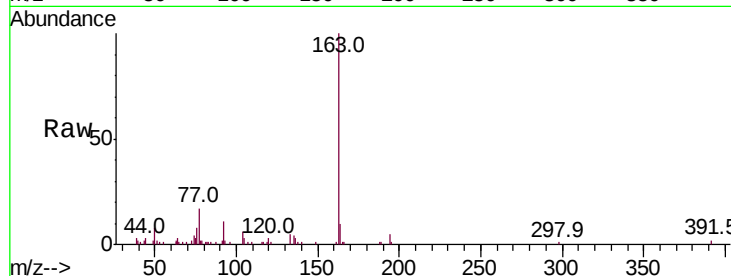

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

