

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100220\
 Data File : BG046778.D
 Acq On : 3 Oct 2020 19:11
 Operator : CG/JU
 Sample : L4150-19
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7M0

Quant Time: Oct 05 01:00:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 00:58:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	78226	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	325825	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	241031	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	561083	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	577314	20.00	ng/ul	0.00
86) Perylene-d12	25.03	264	578621	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	10938	6.86	ng/uL	0.00
5) Phenol-d5	7.25	99	231268	34.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	136325	33.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	174022	35.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	183358	35.02	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	89190	36.57	ng/ul	0.00
22) 2-Nitrophenol-d4	10.00	143	108865	43.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	204001	34.99	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	219622	31.69	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	614897	33.39	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	776345	35.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	113583	36.17	ng/ul	0.00
58) Fluorene-d10	15.72	176	578862	34.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	94045	33.54	ng/ul	0.00
71) Anthracene-d10	17.58	188	874460	33.97	ng/ul	0.00
79) Pyrene-d10	19.86	212	1017978	33.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.80	264	1066925	34.21	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	14.18	163	24219	1.299	ng/ul# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100220\
Data File : BG046778.D
Acq On : 3 Oct 2020 19:11
Operator : CG/JU
Sample : L4150-19
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7M0

Quant Time: Oct 05 01:00:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 00:58:20 2020
Response via : Initial Calibration

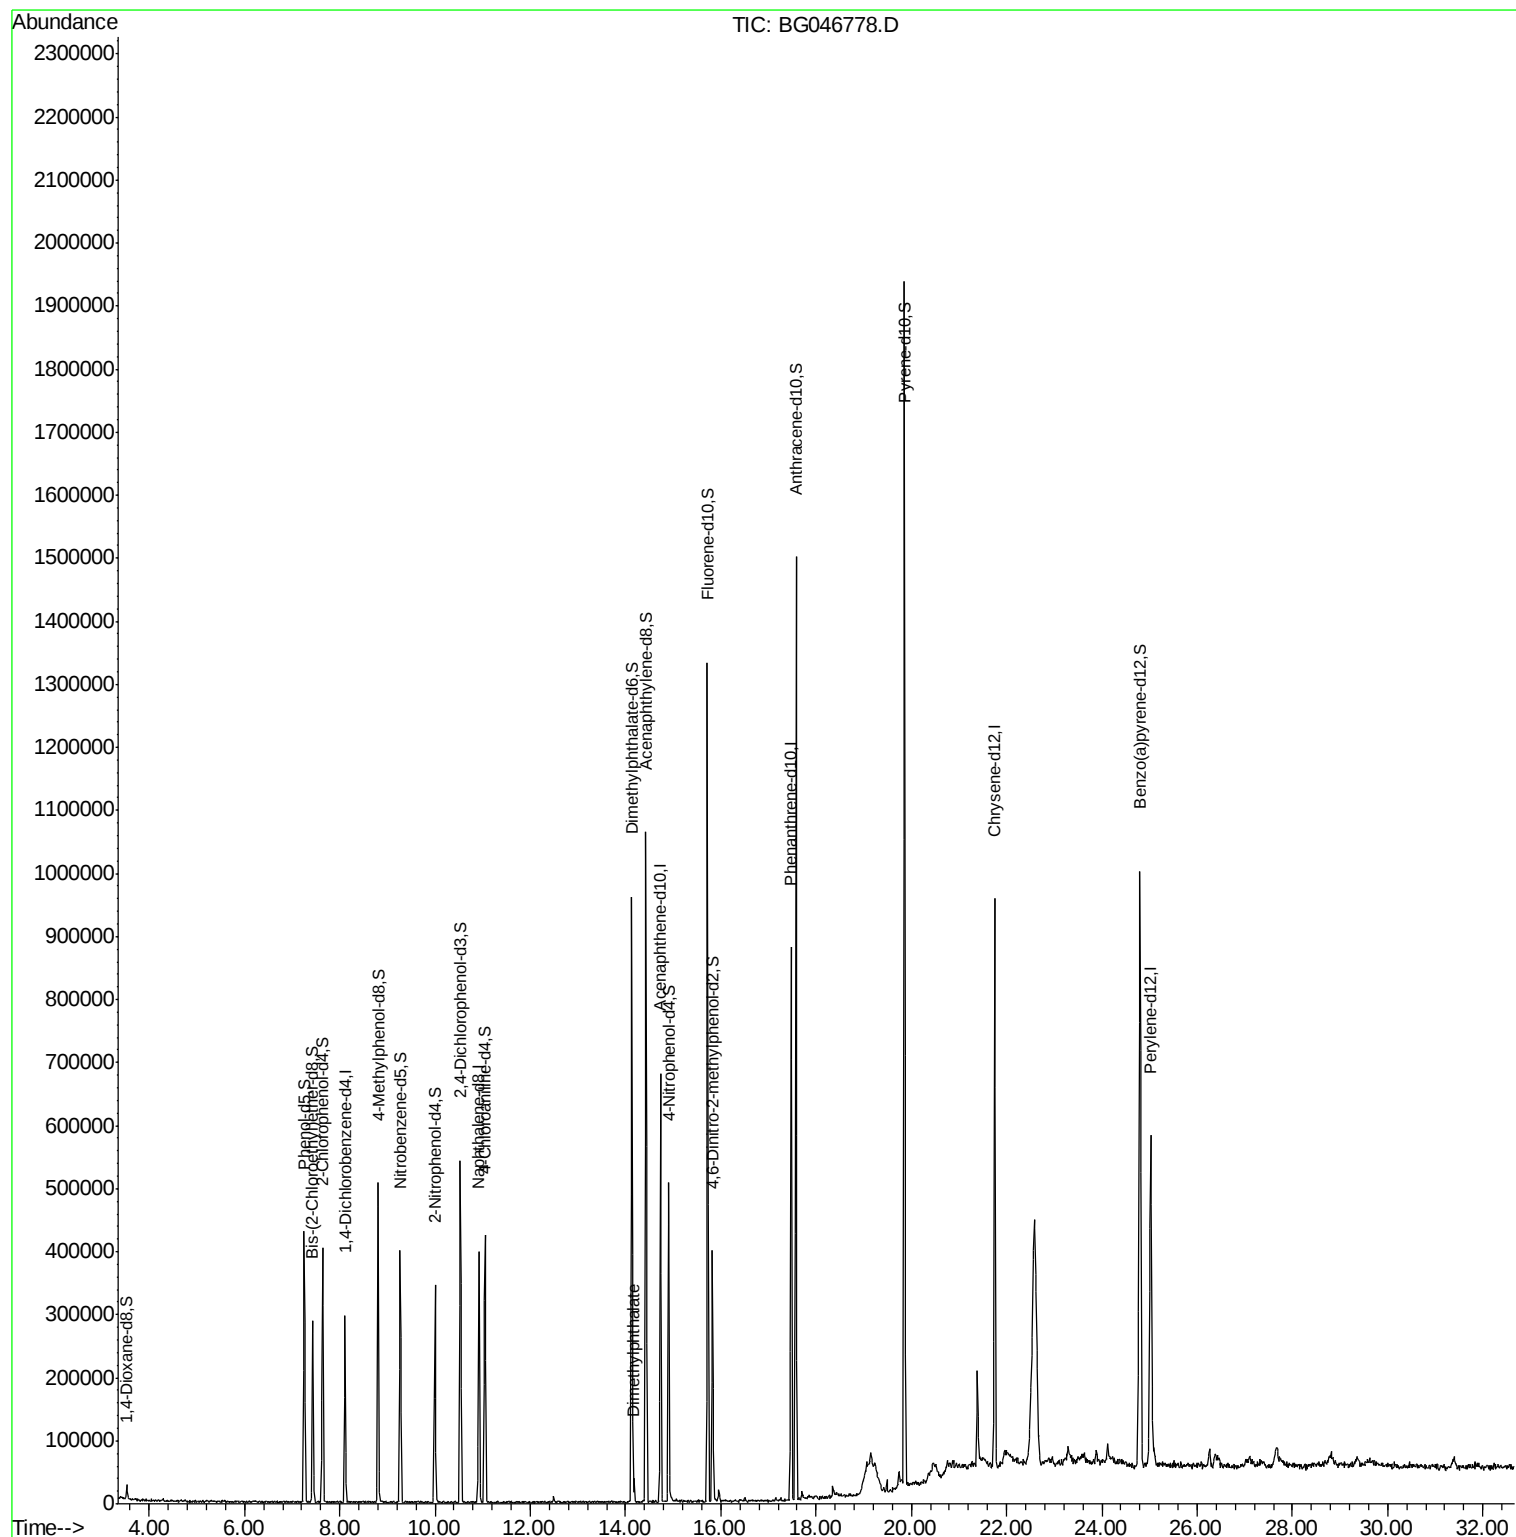

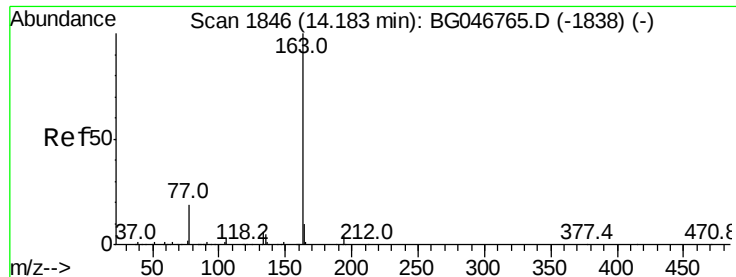

#45

Dimethylphthalate

Concen: 1.299 ng/ul

RT: 14.18 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BG046778.D

Acq: 3 Oct 2020 19:11

Instrument :

BNA_G

ClientSampleId :

CB7M0


Tot Ion:163 Resp: 24219

Ion Ratio Lower Upper

163 100

194 3.6 3.6 5.4#

164 9.1 7.4 11.0

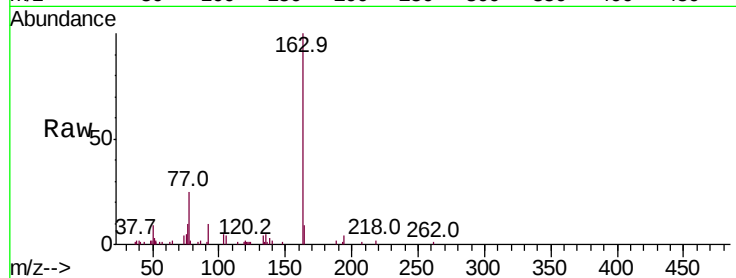

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

