

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100220\
 Data File : BG046780.D
 Acq On : 3 Oct 2020 20:32
 Operator : CG/JU
 Sample : L4151-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7L6

Quant Time: Oct 05 01:00:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 00:58:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.11	152	72018	20.00	ng/ul	0.00
18) Naphthalene-d8	10.92	136	301064	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	218113	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	511240	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	514222	20.00	ng/ul	0.00
86) Perylene-d12	25.03	264	537749	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	5222	3.56	ng/uL	0.00
5) Phenol-d5	7.25	99	119897	19.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.43	67	76041	20.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.64	132	92635	20.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.80	113	99136	20.57	ng/ul	0.00
19) Nitrobenzene-d5	9.27	128	50022	22.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.99	143	59042	25.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.53	165	110396	20.49	ng/ul	0.00
29) 4-Chloroaniline-d4	11.05	131	96462	15.07	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	357696	21.46	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	407096	20.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.90	143	56240	19.79	ng/ul	0.00
58) Fluorene-d10	15.72	176	316170	20.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.82	200	43758	17.13	ng/ul	0.00
71) Anthracene-d10	17.58	188	445725	19.00	ng/ul	0.00
79) Pyrene-d10	19.86	212	528616	19.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.80	264	518703	17.90	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	14.18	163	37169	2.204	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100220\
Data File : BG046780.D
Acq On : 3 Oct 2020 20:32
Operator : CG/JU
Sample : L4151-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7L6

Quant Time: Oct 05 01:00:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 00:58:20 2020
Response via : Initial Calibration

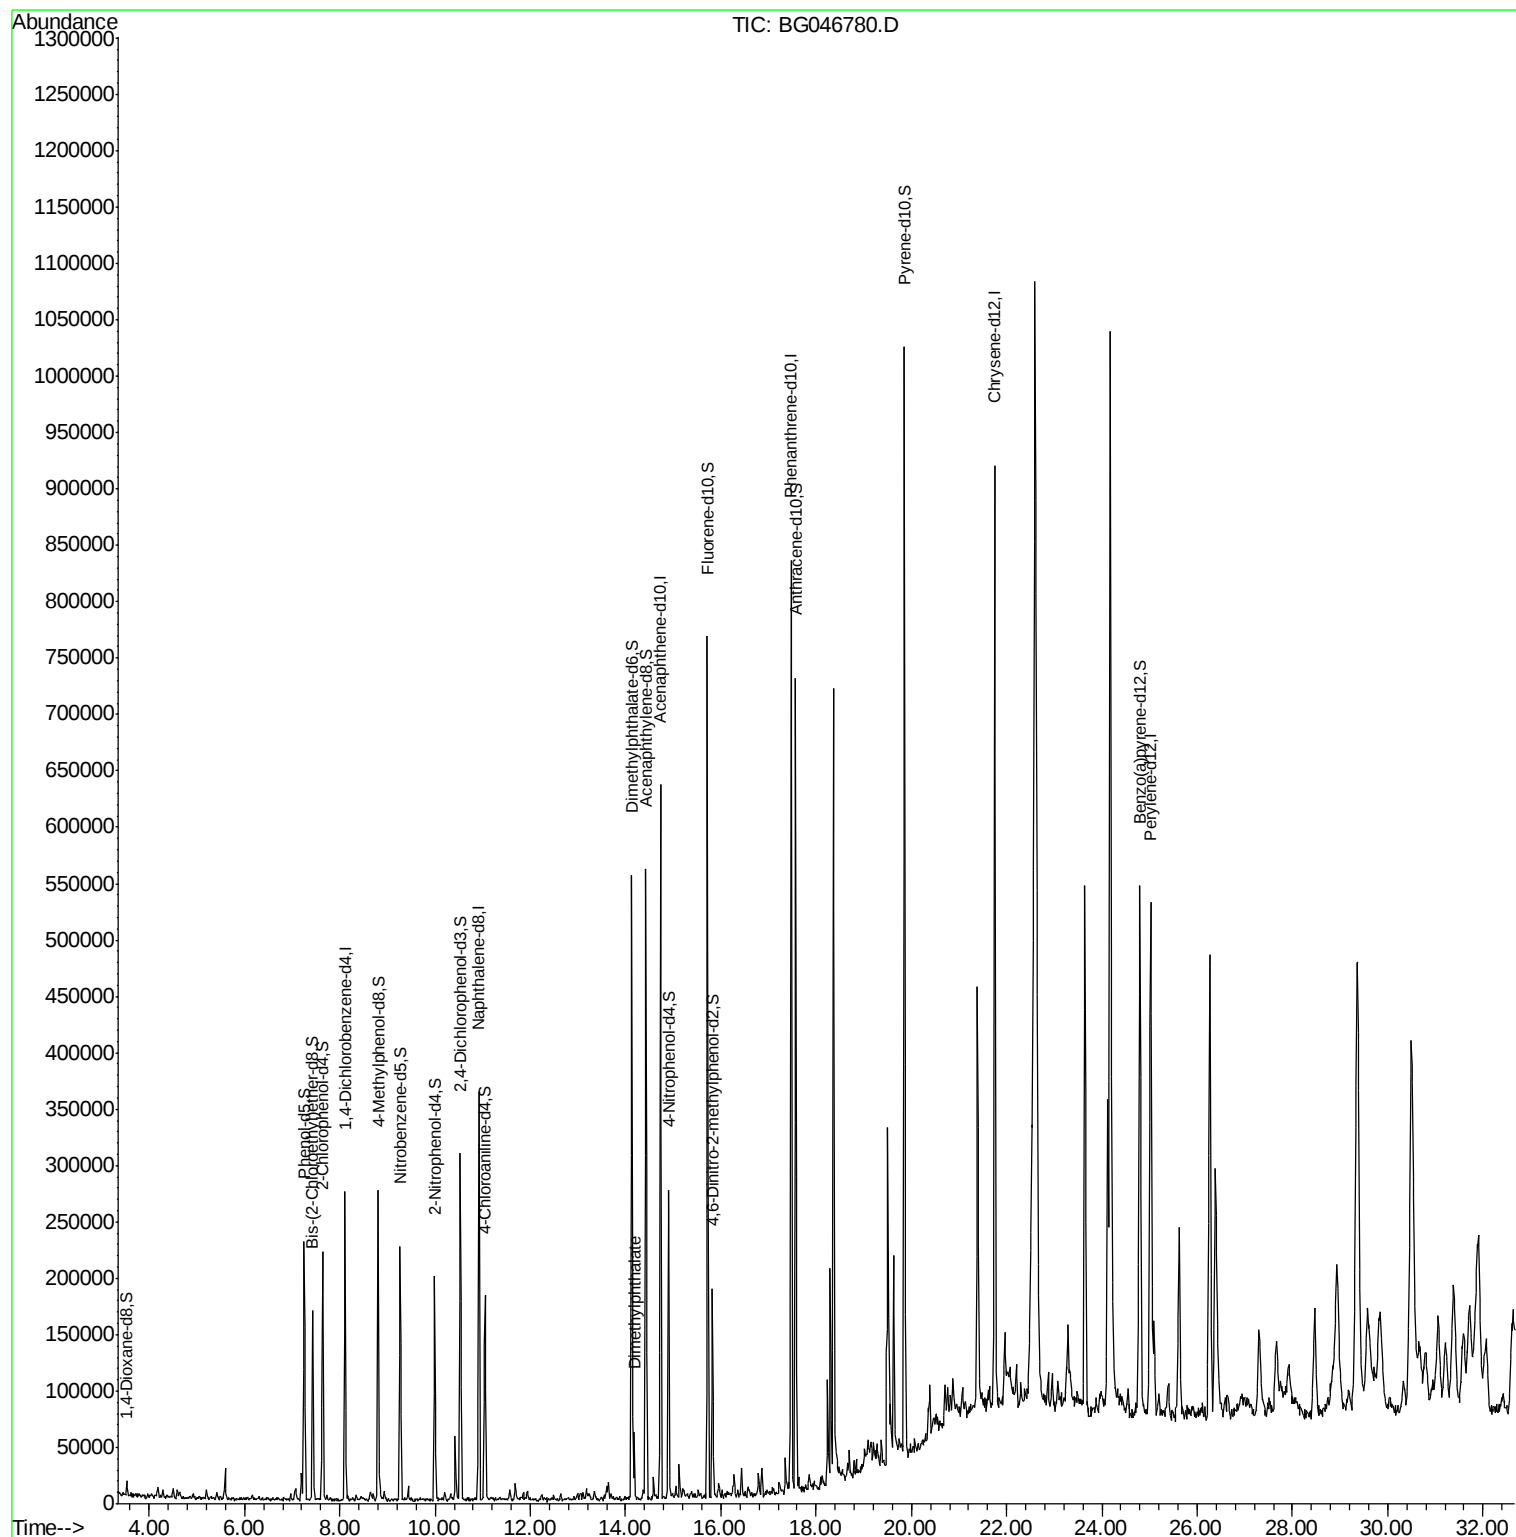

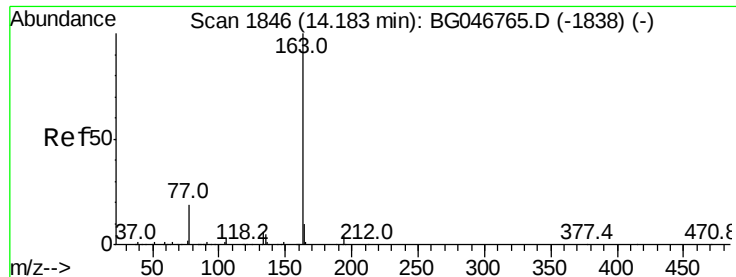

#45

Dimethylphthalate

Concen: 2.204 ng/ul

RT: 14.18 min Scan# 1845

Delta R.T. -0.00 min

Lab File: BG046780.D

Acq: 3 Oct 2020 20:32

Instrument :

BNA_G

ClientSampleId :

CB7L6


Tot Ion:163 Resp: 37169

Ion Ratio Lower Upper

163 100

194 3.0 3.6 5.4#

164 10.5 7.4 11.0

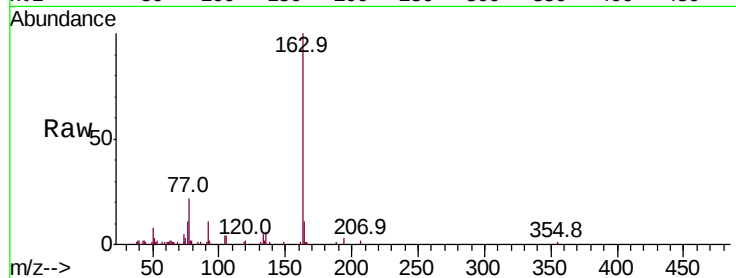

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

