

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046732.D
 Acq On : 2 Oct 2020 11:20
 Operator : CG/JU
 Sample : L4188-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BG0Q8

Quant Time: Oct 02 11:55:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 10:06:22 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	57584	20.00	ng/ul	0.00
18) Naphthalene-d8	10.922	136	233961	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.736	164	174427	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.479	188	444125	20.00	ng/ul	0.00
78) Chrysene-d12	21.751	240	511146	20.00	ng/ul	0.00
86) Perylene-d12	25.029	264	506598	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.531	96	6734	5.74	ng/uL	0.00
5) Phenol-d5	7.256	99	13032	2.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.432	67	78459	26.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.644	132	98787	27.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.801	113	13740	3.56	ng/ul	0.00
19) Nitrobenzene-d5	9.271	128	50925	29.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.994	143	52205	29.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.535	165	104786	25.03	ng/ul	0.00
29) 4-Chloroaniline-d4	0.000	131	0d	0.00	ng/ul	
44) Dimethylphthalate-d6	14.136	166	450619	33.81	ng/ul	0.00
47) Acenaphthylene-d8	14.424	160	178043	11.25	ng/ul	0.00
52) 4-Nitrophenol-d4	14.900	143	16432	7.23	ng/ul	0.00
58) Fluorene-d10	15.723	176	387703	31.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.828	200	71783	32.35	ng/ul	0.00
71) Anthracene-d10	17.579	188	424650	20.84	ng/ul	0.00
79) Pyrene-d10	19.859	212	803592	30.30	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.800	264	593294	21.73	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	14.177	163	48940	3.63	ng/ul	99
84) Bis(2-ethylhexyl)phtha...	21.651	149	39120	2.30	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046732.D
Acq On : 2 Oct 2020 11:20
Operator : CG/JU
Sample : L4188-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BG0Q8

Quant Time: Oct 02 11:55:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 10:06:22 2020
Response via : Initial Calibration




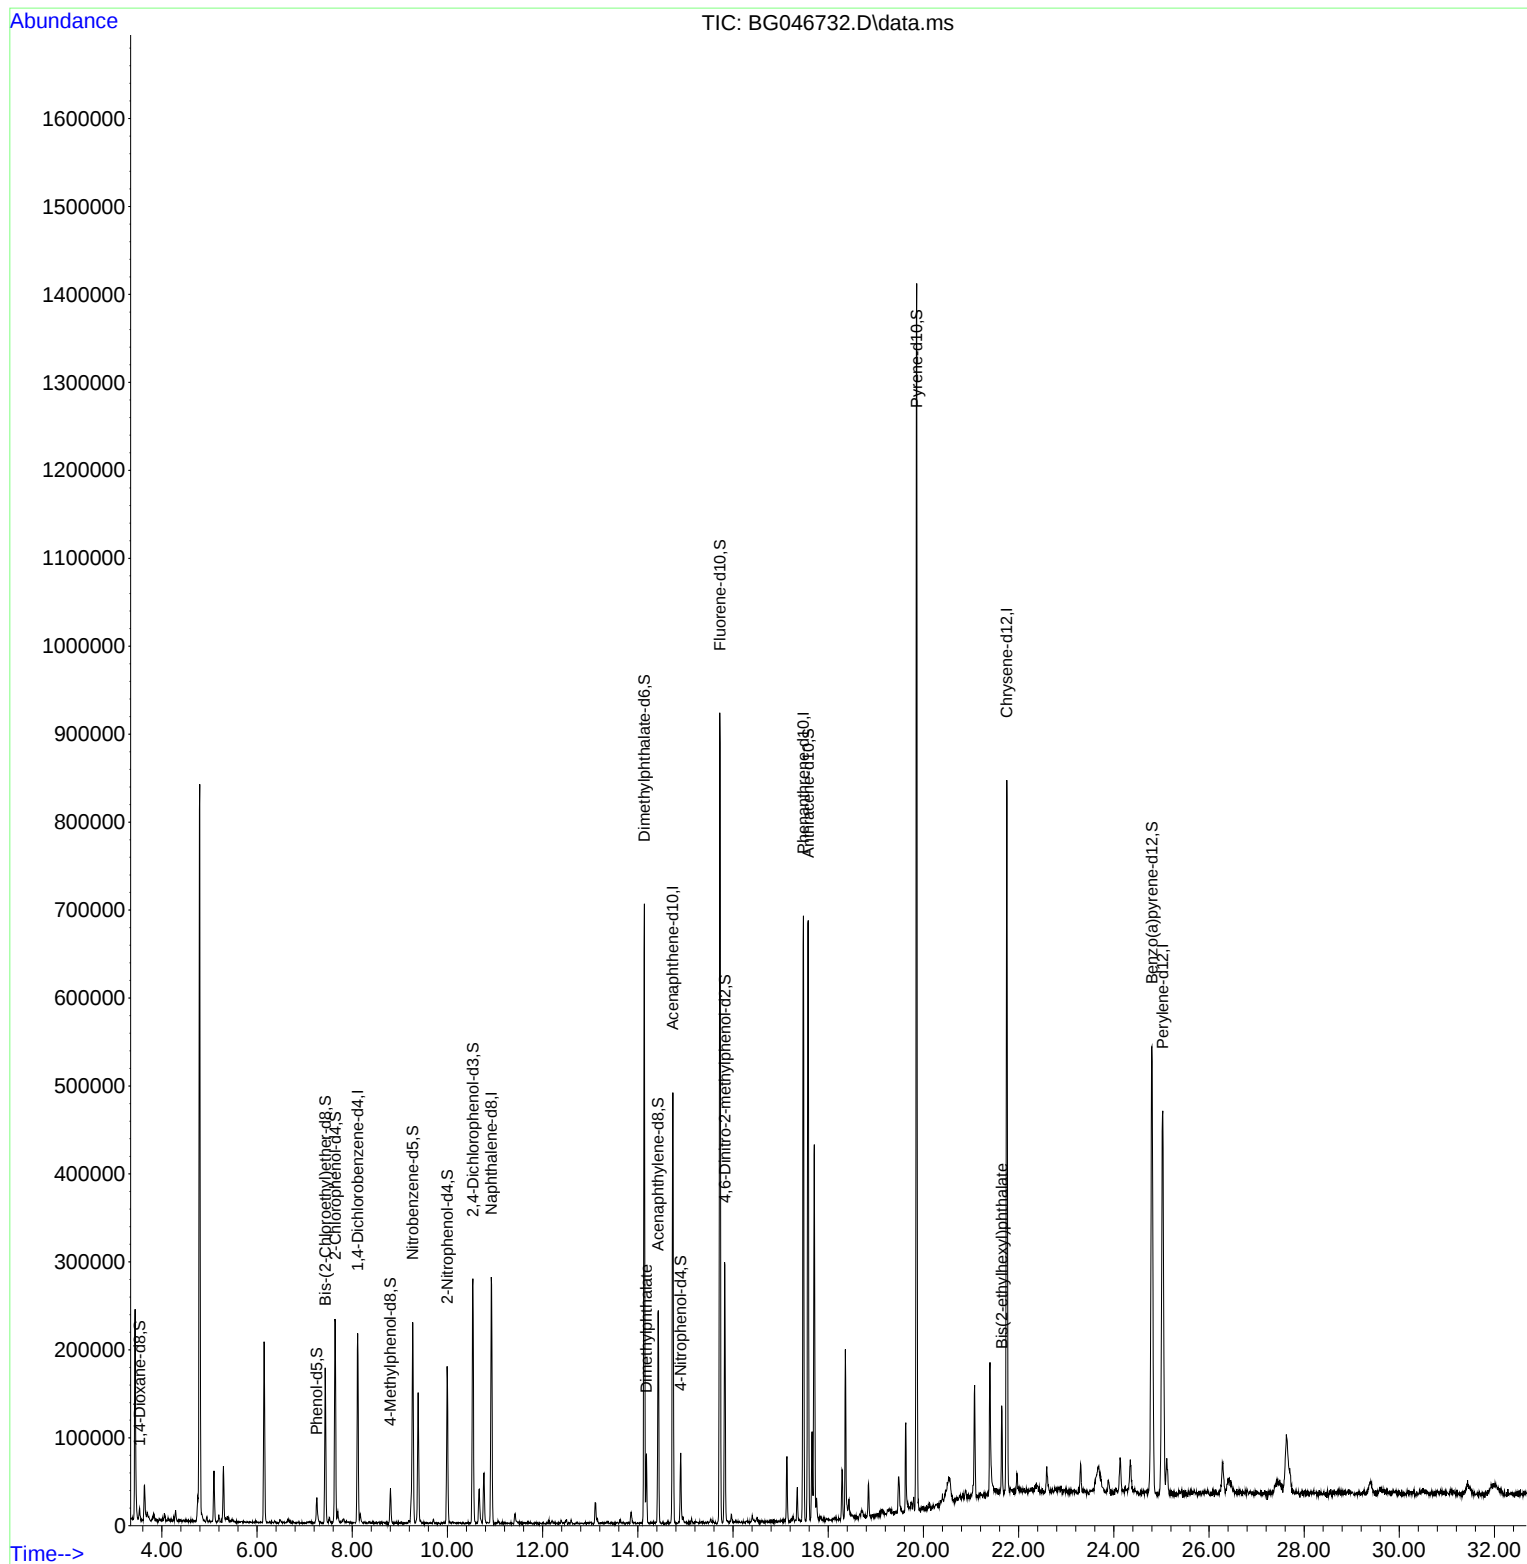


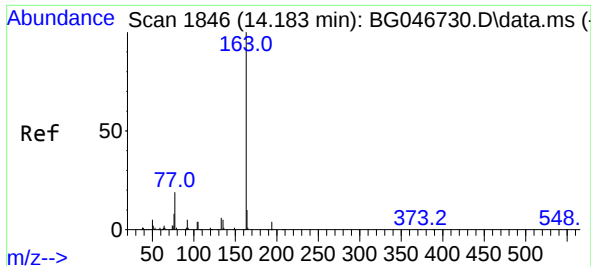

#45
Dimethylphthalate
Concen: 3.63 ng/ul
RT: 14.177 min Scan# 1845
Delta R.T. -0.006 min
Lab File: BG046732.D
Acq: 2 Oct 2020 11:20

Instrument :
BNA_G
ClientSampleId :
BG0Q8

Tgt Ion:163 Resp: 48940
Ion Ratio Lower Upper
163 100
194 5.2 3.6 5.4
164 9.3 7.4 11.0

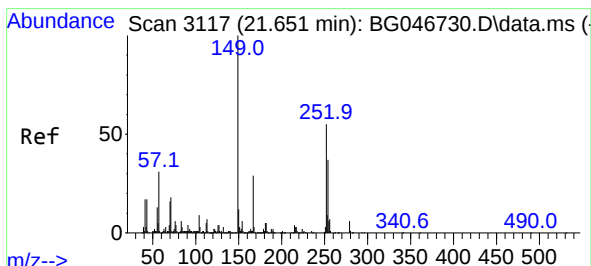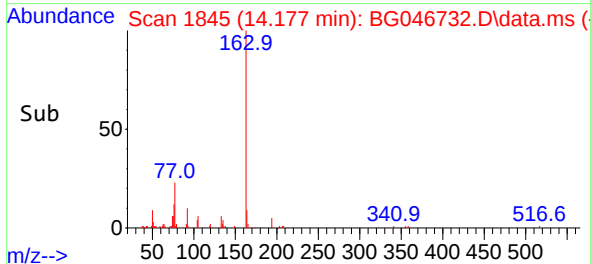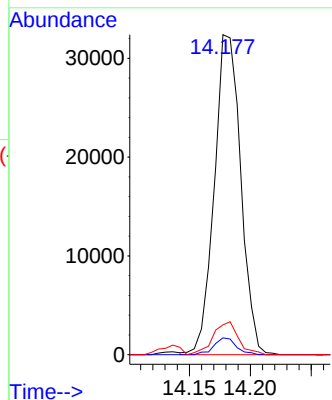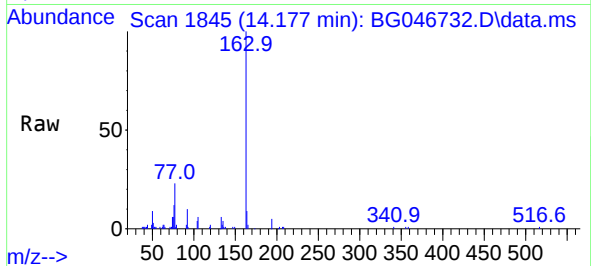

#84
Bis(2-ethylhexyl)phthalate
Concen: 2.30 ng/ul
RT: 21.651 min Scan# 3117
Delta R.T. -0.000 min
Lab File: BG046732.D
Acq: 2 Oct 2020 11:20

Tgt Ion:149 Resp: 39120
Ion Ratio Lower Upper
149 100
167 27.3 22.7 34.1
279 4.8 4.2 6.2

