

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046740.D
 Acq On : 2 Oct 2020 17:00
 Operator : CG/JU
 Sample : L4141-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0FG4

Quant Time: Oct 02 17:36:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 10:06:22 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.117	152	47528	20.00	ng/ul	0.00
18) Naphthalene-d8	10.926	136	178881	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.733	164	130861	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.477	188	321418	20.00	ng/ul	0.00
78) Chrysene-d12	21.748	240	396502	20.00	ng/ul	0.00
86) Perylene-d12	25.027	264	415084	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.534	96	5338	5.51	ng/uL	0.00
5) Phenol-d5	7.248	99	23161	5.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.430	67	76137	30.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.641	132	72809	24.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.799	113	44102	13.86	ng/ul	0.00
19) Nitrobenzene-d5	9.269	128	47353	35.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.997	143	51325	37.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.532	165	94223	29.43	ng/ul	0.00
29) 4-Chloroaniline-d4	11.049	131	6193	1.63	ng/ul	0.00
44) Dimethylphthalate-d6	14.134	166	347588	34.76	ng/ul	0.00
47) Acenaphthylene-d8	14.428	160	412021	34.70	ng/ul	0.00
52) 4-Nitrophenol-d4	14.898	143	10243	6.01	ng/ul	0.00
58) Fluorene-d10	15.726	176	321314	34.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.826	200	58164	36.22	ng/ul	0.00
71) Anthracene-d10	17.577	188	587332	39.83	ng/ul	0.00
79) Pyrene-d10	19.856	212	778463	37.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.804	264	884872	39.55	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	14.181	163	21834	2.16	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046740.D
Acq On : 2 Oct 2020 17:00
Operator : CG/JU
Sample : L4141-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FG4


Quant Time: Oct 02 17:36:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 10:06:22 2020
Response via : Initial Calibration

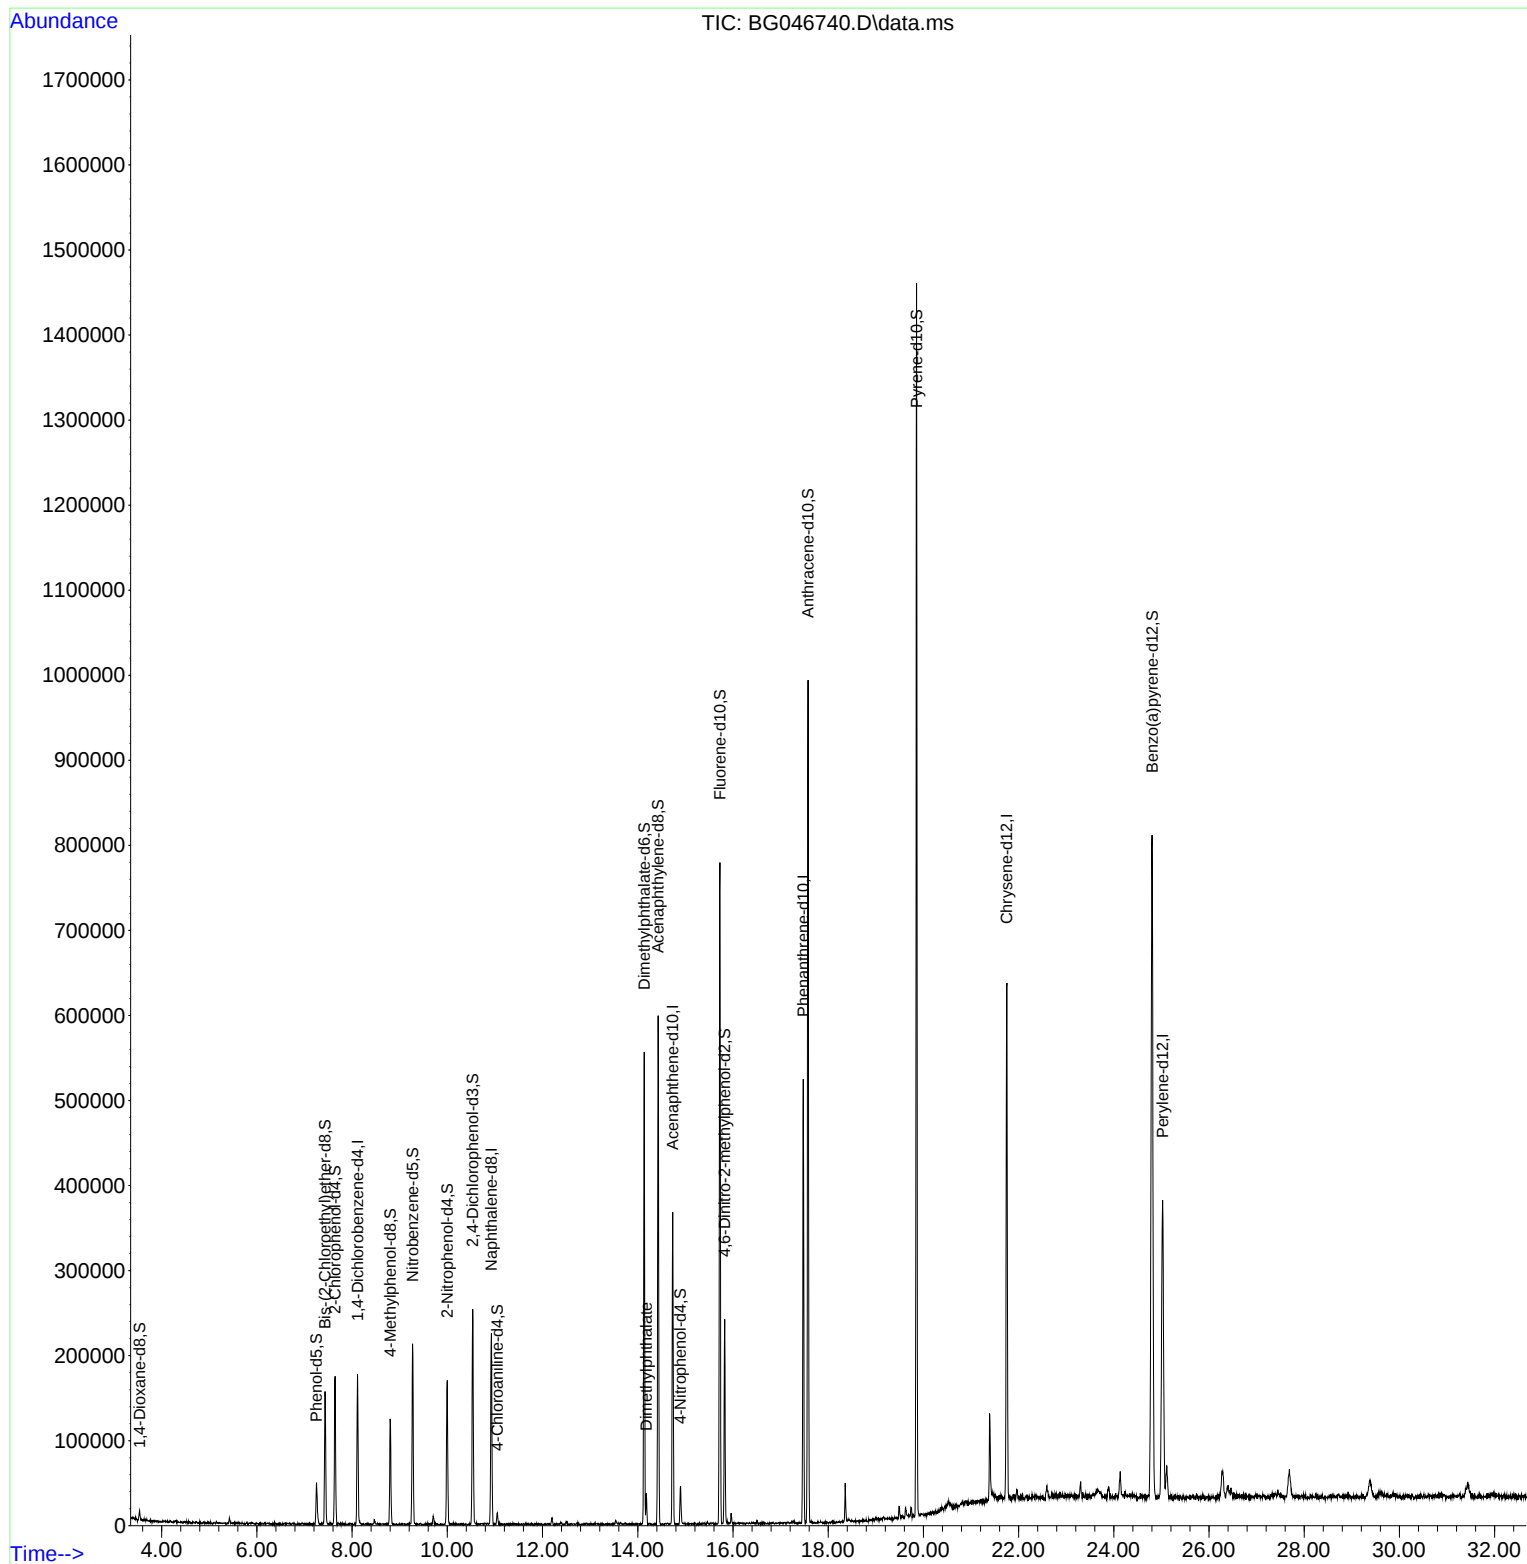

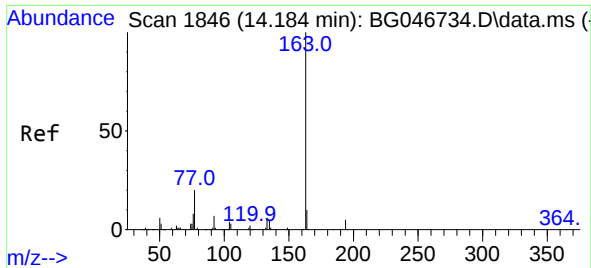

#45
 Dimethylphthalate
 Concen: 2.16 ng/ul
 RT: 14.181 min Scan# 1845
 Delta R.T. -0.003 min
 Lab File: BG046740.D
 Acq: 2 Oct 2020 17:00

Instrument :
 BNA_G
 ClientSampleId :
 C0FG4

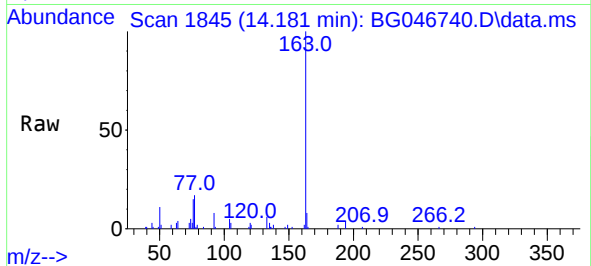

Tgt Ion:163 Resp: 21834

Ion	Ratio	Lower	Upper
163	100		
194	4.5	3.6	5.4
164	9.6	7.4	11.0

