

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046741.D
 Acq On : 2 Oct 2020 17:40
 Operator : CG/JU
 Sample : L4141-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0FG5

Quant Time: Oct 02 18:15:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 10:06:22 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	45716	20.00	ng/ul	0.00
18) Naphthalene-d8	10.923	136	188642	20.00	ng/ul	# 0.00
36) Acenaphthene-d10	14.736	164	132915	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.480	188	339214	20.00	ng/ul	0.00
78) Chrysene-d12	21.751	240	412827	20.00	ng/ul	0.00
86) Perylene-d12	25.024	264	424387	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.537	96	6161	6.62	ng/uL	0.00
5) Phenol-d5	7.256	99	27527	7.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.433	67	82590	34.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.638	132	79663	27.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.802	113	50314	16.44	ng/ul	0.00
19) Nitrobenzene-d5	9.272	128	51981	36.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.994	143	55064	38.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.535	165	101687	30.12	ng/ul	0.00
29) 4-Chloroaniline-d4	11.052	131	7450	1.86	ng/ul	0.00
44) Dimethylphthalate-d6	14.137	166	399649	39.35	ng/ul	0.00
47) Acenaphthylene-d8	14.430	160	455992	37.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.900	143	12516	7.23	ng/ul	0.00
58) Fluorene-d10	15.723	176	360874	38.54	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.823	200	66857	39.45	ng/ul	0.00
71) Anthracene-d10	17.574	188	652484	41.92	ng/ul	0.00
79) Pyrene-d10	19.853	212	852770	39.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.800	264	928256	40.58	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	14.178	163	16423	1.60	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046741.D
Acq On : 2 Oct 2020 17:40
Operator : CG/JU
Sample : L4141-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0FG5


Quant Time: Oct 02 18:15:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 10:06:22 2020
Response via : Initial Calibration

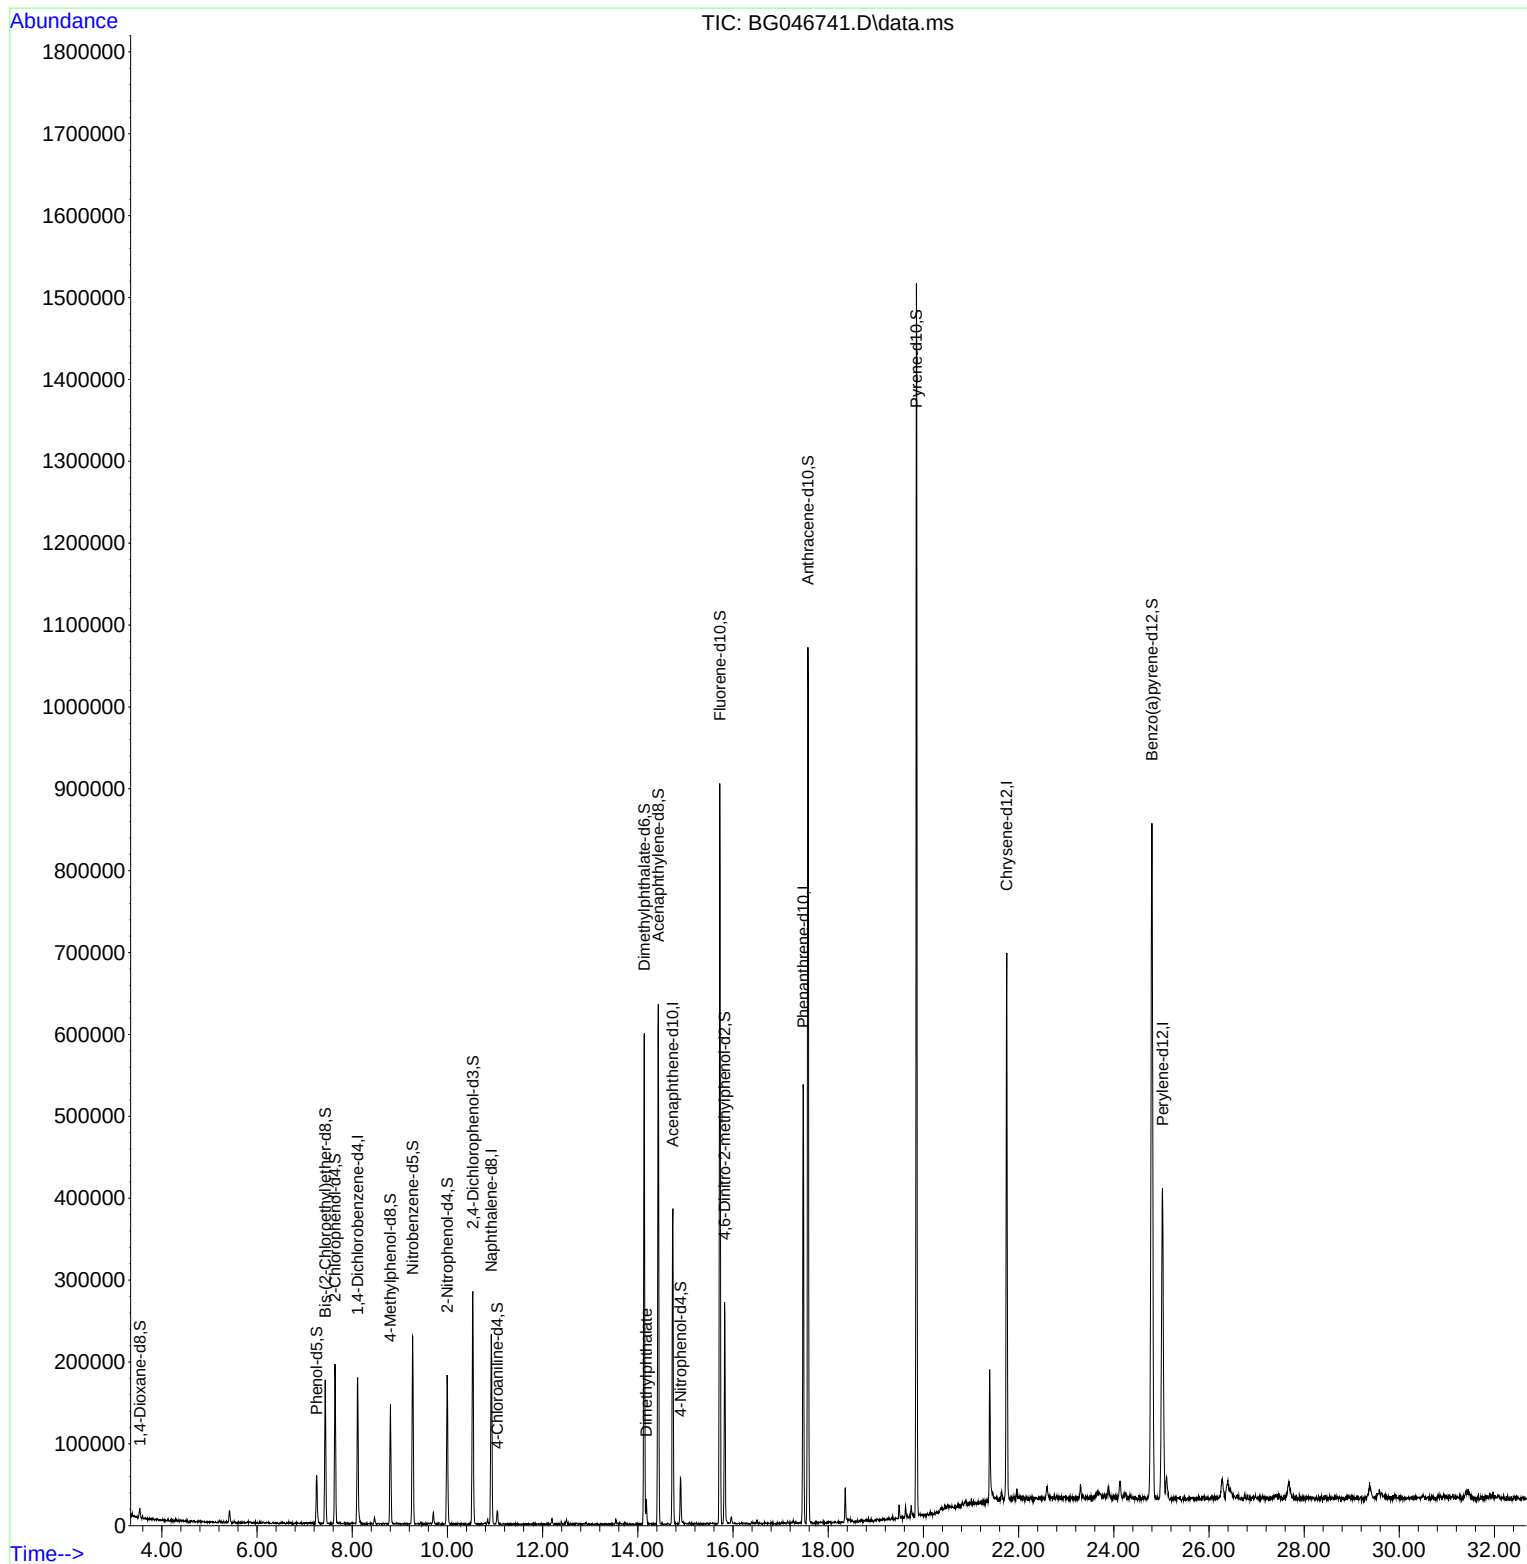

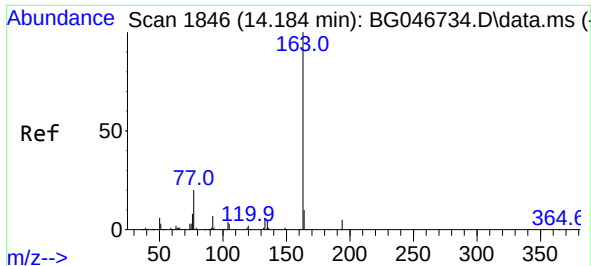

#45
Dimethylphthalate
Concen: 1.60 ng/ul
RT: 14.178 min Scan# 1845
Delta R.T. -0.006 min
Lab File: BG046741.D
Acq: 2 Oct 2020 17:40

Instrument :
BNA_G
ClientSampleId :
C0FG5

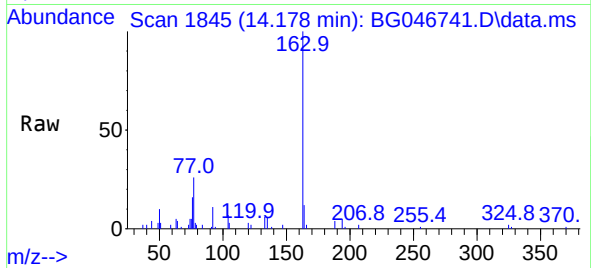

Tgt Ion	Ratio	Lower	Upper
163	100		
194	5.0	3.6	5.4
164	12.3	7.4	11.0#

