

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046756.D
 Acq On : 3 Oct 2020 4:26
 Operator : CG/JU
 Sample : L4151-16
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7L7

Quant Time: Oct 03 06:12:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 03:57:33 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.114	152	72960	20.00	ng/ul	0.00
18) Naphthalene-d8	10.923	136	303592	20.00	ng/ul	# 0.00
36) Acenaphthene-d10	14.730	164	231976	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.474	188	550416	20.00	ng/ul	0.00
78) Chrysene-d12	21.751	240	534730	20.00	ng/ul	0.00
86) Perylene-d12	25.024	264	550351	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.532	96	5640	3.79	ng/uL	0.00
5) Phenol-d5	7.257	99	120054	19.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.433	67	71610	18.80	ng/ul	0.00
9) 2-Chlorophenol-d4	7.639	132	86690	19.02	ng/ul	0.00
13) 4-Methylphenol-d8	8.802	113	90945	18.62	ng/ul	0.00
19) Nitrobenzene-d5	9.272	128	46517	20.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.995	143	54223	23.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.529	165	102874	18.93	ng/ul	0.00
29) 4-Chloroaniline-d4	11.046	131	78041	12.09	ng/ul	0.00
44) Dimethylphthalate-d6	14.131	166	339921	19.18	ng/ul	0.00
47) Acenaphthylene-d8	14.425	160	392948	18.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.901	143	57069	18.89	ng/ul	0.00
58) Fluorene-d10	15.723	176	305286	18.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.823	200	50046	18.20	ng/ul	0.00
71) Anthracene-d10	17.574	188	441353	17.48	ng/ul	0.00
79) Pyrene-d10	19.854	212	519800	18.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.795	264	498198	16.80	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	14.178	163	34142	1.90	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046756.D
Acq On : 3 Oct 2020 4:26
Operator : CG/JU
Sample : L4151-16
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7L7


Quant Time: Oct 03 06:12:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 03:57:33 2020
Response via : Initial Calibration

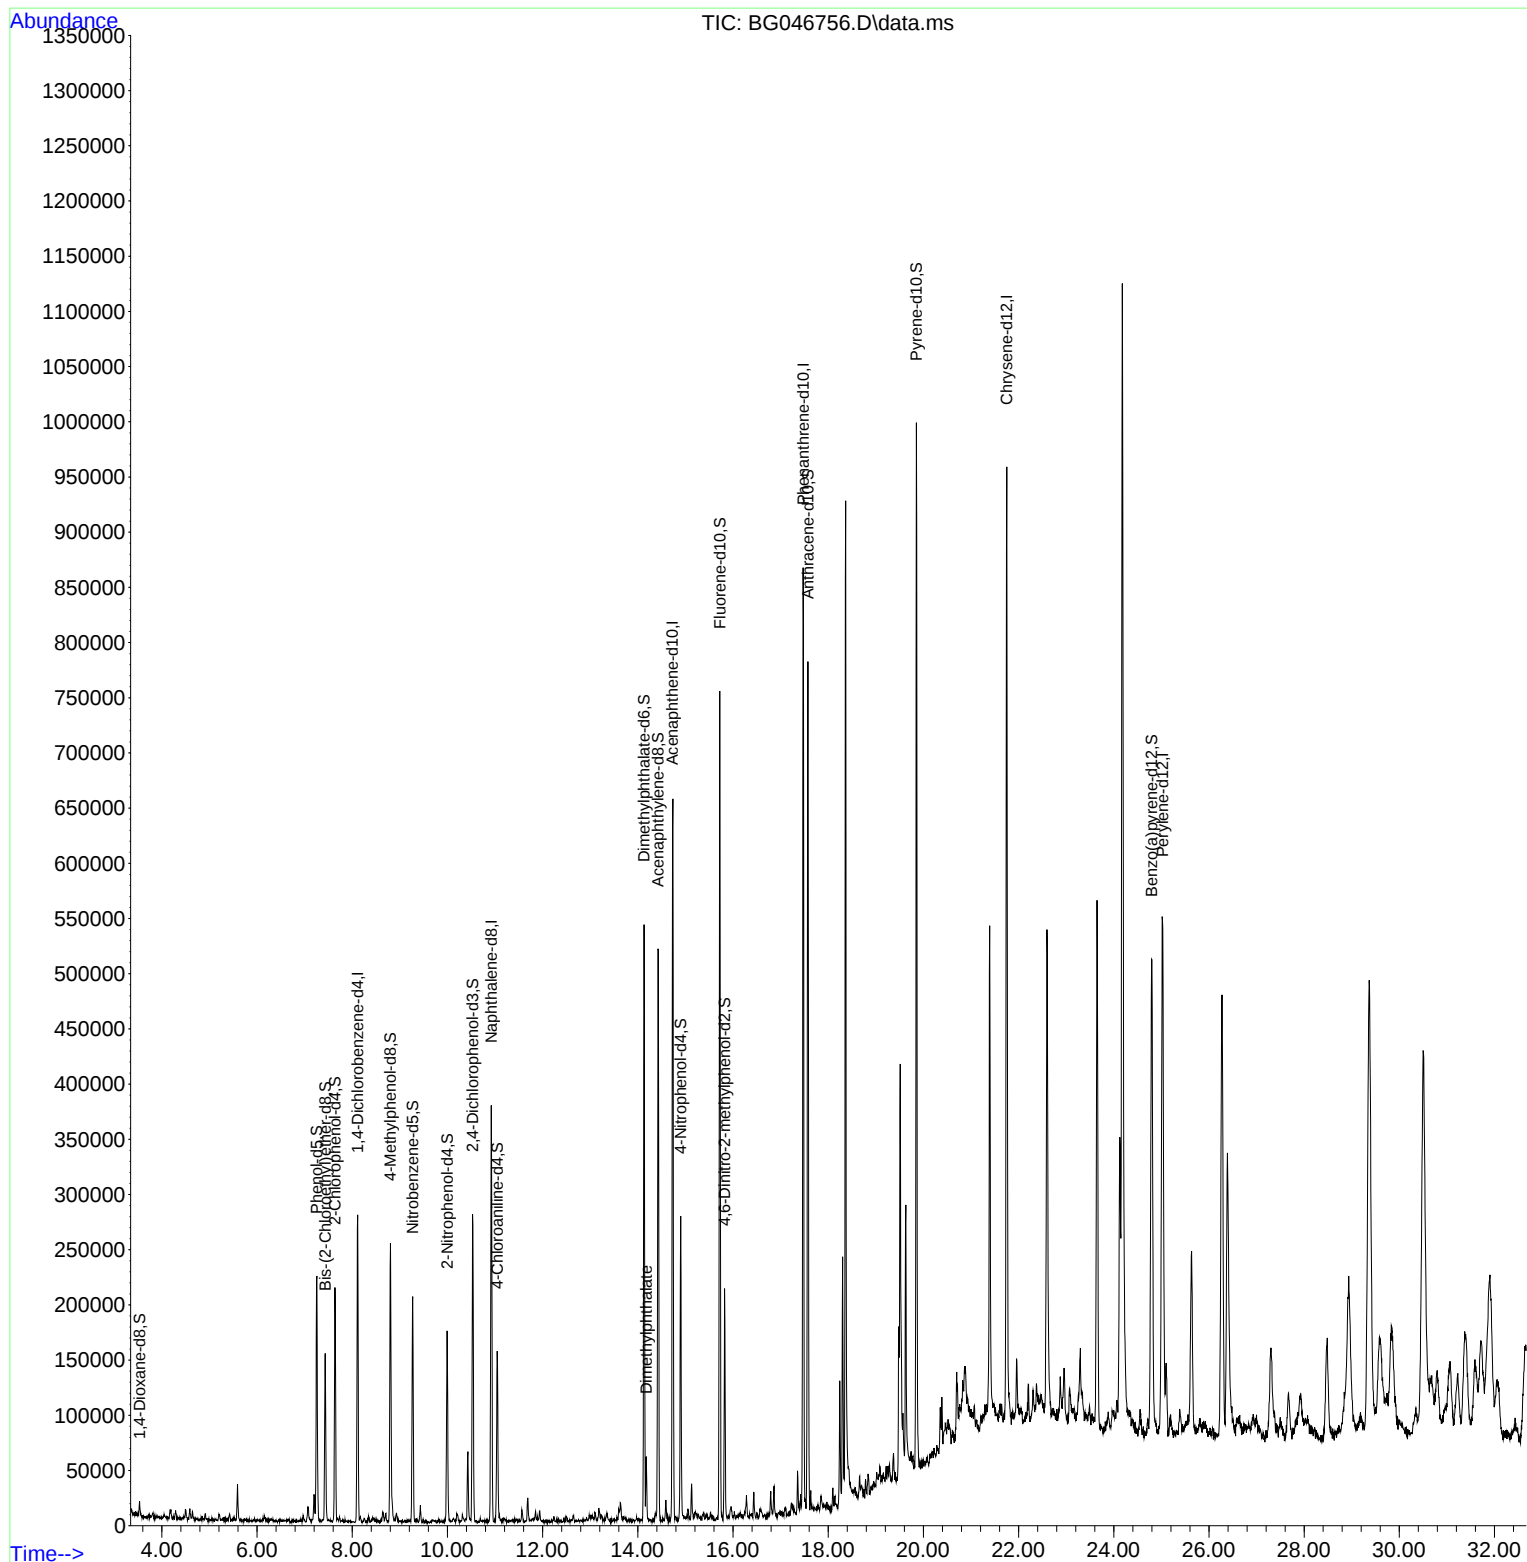

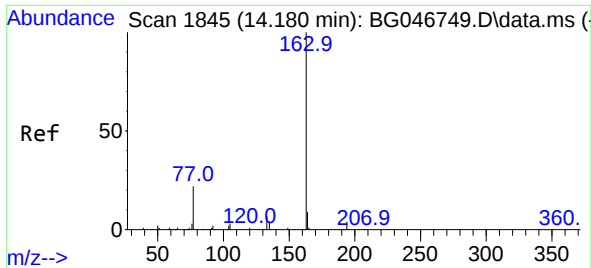

#45
Dimethylphthalate
Concen: 1.90 ng/ul
RT: 14.178 min Scan# 1845
Delta R.T. -0.006 min
Lab File: BG046756.D
Acq: 3 Oct 2020 4:26

Instrument :
BNA_G
ClientSampleId :
CB7L7

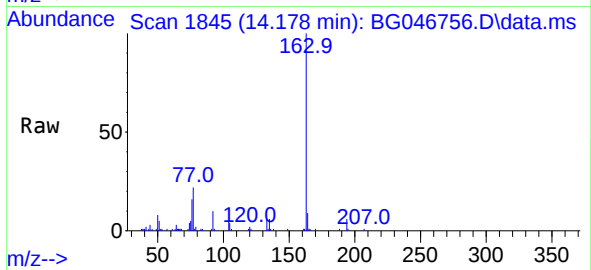

Tgt Ion:	163	Resp:	34142
Ion	Ratio	Lower	Upper
163	100		
194	5.8	3.6	5.4#
164	8.6	7.4	11.0

