

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046759.D
 Acq On : 3 Oct 2020 6:28
 Operator : CG/JU
 Sample : L4151-13
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7L4

Quant Time: Oct 03 07:22:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 03 03:57:33 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.115	152	80883	20.00	ng/ul	0.00
18) Naphthalene-d8	10.923	136	337300	20.00	ng/ul #	0.00
36) Acenaphthene-d10	14.736	164	245395	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.474	188	549025	20.00	ng/ul	0.00
78) Chrysene-d12	21.752	240	548788	20.00	ng/ul	0.00
86) Perylene-d12	25.024	264	577032	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.532	96	6891	4.18	ng/uL	0.00
5) Phenol-d5	7.257	99	150709	21.77	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.427	67	94105	22.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.639	132	115845	22.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.808	113	123761	22.86	ng/ul	0.00
19) Nitrobenzene-d5	9.272	128	59590	23.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.995	143	71906	28.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.535	165	132485	21.95	ng/ul	0.00
29) 4-Chloroaniline-d4	11.047	131	111698	15.57	ng/ul	0.00
44) Dimethylphthalate-d6	14.131	166	446174	23.80	ng/ul	0.00
47) Acenaphthylene-d8	14.425	160	500529	22.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.901	143	76348	23.88	ng/ul	0.00
58) Fluorene-d10	15.723	176	380301	22.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.829	200	61822	22.54	ng/ul	0.00
71) Anthracene-d10	17.574	188	548845	21.79	ng/ul	0.00
79) Pyrene-d10	19.854	212	620528	21.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.801	264	632367	20.33	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	14.178	163	63922	3.37	ng/ul#	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046759.D
Acq On : 3 Oct 2020 6:28
Operator : CG/JU
Sample : L4151-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7L4


Quant Time: Oct 03 07:22:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 03 03:57:33 2020
Response via : Initial Calibration

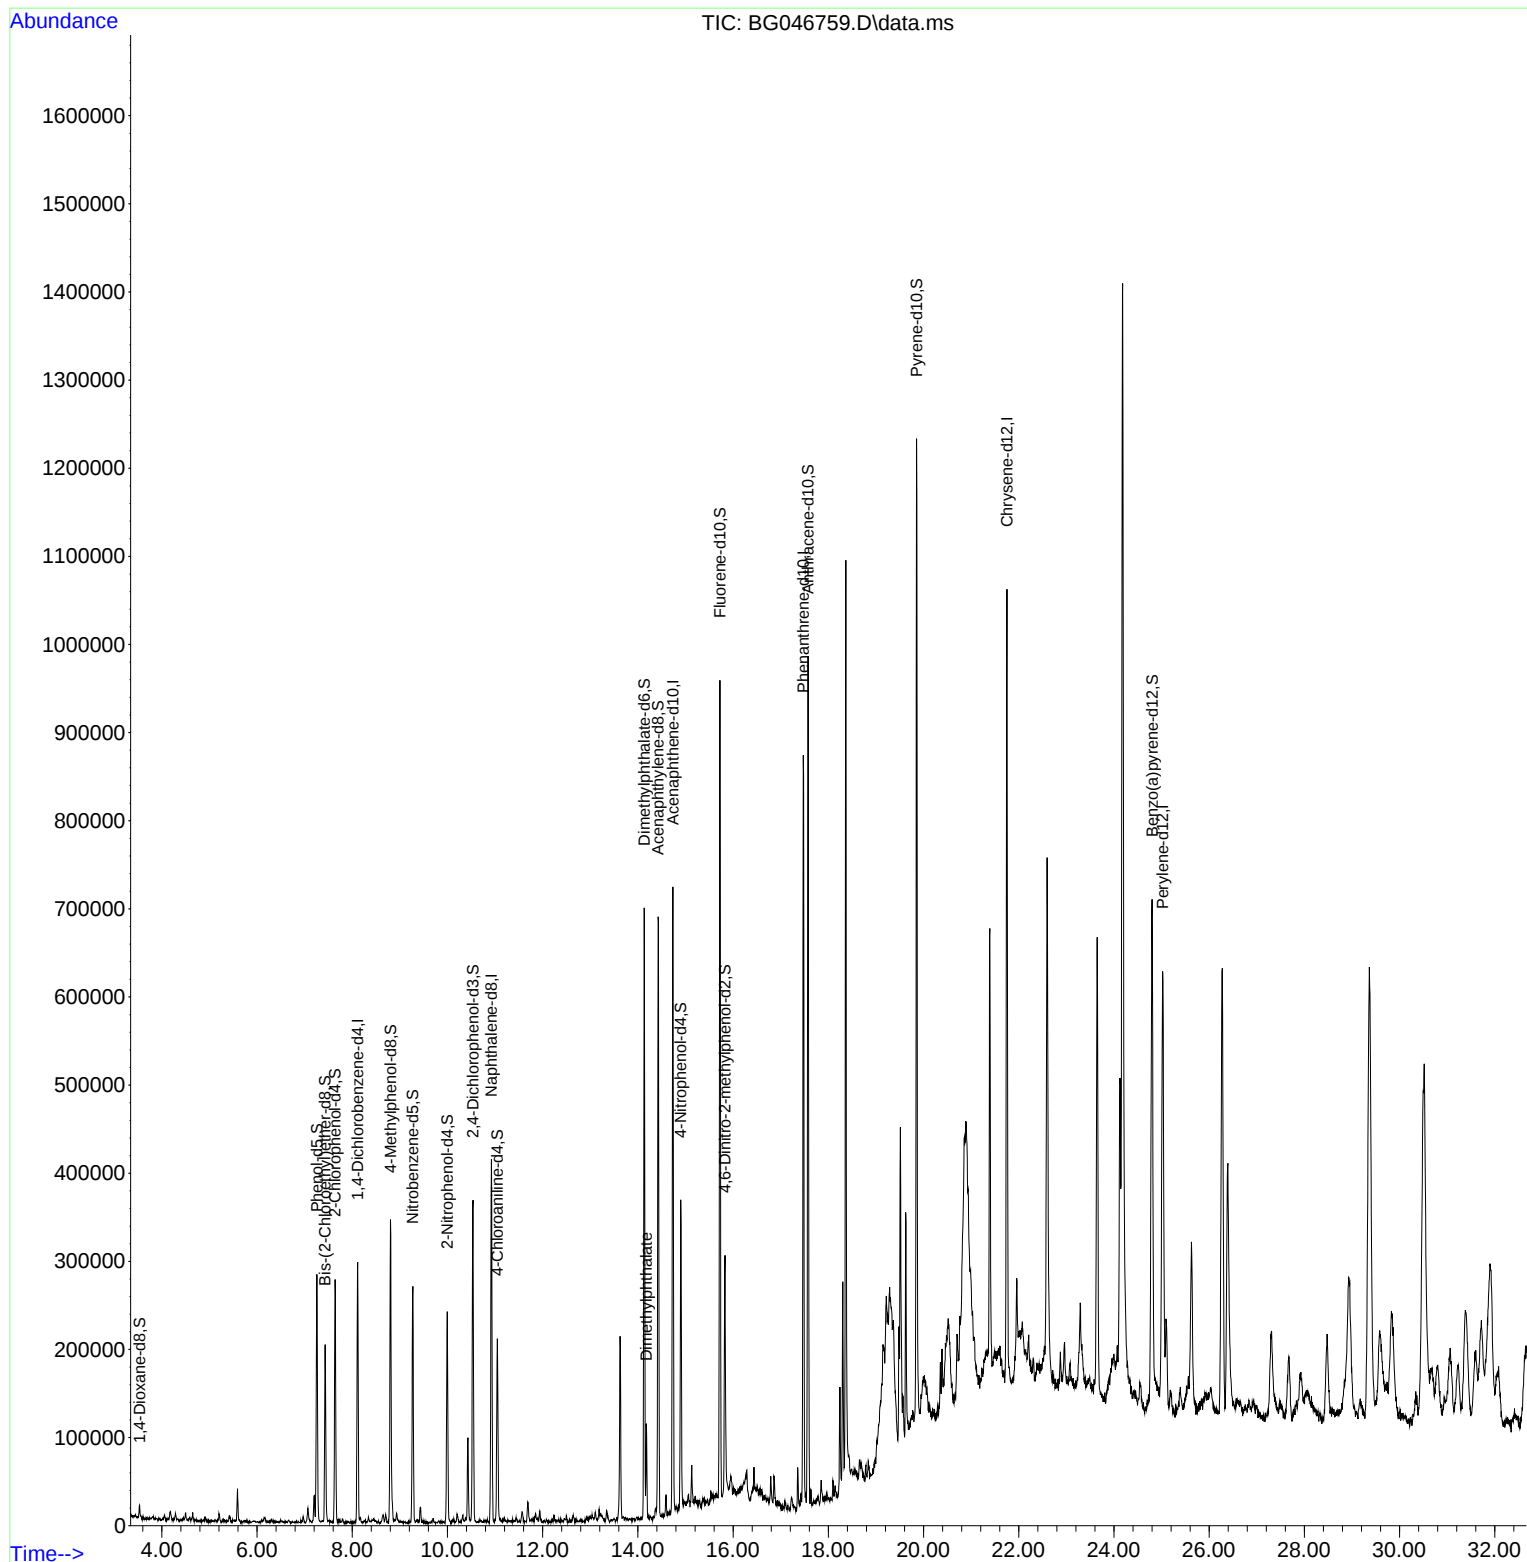

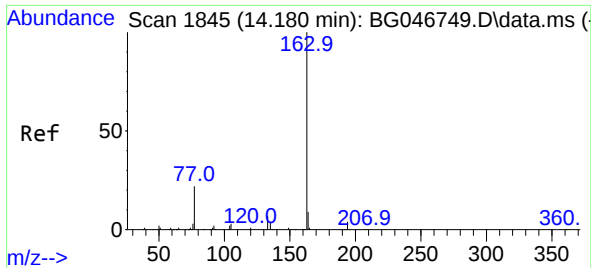

#45
Dimethylphthalate
Concen: 3.37 ng/ul
RT: 14.178 min Scan# 1845
Delta R.T. -0.005 min
Lab File: BG046759.D
Acq: 3 Oct 2020 6:28

Instrument :
BNA_G
ClientSampleId :
CB7L4

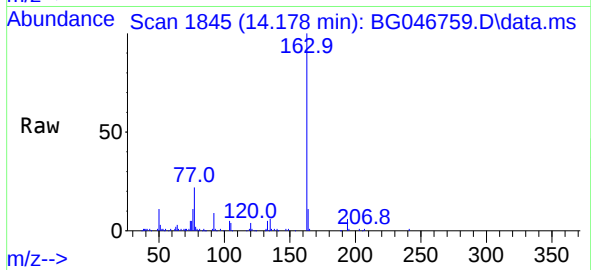

Tgt Ion:163 Resp: 63922
Ion Ratio Lower Upper
163 100
194 5.7 3.6 5.4#
164 10.5 7.4 11.0

