

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046760.D
 Acq On : 3 Oct 2020 7:08
 Operator : CG/JU
 Sample : L4150-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7H9

Quant Time: Oct 05 00:06:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 10:06:22 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.110	152	76979	20.00	ng/ul	0.00
18) Naphthalene-d8	10.925	136	311193	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.732	164	231996	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.476	188	546420	20.00	ng/ul	0.00
78) Chrysene-d12	21.753	240	528199	20.00	ng/ul	0.00
86) Perylene-d12	25.032	264	555029	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.533	96	13016	8.30	ng/uL	0.00
5) Phenol-d5	7.258	99	295512	44.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.435	67	166872	41.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.640	132	215360	44.78	ng/ul	0.00
13) 4-Methylphenol-d8	8.804	113	233798	45.38	ng/ul	0.00
19) Nitrobenzene-d5	9.274	128	111011	47.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.996	143	130141	54.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.531	165	248391	44.60	ng/ul	0.00
29) 4-Chloroaniline-d4	11.048	131	235167	35.53	ng/ul	0.00
44) Dimethylphthalate-d6	14.133	166	768607	43.36	ng/ul	0.00
47) Acenaphthylene-d8	14.426	160	940361	44.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.908	143	146049	48.33	ng/ul	0.00
58) Fluorene-d10	15.725	176	708923	43.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.831	200	121561	44.52	ng/ul	0.00
71) Anthracene-d10	17.576	188	1084802	43.27	ng/ul	0.00
79) Pyrene-d10	19.855	212	1215892	44.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.802	264	1253557	41.90	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	14.180	163	74442	4.15	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046760.D
Acq On : 3 Oct 2020 7:08
Operator : CG/JU
Sample : L4150-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7H9


Quant Time: Oct 05 00:06:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 10:06:22 2020
Response via : Initial Calibration

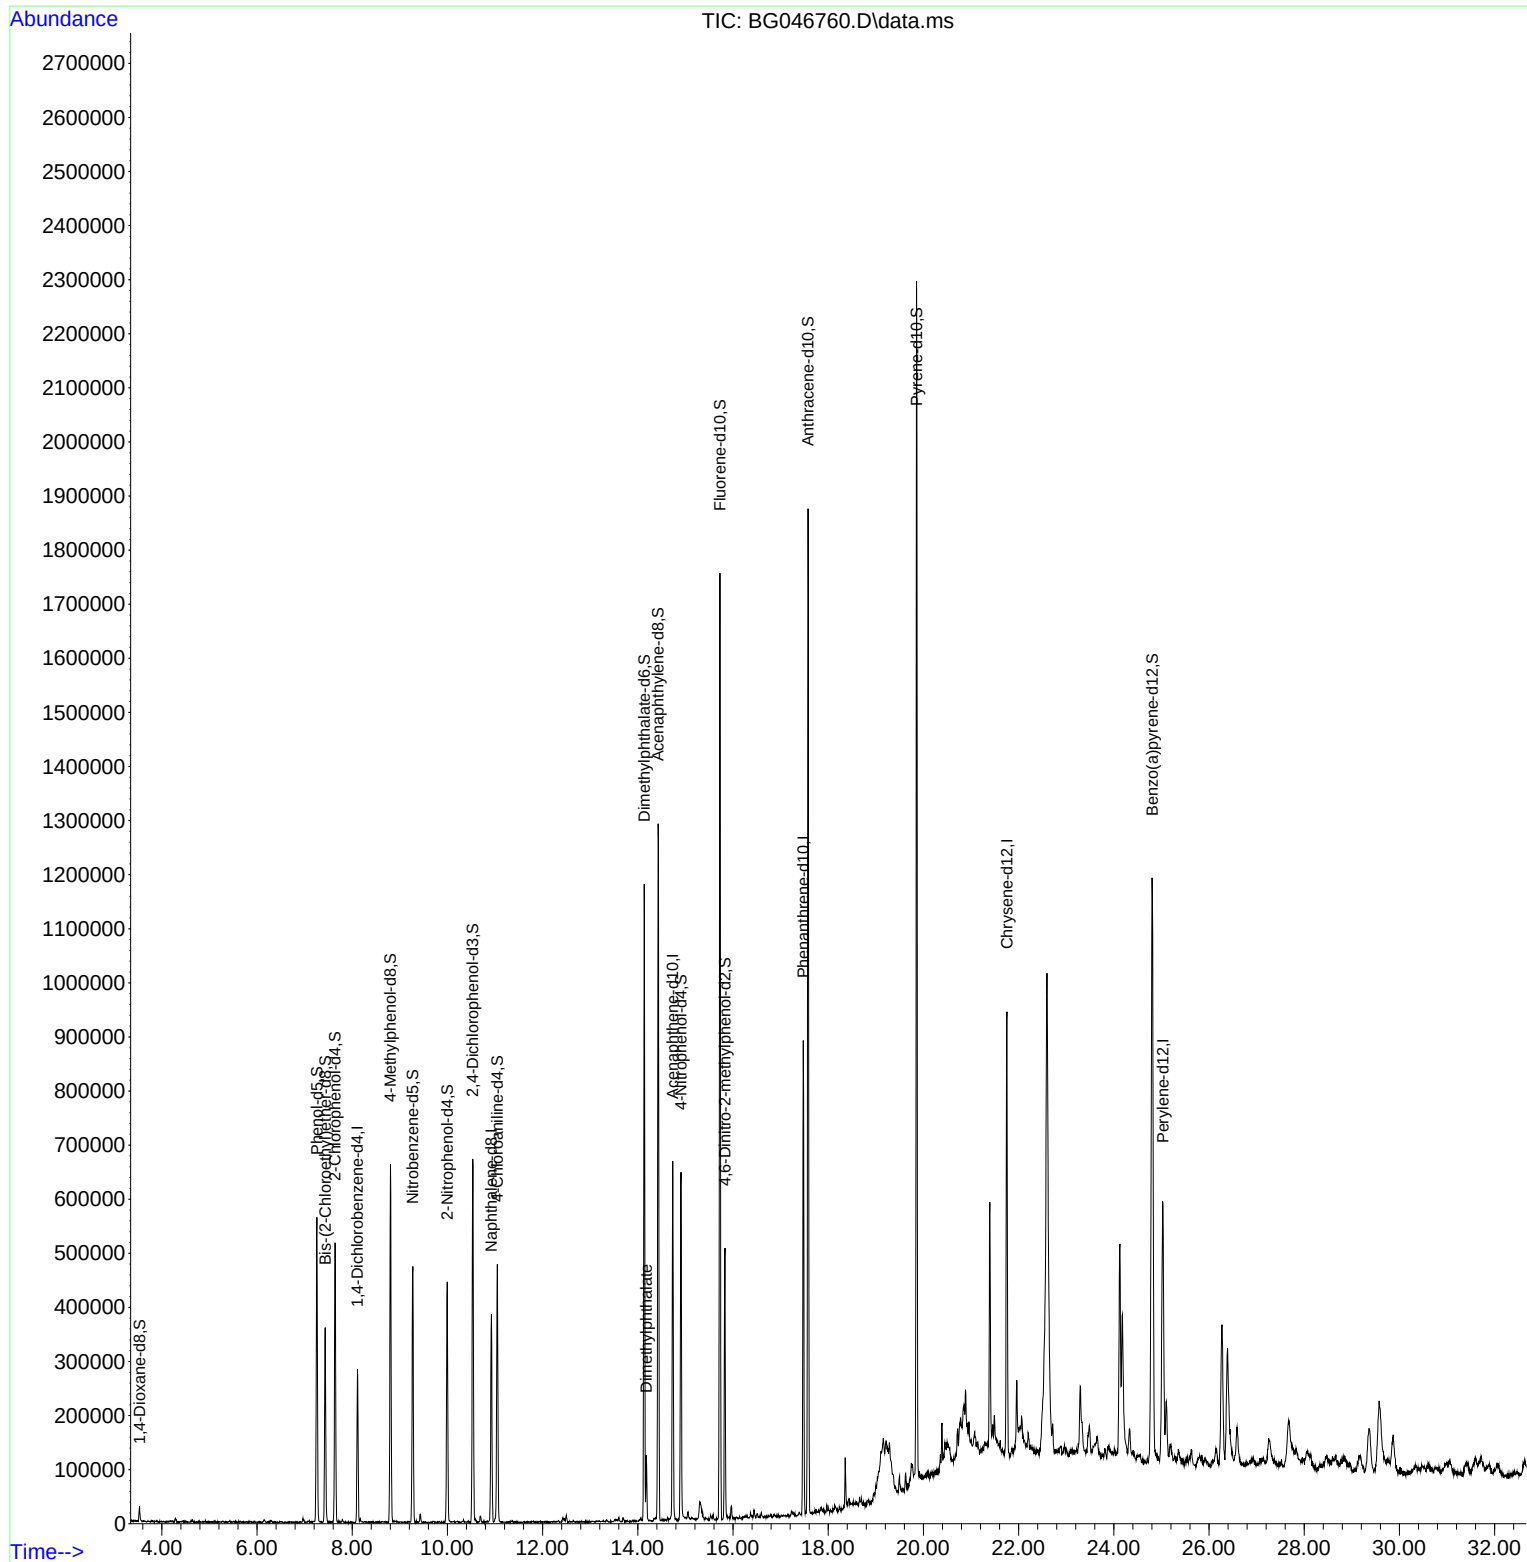

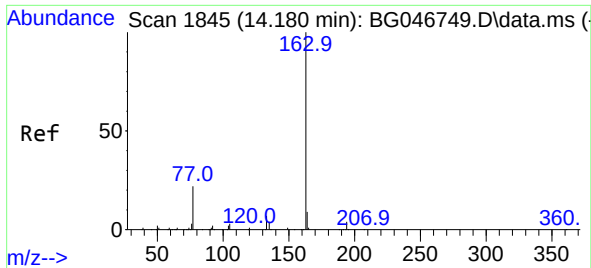

#45
Dimethylphthalate
Concen: 4.15 ng/ul
RT: 14.180 min Scan# 1845
Delta R.T. -0.004 min
Lab File: BG046760.D
Acq: 3 Oct 2020 7:08

Instrument :
BNA_G
ClientSampleId :
CB7H9

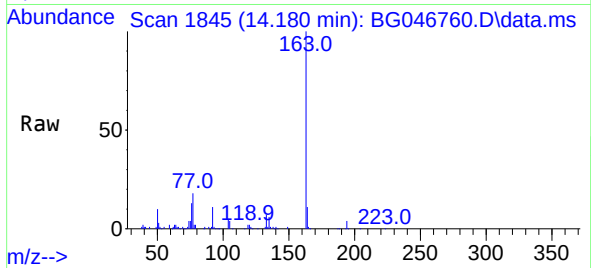

Tgt Ion:163 Resp: 74442
Ion Ratio Lower Upper
163 100
194 4.1 3.6 5.4
164 11.4 7.4 11.0#

