

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046761.D
 Acq On : 3 Oct 2020 7:48
 Operator : CG/JU
 Sample : L4150-04
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7J0

Quant Time: Oct 05 00:06:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 02 10:06:22 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.111	152	76869	20.00	ng/ul	0.00
18) Naphthalene-d8	10.925	136	313996	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.733	164	224326	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.476	188	531789	20.00	ng/ul	0.00
78) Chrysene-d12	21.754	240	527544	20.00	ng/ul	0.00
86) Perylene-d12	25.026	264	546813	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.534	96	15453	9.87	ng/uL	0.00
5) Phenol-d5	7.259	99	327490	49.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.435	67	187768	46.78	ng/ul	0.00
9) 2-Chlorophenol-d4	7.641	132	242128	50.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.804	113	264033	51.32	ng/ul	0.00
19) Nitrobenzene-d5	9.268	128	123396	52.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.997	143	145476	60.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.538	165	276862	49.27	ng/ul	0.00
29) 4-Chloroaniline-d4	11.049	131	262010	39.23	ng/ul	0.00
44) Dimethylphthalate-d6	14.133	166	827526	48.28	ng/ul	0.00
47) Acenaphthylene-d8	14.427	160	1021371	50.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.909	143	156985	53.72	ng/ul	0.00
58) Fluorene-d10	15.726	176	769596	48.70	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.831	200	133979	50.42	ng/ul	0.00
71) Anthracene-d10	17.576	188	1174965	48.16	ng/ul	0.00
79) Pyrene-d10	19.856	212	1369850	50.04	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.809	264	1383571	46.94	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	14.180	163	95180	5.49	ng/ul#	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046761.D
Acq On : 3 Oct 2020 7:48
Operator : CG/JU
Sample : L4150-04
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7J0


Quant Time: Oct 05 00:06:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 02 10:06:22 2020
Response via : Initial Calibration

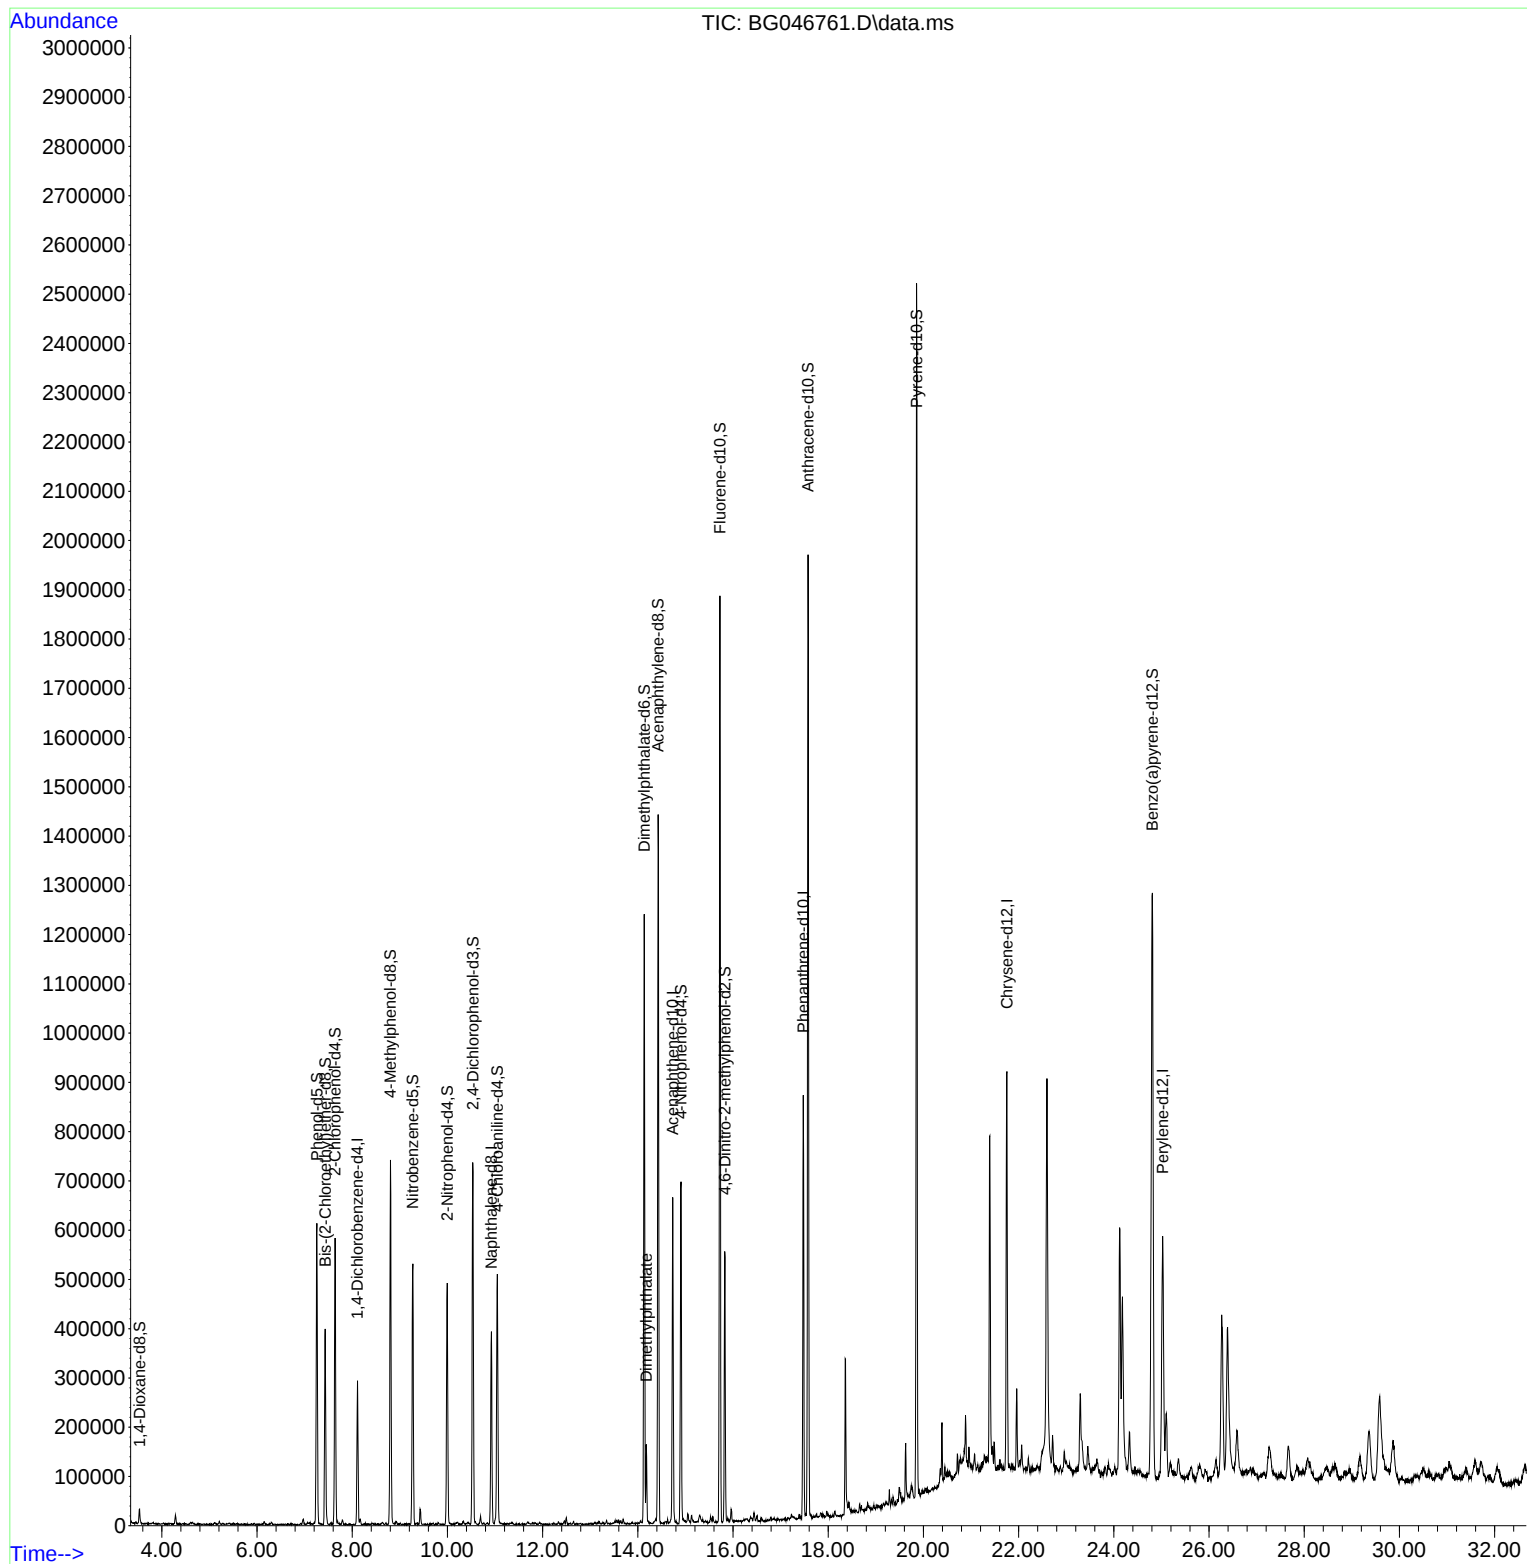

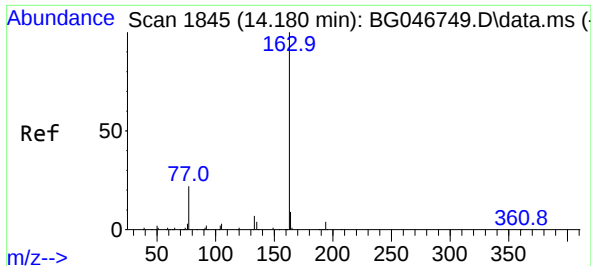

#45
Dimethylphthalate
Concen: 5.49 ng/ul
RT: 14.180 min Scan# 1845
Delta R.T. -0.003 min
Lab File: BG046761.D
Acq: 3 Oct 2020 7:48

Instrument :
BNA_G
ClientSampleId :
CB7J0

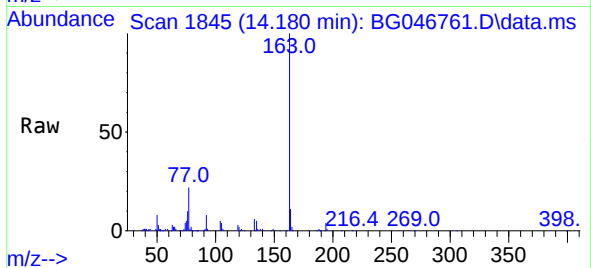

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.6	5.4
164	11.2	7.4	11.0#

