

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046771.D
 Acq On : 3 Oct 2020 14:30
 Operator : CG/JU
 Sample : L4150-21
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7M2

Quant Time: Oct 05 00:59:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 00:58:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.109	152	74424	20.00	ng/ul	0.00
18) Naphthalene-d8	10.923	136	305814	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.737	164	226908	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.475	188	512540	20.00	ng/ul	0.00
78) Chrysene-d12	21.752	240	497172	20.00	ng/ul	0.00
86) Perylene-d12	25.025	264	496773	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.526	96	4641	3.06	ng/uL	0.00
5) Phenol-d5	7.257	99	119612	18.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.428	67	73816	19.00	ng/ul	0.00
9) 2-Chlorophenol-d4	7.639	132	93416	20.09	ng/ul	0.00
13) 4-Methylphenol-d8	8.802	113	101761	20.43	ng/ul	0.00
19) Nitrobenzene-d5	9.272	128	49507	21.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.995	143	56297	24.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.530	165	107056	19.56	ng/ul	0.00
29) 4-Chloroaniline-d4	11.047	131	103256	15.88	ng/ul	0.00
44) Dimethylphthalate-d6	14.131	166	363380	20.96	ng/ul	0.00
47) Acenaphthylene-d8	14.425	160	415397	20.18	ng/ul	0.00
52) 4-Nitrophenol-d4	14.901	143	62256	21.06	ng/ul	0.00
58) Fluorene-d10	15.724	176	317056	19.83	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.829	200	45179	17.64	ng/ul	0.00
71) Anthracene-d10	17.575	188	460952	19.60	ng/ul	0.00
79) Pyrene-d10	19.854	212	535508	20.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.795	264	525806	19.64	ng/ul	0.00
Target Compounds						
14) Acetophenone	8.932	105	9613	1.19	ng/ul	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046771.D
Acq On : 3 Oct 2020 14:30
Operator : CG/JU
Sample : L4150-21
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7M2

Quant Time: Oct 05 00:59:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 00:58:20 2020
Response via : Initial Calibration

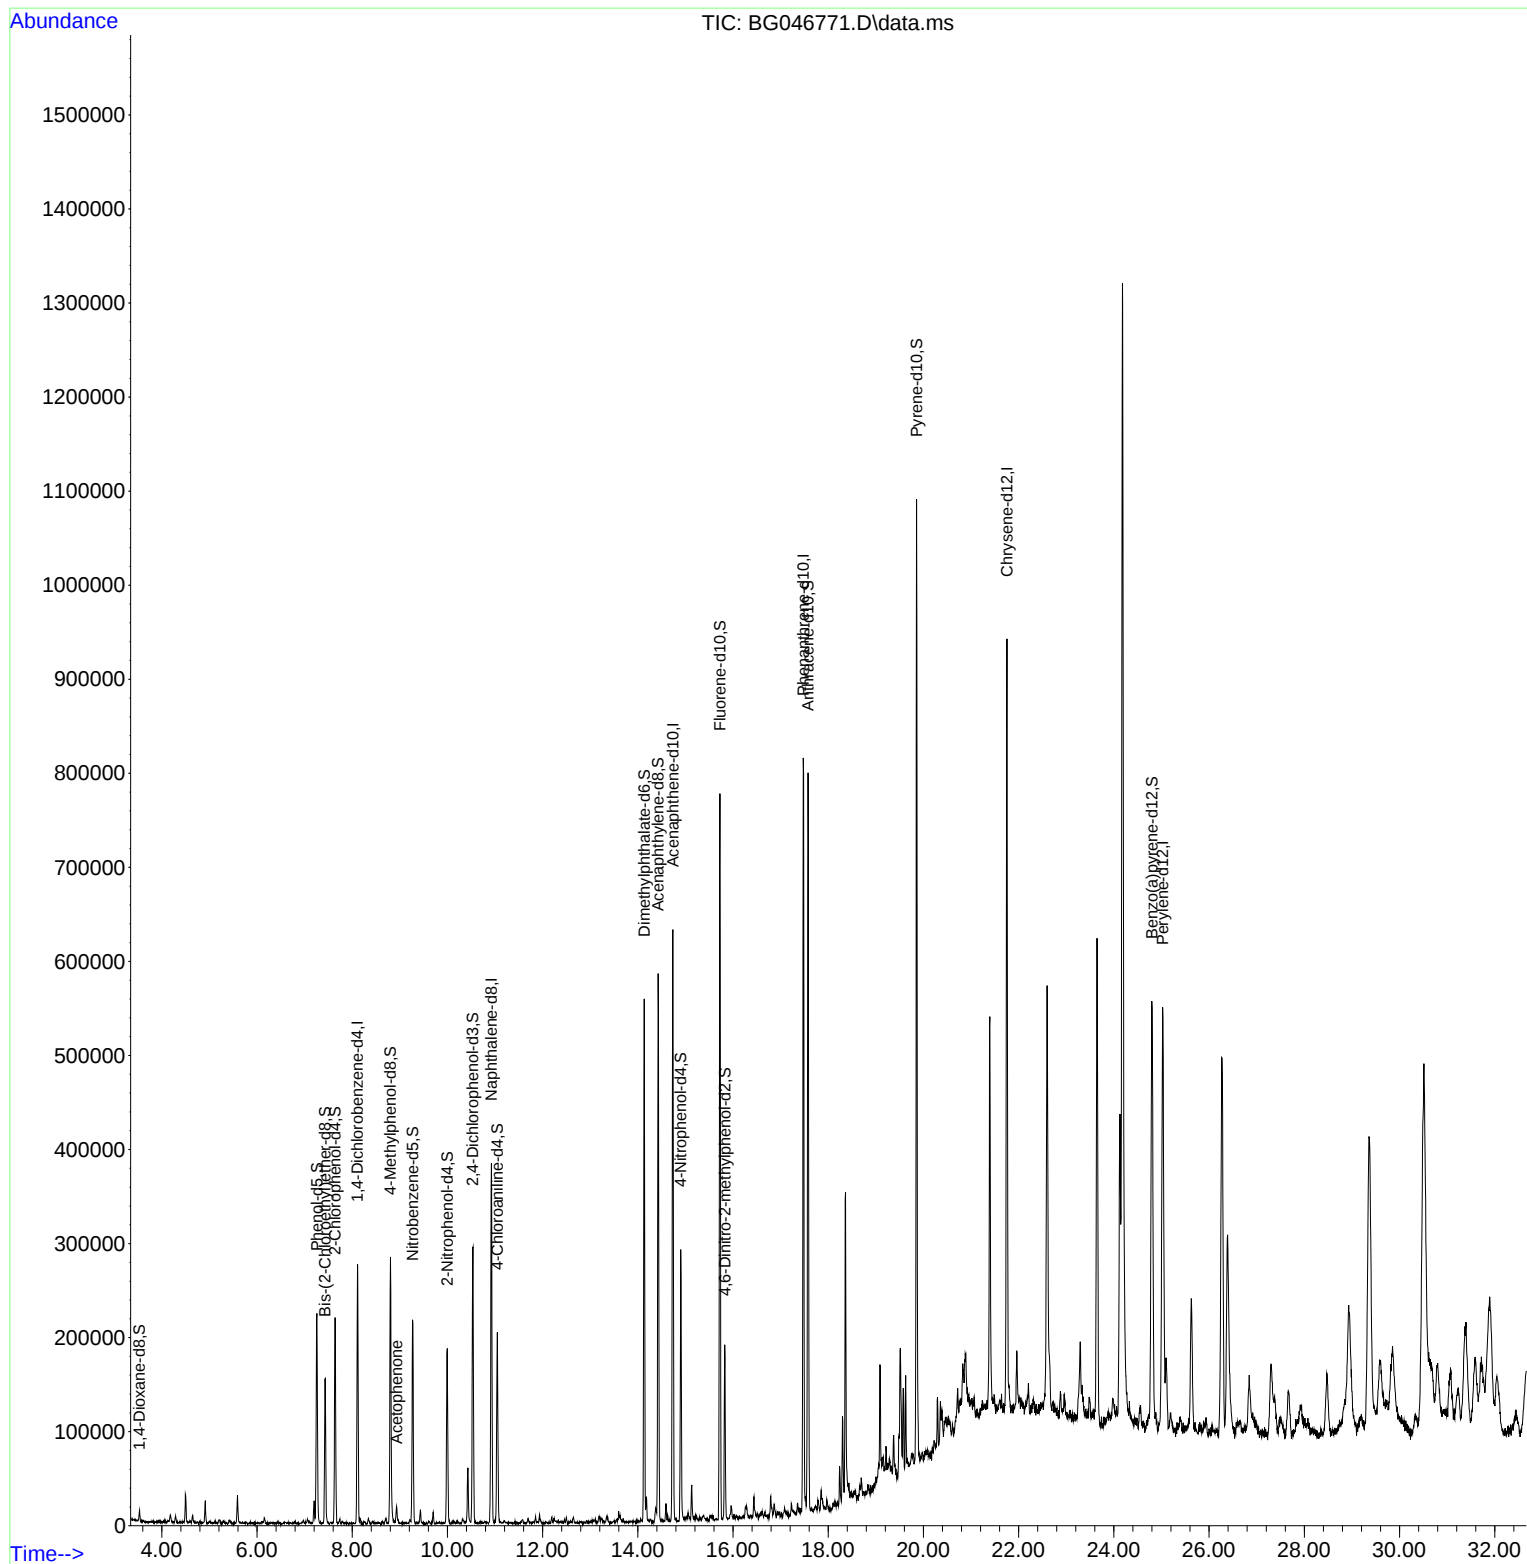

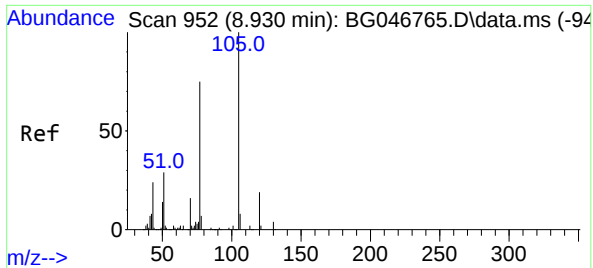

#14
Acetophenone
Concen: 1.19 ng/ul
RT: 8.932 min Scan# 952
Delta R.T. 0.001 min
Lab File: BG046771.D
Acq: 3 Oct 2020 14:30

Instrument :
BNA_G
ClientSampleId :
CB7M2

Tgt Ion:105 Resp: 9613

Ion	Ratio	Lower	Upper
105	100		
77	88.6	60.4	90.6
51	30.2	24.1	36.1

