

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046778.D
 Acq On : 3 Oct 2020 19:11
 Operator : CG/JU
 Sample : L4150-19
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7M0

Quant Time: Oct 05 01:00:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 00:58:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.111	152	78226	20.00	ng/ul	0.00
18) Naphthalene-d8	10.920	136	325825	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.733	164	241031	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.477	188	561083	20.00	ng/ul	0.00
78) Chrysene-d12	21.748	240	577314	20.00	ng/ul	0.00
86) Perylene-d12	25.027	264	578621	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.528	96	10938	6.86	ng/uL	0.00
5) Phenol-d5	7.253	99	231268	34.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.430	67	136325	33.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.641	132	174022	35.60	ng/ul	0.00
13) 4-Methylphenol-d8	8.805	113	183358	35.02	ng/ul	0.00
19) Nitrobenzene-d5	9.275	128	89190	36.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.997	143	108865	43.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.532	165	204001	34.99	ng/ul	0.00
29) 4-Chloroaniline-d4	11.049	131	219622	31.69	ng/ul	0.00
44) Dimethylphthalate-d6	14.134	166	614897	33.39	ng/ul	0.00
47) Acenaphthylene-d8	14.427	160	776345	35.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.903	143	113583	36.17	ng/ul	0.00
58) Fluorene-d10	15.720	176	578862	34.09	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.826	200	94045	33.54	ng/ul	0.00
71) Anthracene-d10	17.577	188	874460	33.97	ng/ul	0.00
79) Pyrene-d10	19.856	212	1017978	33.98	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.804	264	1066925	34.21	ng/ul	0.00
Target Compounds						Qvalue
45) Dimethylphthalate	14.181	163	24219	1.30	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046778.D
Acq On : 3 Oct 2020 19:11
Operator : CG/JU
Sample : L4150-19
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7M0


Quant Time: Oct 05 01:00:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 00:58:20 2020
Response via : Initial Calibration

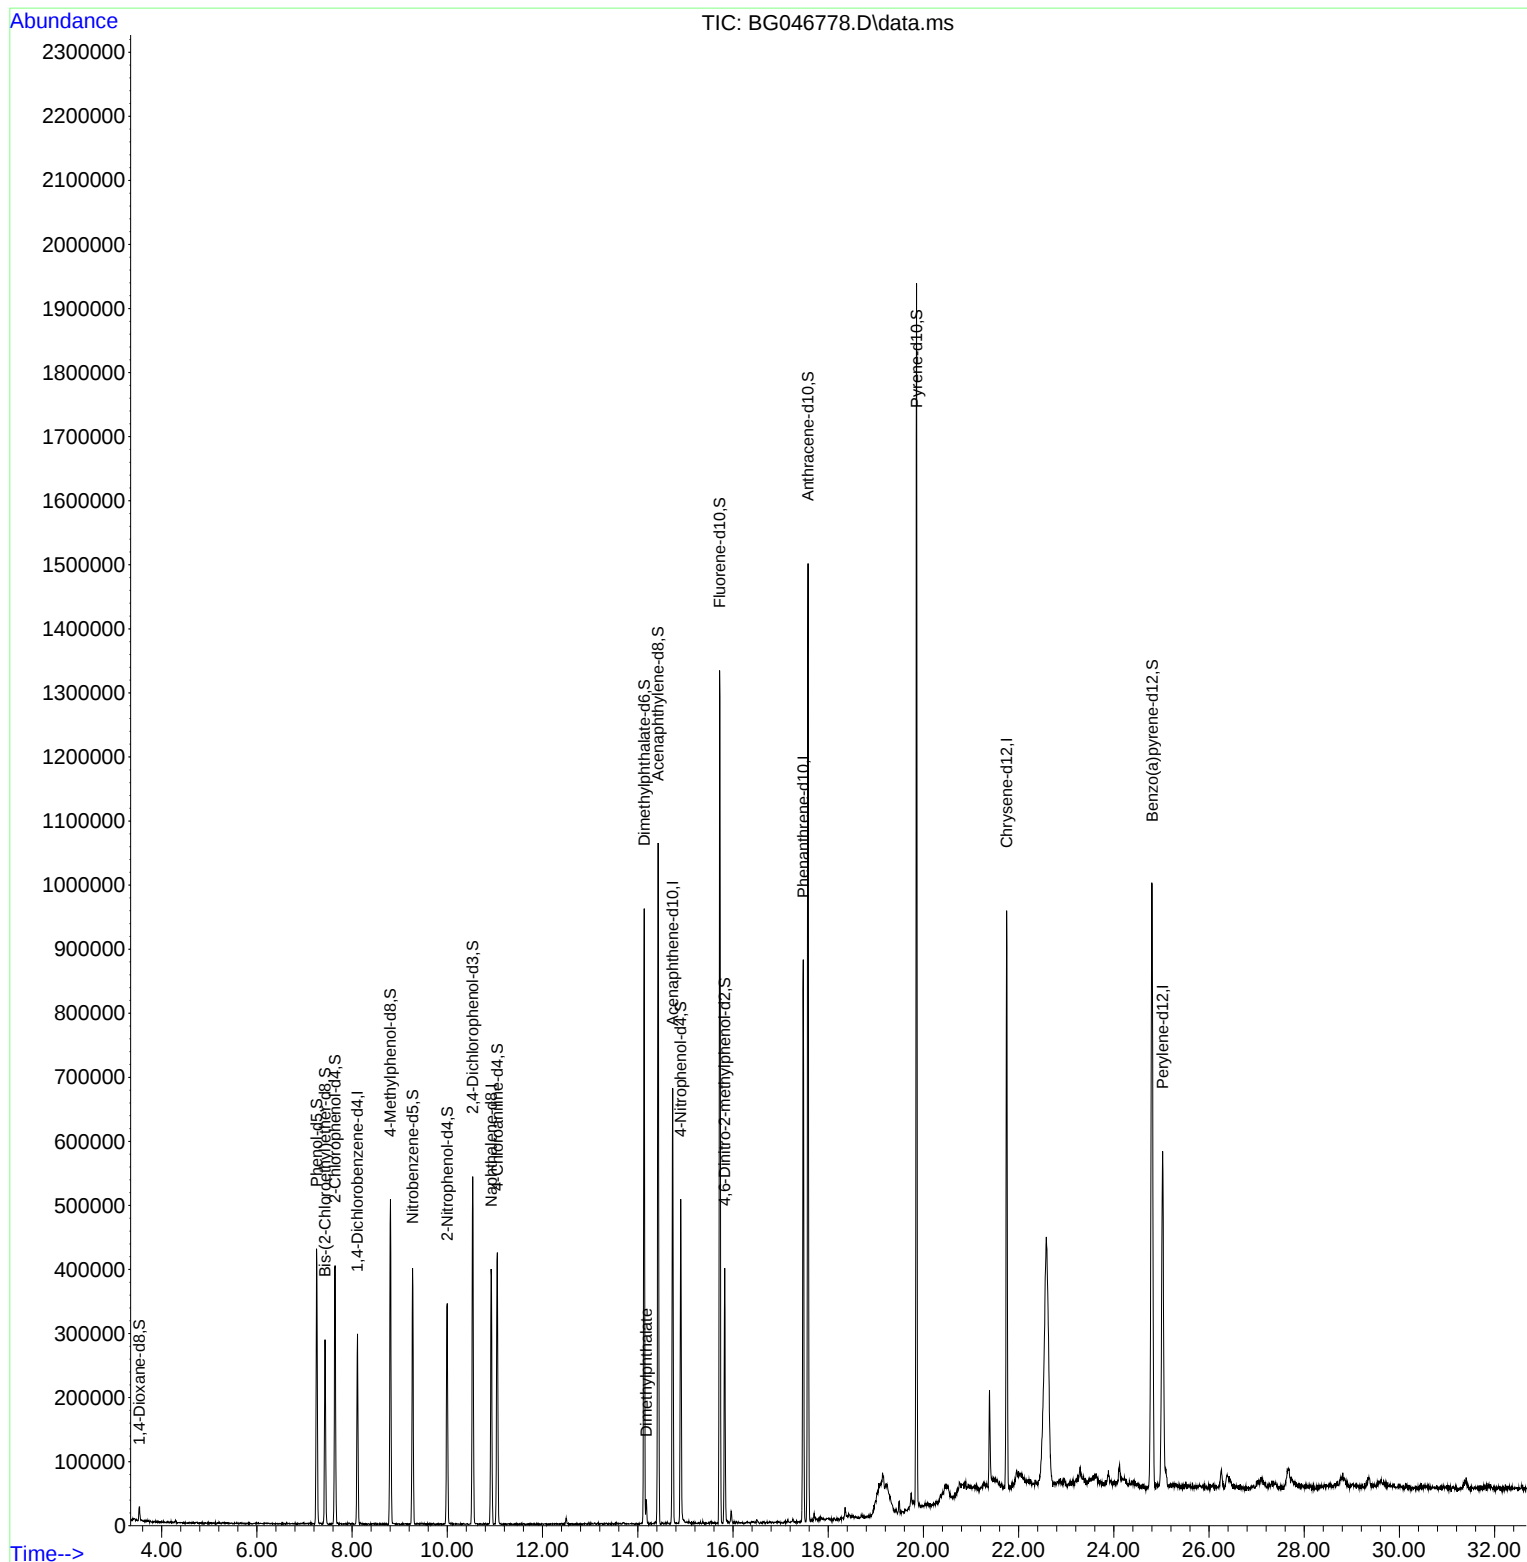

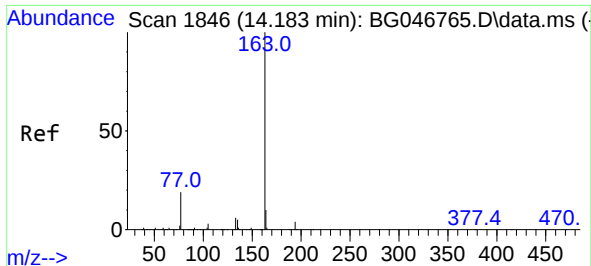

#45
 Dimethylphthalate
 Concen: 1.30 ng/ul
 RT: 14.181 min Scan# 1845
 Delta R.T. -0.002 min
 Lab File: BG046778.D
 Acq: 3 Oct 2020 19:11

Instrument :
 BNA_G
 ClientSampleId :
 CB7M0

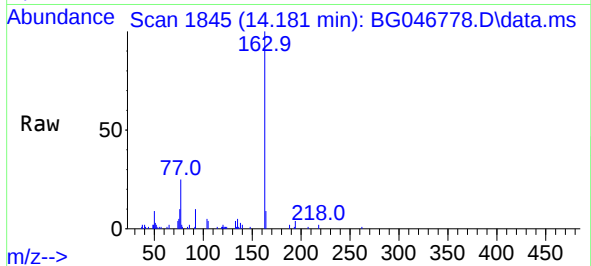

Tgt Ion:163 Resp: 24219
 Ion Ratio Lower Upper
 163 100
 194 3.6 3.6 5.4#
 164 9.1 7.4 11.0

