

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
 Data File : BG046780.D
 Acq On : 3 Oct 2020 20:32
 Operator : CG/JU
 Sample : L4151-15
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CB7L6

Quant Time: Oct 05 01:00:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 00:58:20 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.111	152	72018	20.00	ng/ul	0.00
18) Naphthalene-d8	10.919	136	301064	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.732	164	218113	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.476	188	511240	20.00	ng/ul	0.00
78) Chrysene-d12	21.747	240	514222	20.00	ng/ul	0.00
86) Perylene-d12	25.026	264	537749	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.534	96	5222	3.56	ng/uL	0.00
5) Phenol-d5	7.253	99	119897	19.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.429	67	76041	20.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.640	132	92635	20.59	ng/ul	0.00
13) 4-Methylphenol-d8	8.804	113	99136	20.57	ng/ul	0.00
19) Nitrobenzene-d5	9.268	128	50022	22.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.991	143	59042	25.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.531	165	110396	20.49	ng/ul	0.00
29) 4-Chloroaniline-d4	11.048	131	96462	15.07	ng/ul	0.00
44) Dimethylphthalate-d6	14.133	166	357696	21.46	ng/ul	0.00
47) Acenaphthylene-d8	14.427	160	407096	20.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.903	143	56240	19.79	ng/ul	0.00
58) Fluorene-d10	15.719	176	316170	20.58	ng/ul	0.00
63) 4,6-Dinitro-2-methylph...	15.825	200	43758	17.13	ng/ul	0.00
71) Anthracene-d10	17.576	188	445725	19.00	ng/ul	0.00
79) Pyrene-d10	19.856	212	528616	19.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.797	264	518703	17.90	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	14.180	163	37169	2.20	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100220\
Data File : BG046780.D
Acq On : 3 Oct 2020 20:32
Operator : CG/JU
Sample : L4151-15
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CB7L6


Quant Time: Oct 05 01:00:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG092920MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 00:58:20 2020
Response via : Initial Calibration

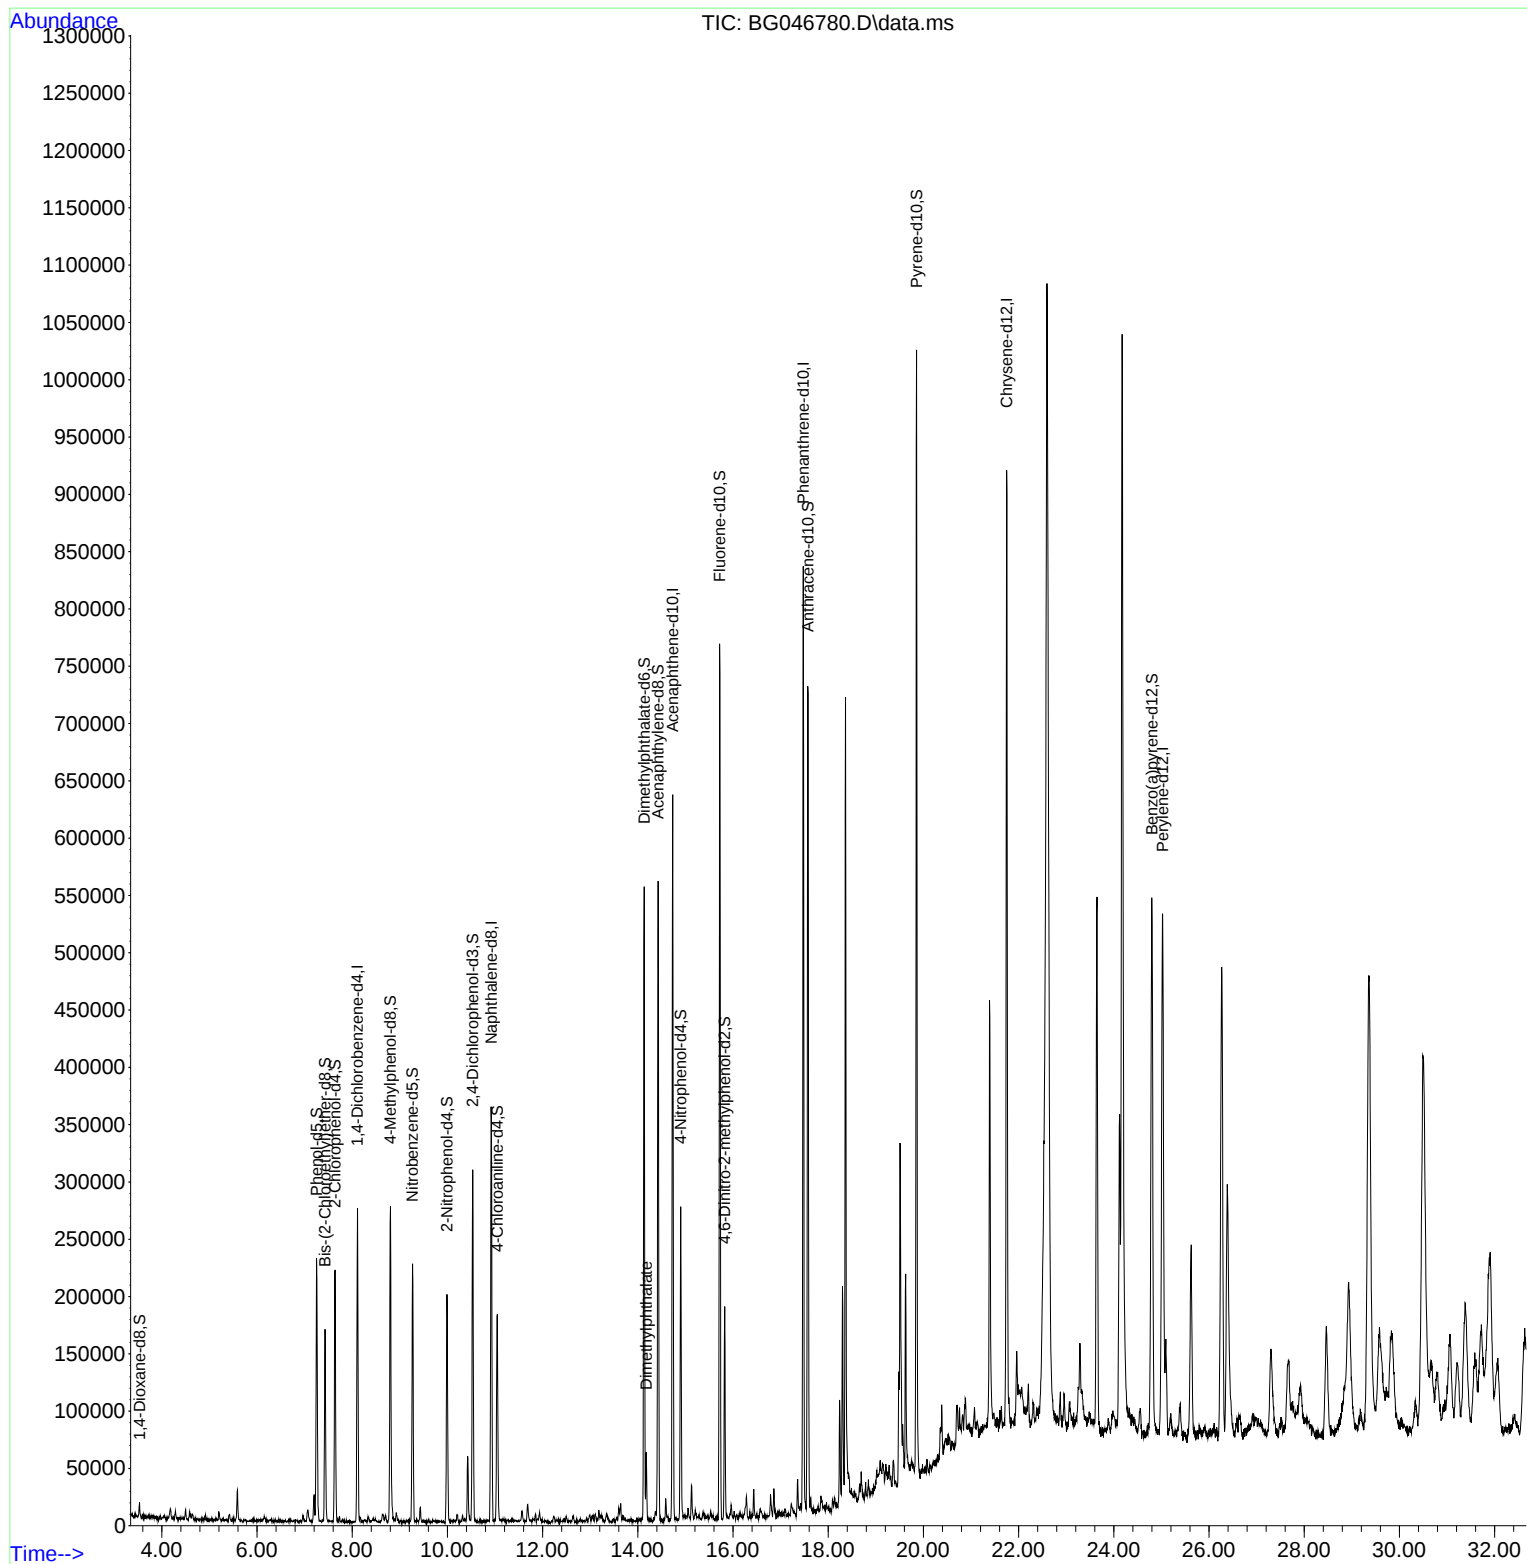

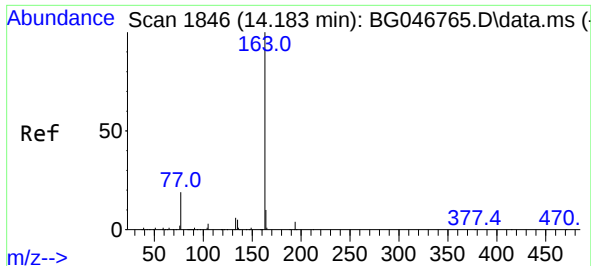

#45
Dimethylphthalate
Concen: 2.20 ng/ul
RT: 14.180 min Scan# 1845
Delta R.T. -0.003 min
Lab File: BG046780.D
Acq: 3 Oct 2020 20:32

Instrument :
BNA_G
ClientSampleId :
CB7L6

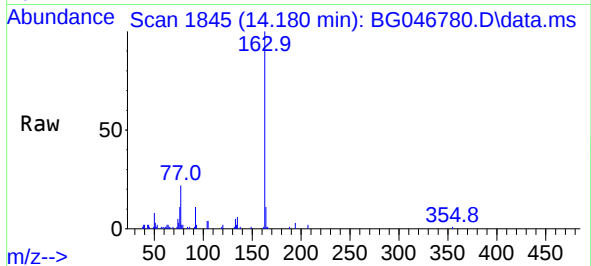

Tgt Ion:163 Resp: 37169
Ion Ratio Lower Upper
163 100
194 3.0 3.6 5.4#
164 10.5 7.4 11.0

