

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100317\
 Data File : BG029030.D
 Acq On : 4 Oct 2017 7:49
 Operator : SJ/JU
 Sample : I5517-06
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 04 11:23:03 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.24	152	36210	20.00	ng	-0.09
21) Naphthalene-d8	11.06	136	144989	20.00	ng	-0.09
38) Acenaphthene-d10	14.87	164	107313	20.00	ng	-0.08
63) Phenanthrene-d10	17.62	188	279097	20.00	ng	-0.08
75) Chrysene-d12	21.93	240	298109	20.00	ng	-0.10
86) Perylene-d12	25.35	264	299635	20.00	ng	-0.18
System Monitoring Compounds						
5) 2-Fluorophenol	5.81	112	147399	67.17	ng	-0.10
7) Phenol-d6	7.40	99	121658	36.82	ng	-0.09
23) Nitrobenzene-d5	9.41	82	327019	107.90	ng	-0.10
41) 2,4,6-Tribromophenol	16.36	330	307706	173.37	ng	-0.08
44) 2-Fluorobiphenyl	13.49	172	827406	102.81	ng	-0.08
78) Terphenyl-d14	20.21	244	1502771	107.50	ng	-0.07
Target Compounds						
53) 2,4-Dinitrophenol	14.91	184	81	8.071	ng	Qvalue # 15


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100317\
Data File : BG029030.D
Acq On : 4 Oct 2017 7:49
Operator : SJ/JU
Sample : I5517-06
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 04 11:23:03 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

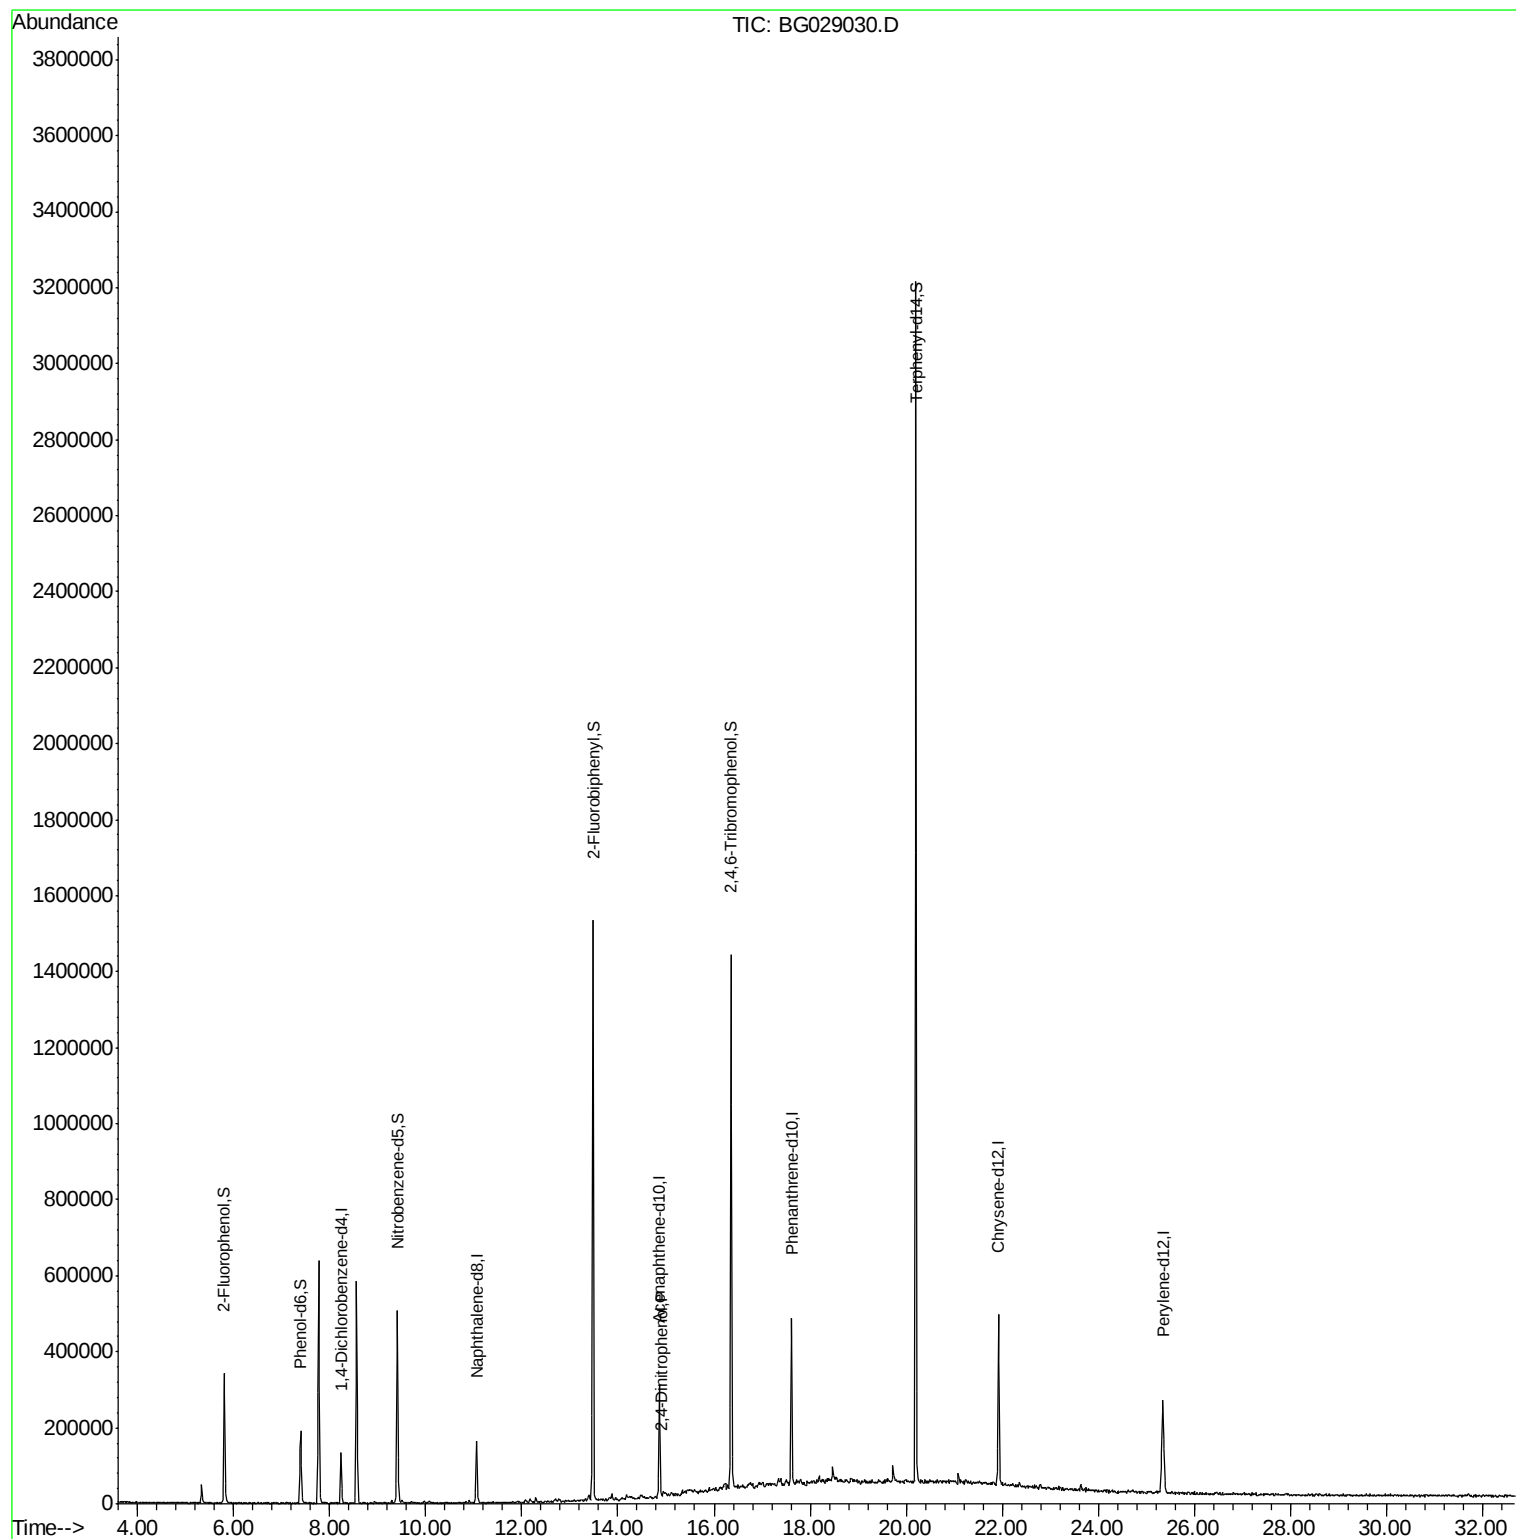




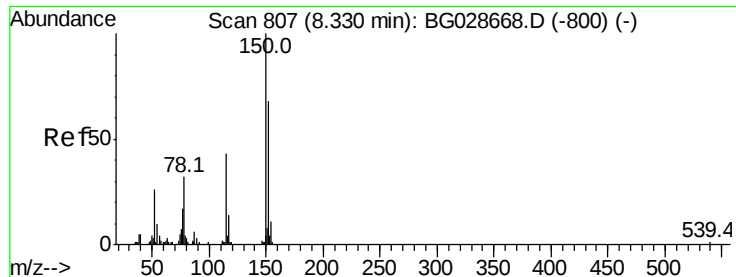


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.24 min Scan# 791
Delta R.T. -0.09 min
Lab File: BG029030.D
Acq: 4 Oct 2017 7:49

Instrument :
BNA_G
ClientSampleId :




Tot Ion:152 Resp: 36210
Ion Ratio Lower Upper
152 100
150 153.5 114.0 171.0
115 54.7 48.1 72.1

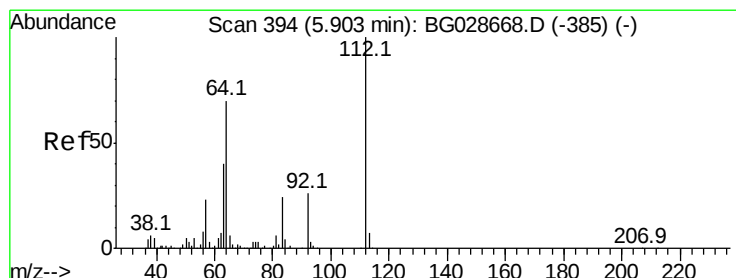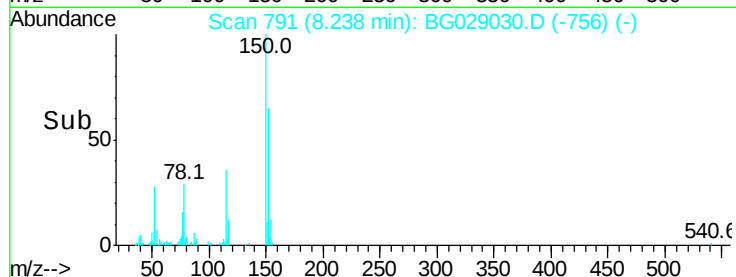
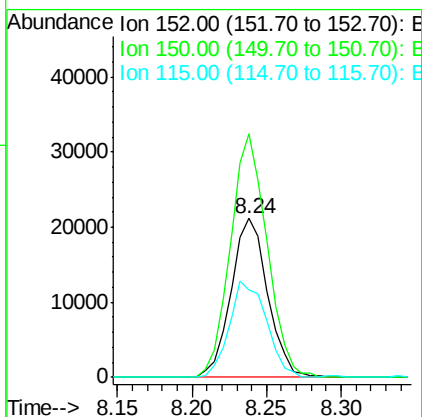
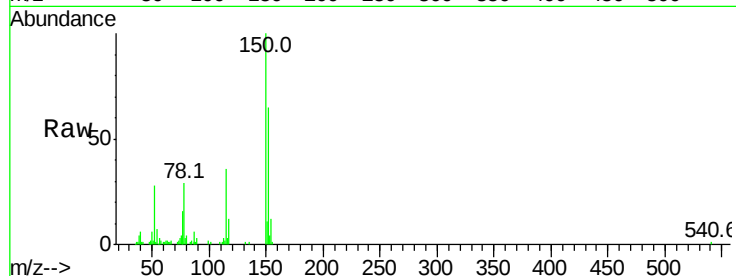


#5

2-Fluorophenol
Concen: 67.168 ng
RT: 5.81 min Scan# 377
Delta R.T. -0.10 min
Lab File: BG029030.D
Acq: 4 Oct 2017 7:49

Tgt Ion:112 Resp: 147399
Ion Ratio Lower Upper
112 100
64 69.2 61.8 92.6
63 42.3 37.2 55.8

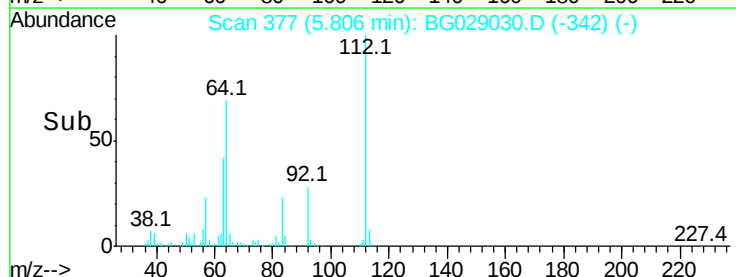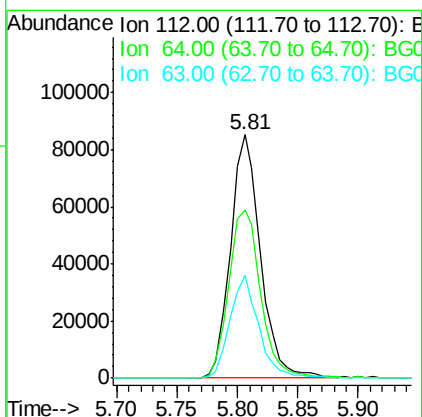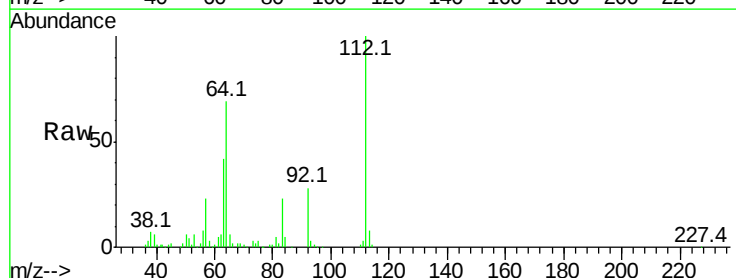

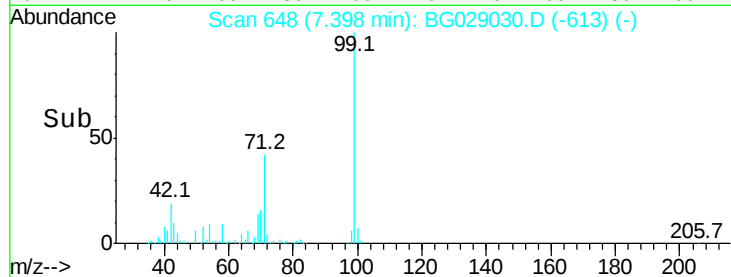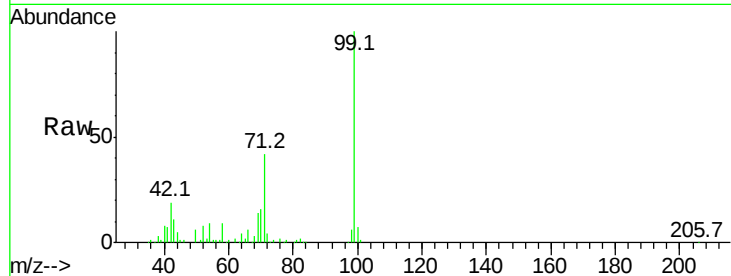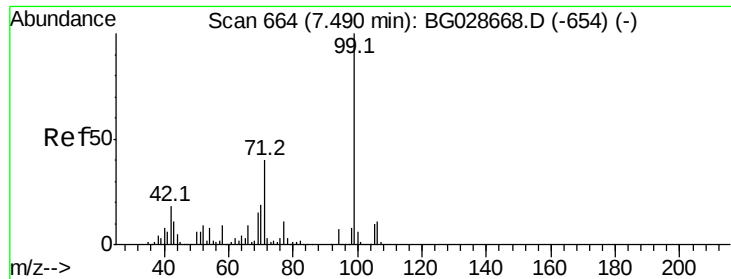

#7

Phenol-d6

Concen: 36.821 ng

RT: 7.40 min Scan# 648

Delta R.T. -0.09 min

Lab File: BG029030.D

Acq: 4 Oct 2017 7:49





Instrument :

BNA_G

ClientSampleId :

Tot Ion: 99 Resp: 121658

Ion	Ratio	Lower	Upper
99	100		
42	18.6	20.5	30.7#
71	42.4	37.6	56.4

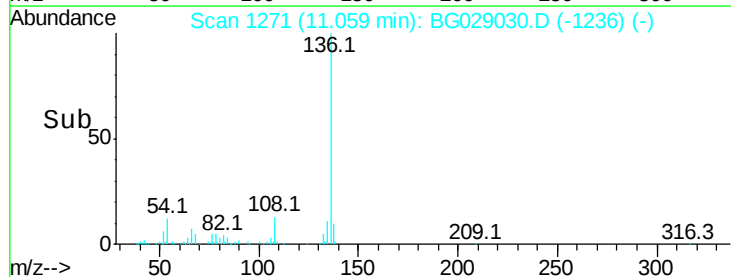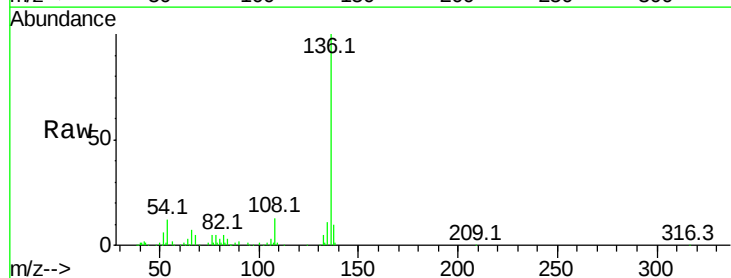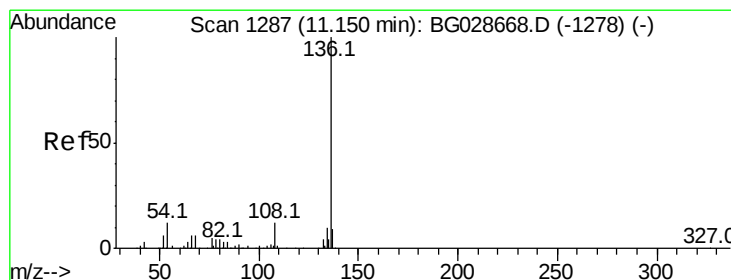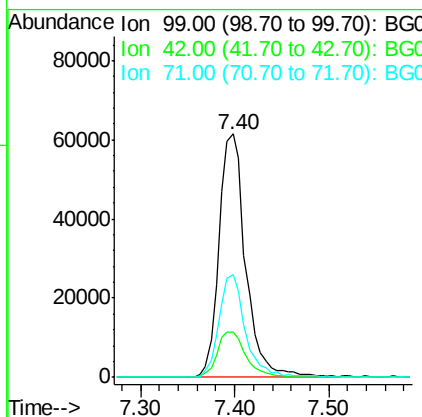

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.06 min Scan# 1271


Delta R.T. -0.09 min


Lab File: BG029030.D

Acq: 4 Oct 2017 7:49

Tgt Ion: 136 Resp: 144989

Ion	Ratio	Lower	Upper
136	100		
137	10.4	8.9	13.3
54	11.6	9.3	13.9
68	5.3	5.1	7.7

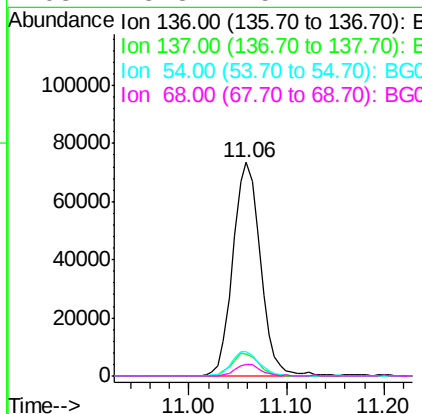


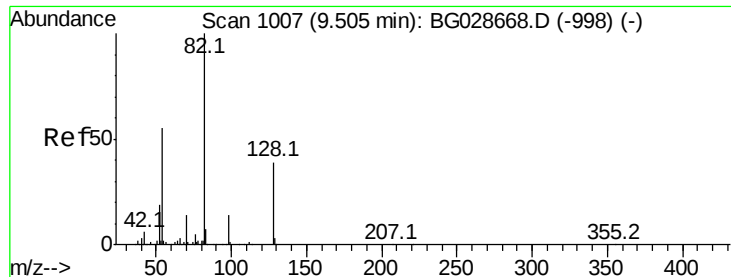




#23
Nitrobenzene-d5
Concen: 107.896 ng
RT: 9.41 min Scan# 990
Delta R.T. -0.10 min
Lab File: BG029030.D
Acq: 4 Oct 2017 7:49

Instrument :
BNA_G
ClientSampleId :

Tot Ion	82	Resp	327019
Ion Ratio	Lower	Upper	
82	100		
128	39.2	26.4	39.6
54	59.1	49.4	74.2

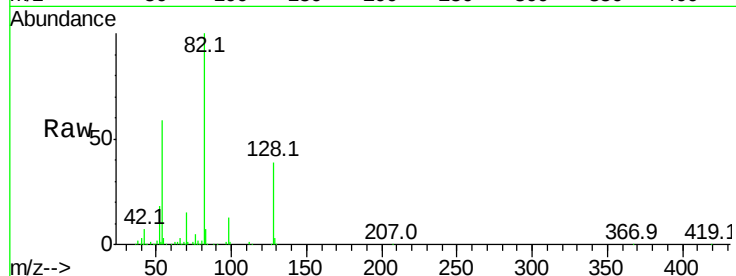


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

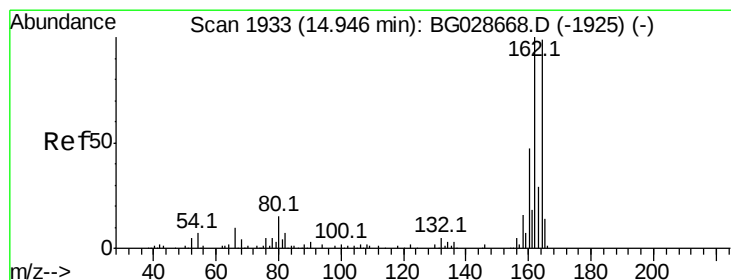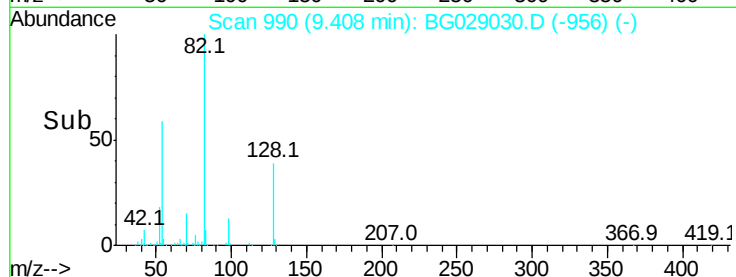
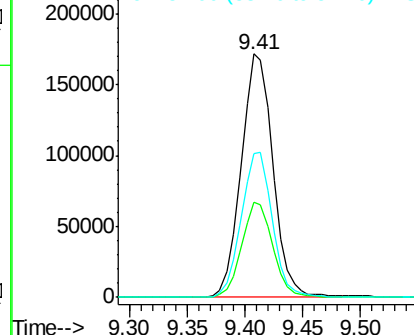



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.87 min Scan# 1919
Delta R.T. -0.08 min
Lab File: BG029030.D
Acq: 4 Oct 2017 7:49

Tgt Ion	164	Resp	107313
Ion Ratio	Lower	Upper	
164	100		
162	102.9	85.1	127.7
160	51.3	34.7	52.1

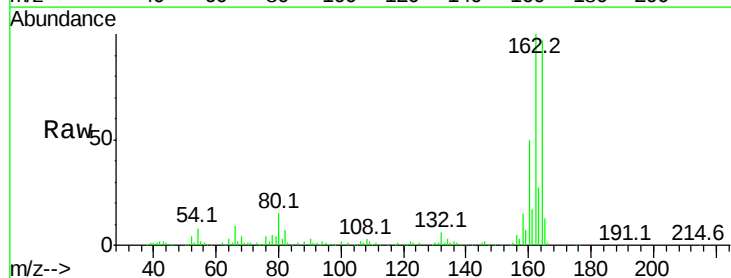

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

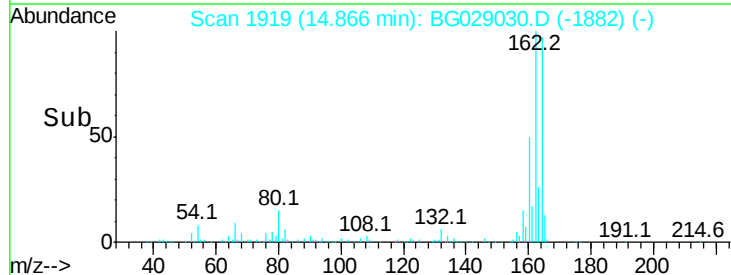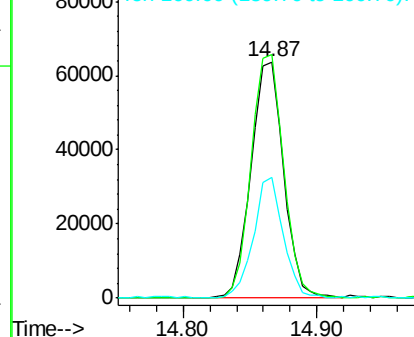


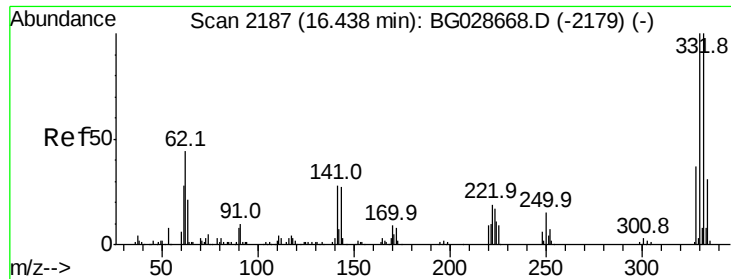




#41
 2,4,6-Tribromophenol
 Concen: 173.366 ng
 RT: 16.36 min Scan# 2173
 Delta R.T. -0.08 min
 Lab File: BG029030.D
 Acq: 4 Oct 2017 7:49

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.3	115.9
141	31.4	32.1	48.1#

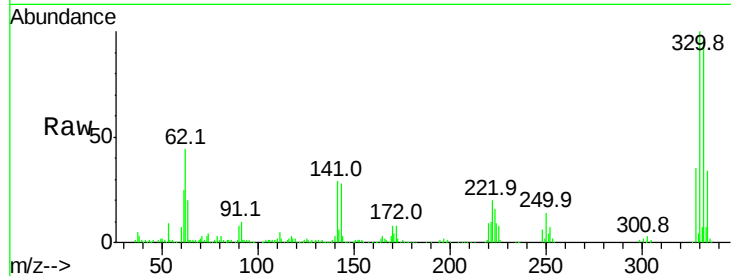


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

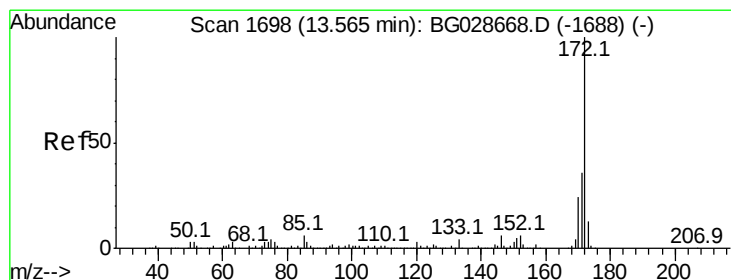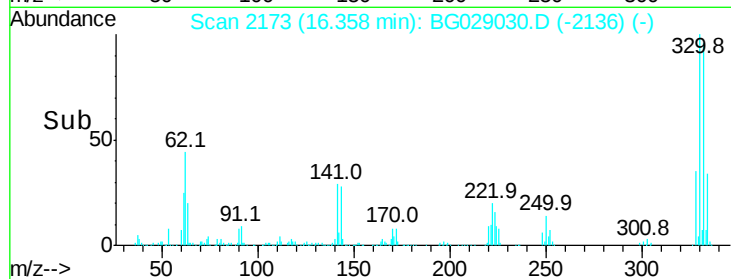
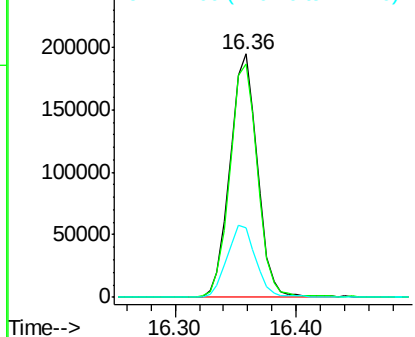



#44
 2-Fluorobiphenyl
 Concen: 102.810 ng
 RT: 13.49 min Scan# 1684
 Delta R.T. -0.08 min
 Lab File: BG029030.D
 Acq: 4 Oct 2017 7:49

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	32.2	48.2
170	22.3	21.8	32.6

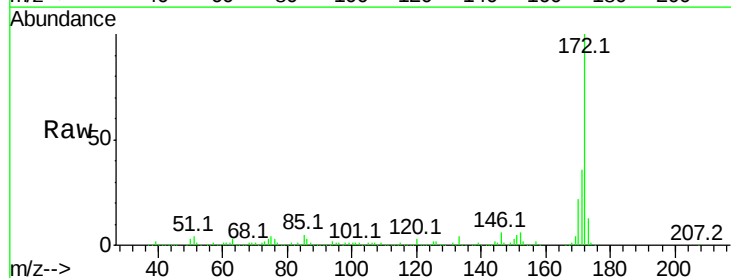

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



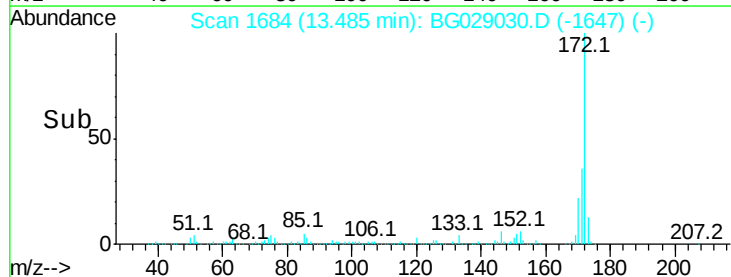
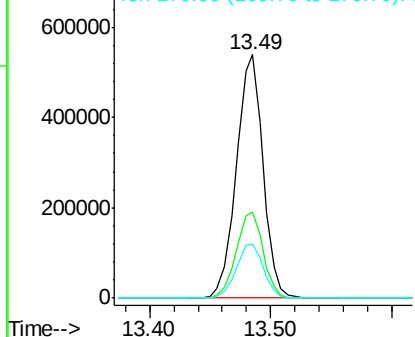


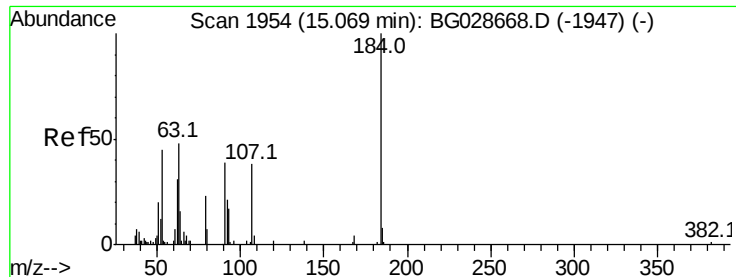

#53
 2,4-Dinitrophenol
 Concen: 8.071 ng
 RT: 14.91 min Scan# 1926
 Delta R.T. -0.16 min
 Lab File: BG029030.D
 Acq: 4 Oct 2017 7:49




Instrument :
 BNA_G
 ClientSampled :


Tot Ion:184 Resp: 81
 Ion Ratio Lower Upper
 184 100
 63 0.0 52.7 79.1#
 154 0.0 57.3 85.9#

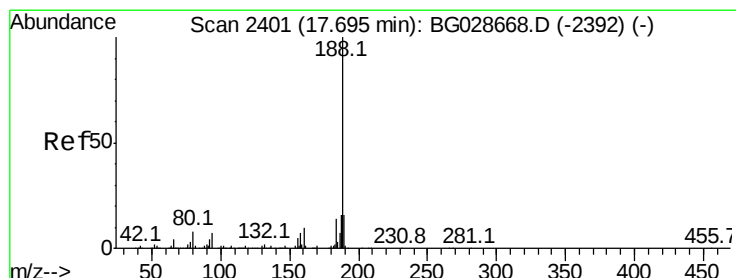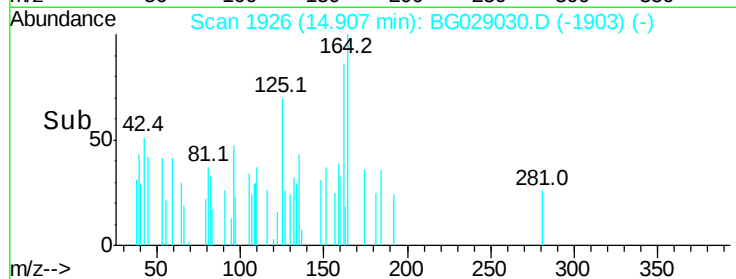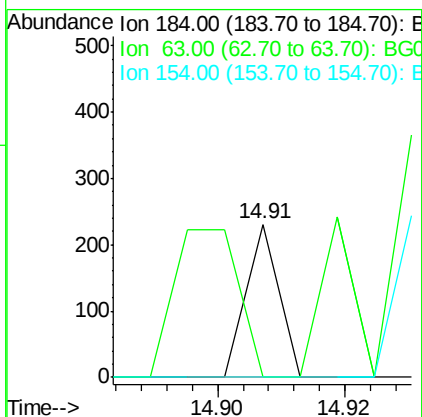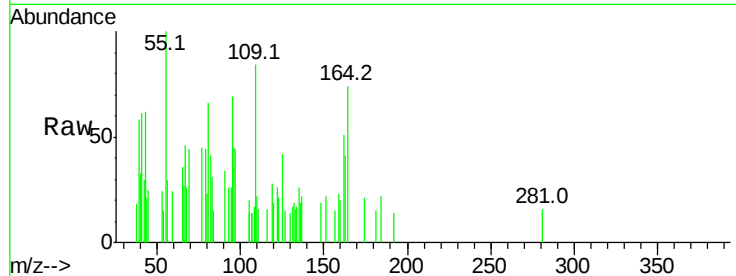

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.62 min Scan# 2387
 Delta R.T. -0.08 min
 Lab File: BG029030.D
 Acq: 4 Oct 2017 7:49

Tgt Ion:188 Resp: 279097
 Ion Ratio Lower Upper
 188 100
 94 7.6 5.8 8.8
 80 5.9 7.5 11.3#

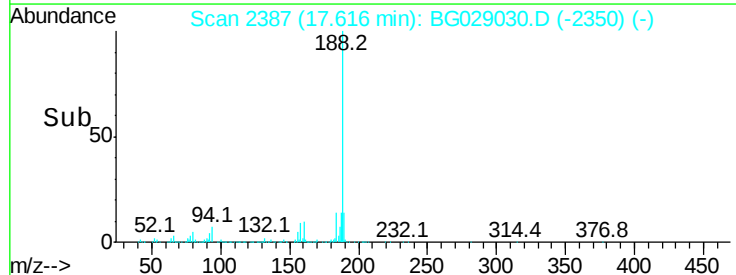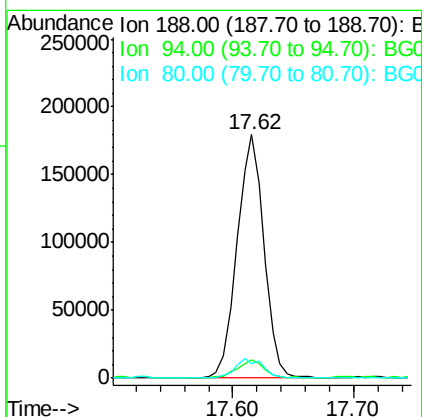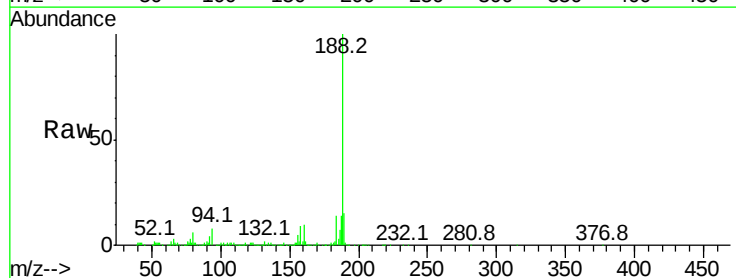

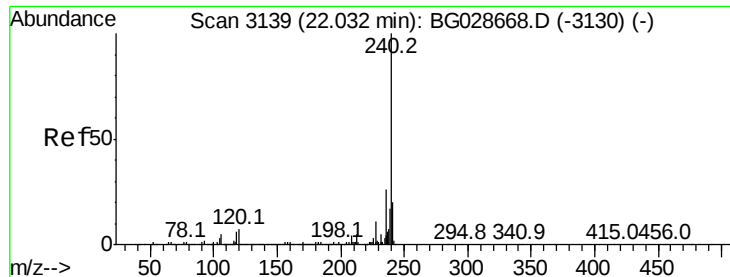

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.93 min Scan# 3121

Delta R.T. -0.10 min

Lab File: BG029030.D

Acq: 4 Oct 2017 7:49

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 298109

Ion Ratio Lower Upper

240 100

120 5.5 5.7 8.5#




236 23.7 22.2 33.4

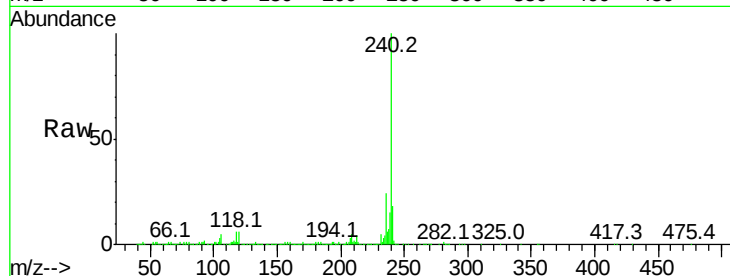

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

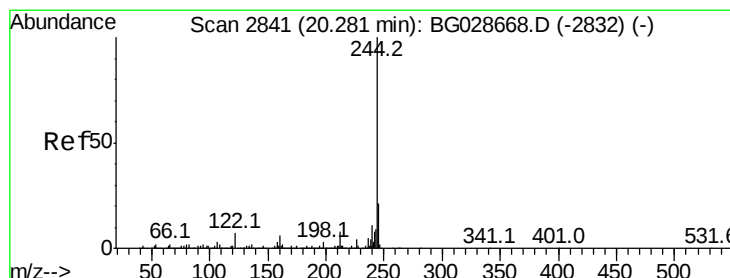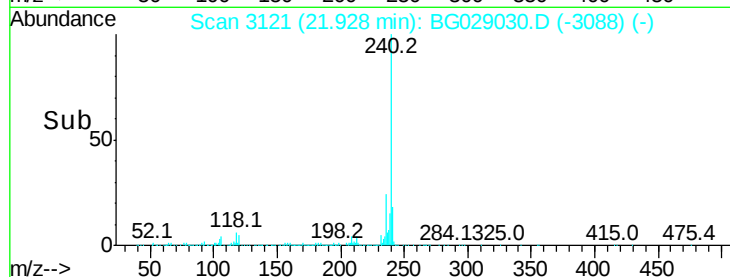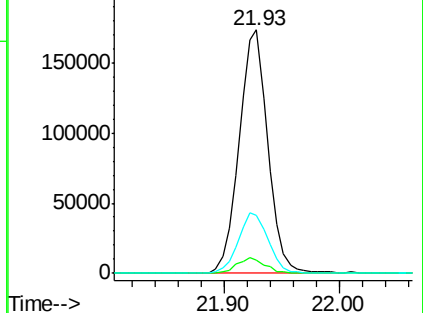

#78

Terphenyl-d14

Concen: 107.503 ng

RT: 20.21 min Scan# 2828

Delta R.T. -0.07 min

Lab File: BG029030.D

Acq: 4 Oct 2017 7:49


Tgt Ion:244 Resp: 1502771

Ion Ratio Lower Upper

244 100

212 8.0 10.0 15.0#



122 7.3 8.6 12.8#

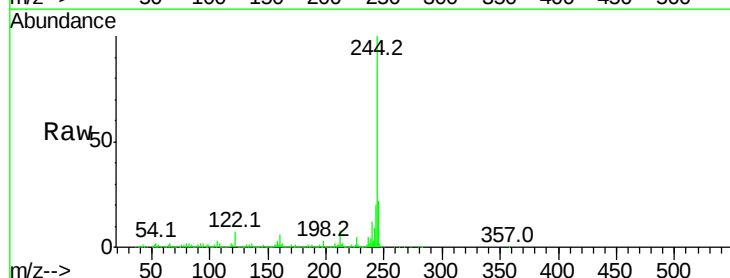


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

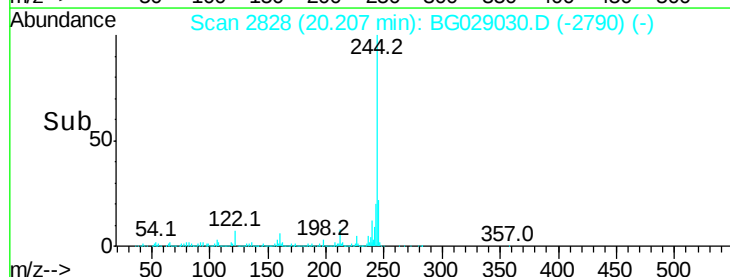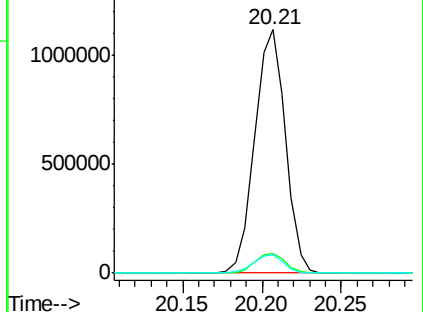


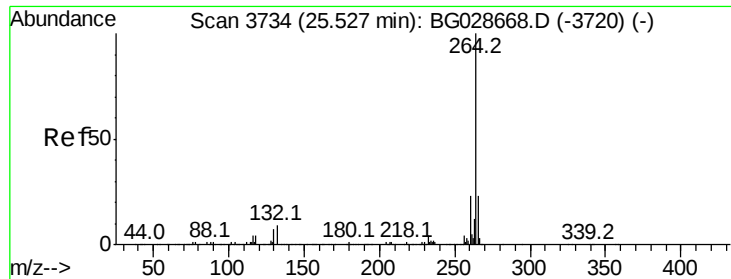

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 25.35 min Scan# 3703
 Delta R.T. -0.18 min
 Lab File: BG029030.D
 Acq: 4 Oct 2017 7:49

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	21.8	32.8
265	21.8	18.2	27.4

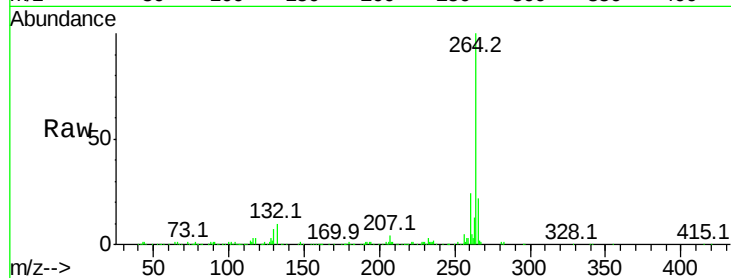

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

