
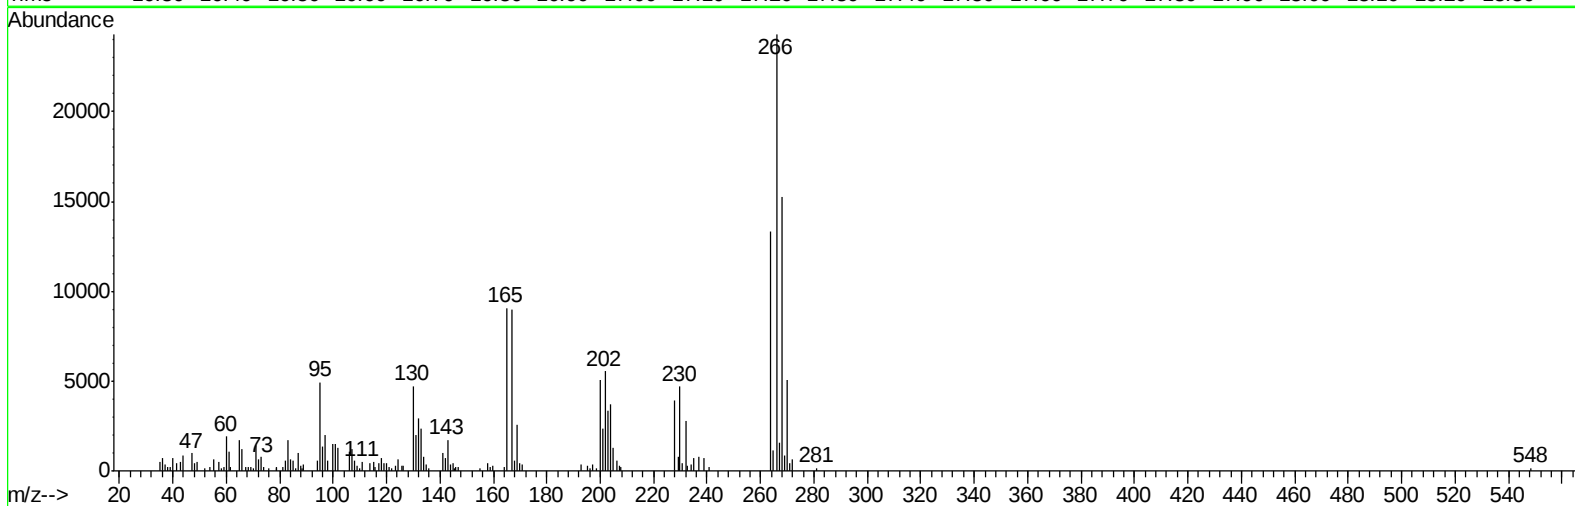


Data Path : Z:\HPCHEM1\BNA G\Data\BG100317\
Data File : BG029001.D
Acq On : 3 Oct 2017 11:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 07:56:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

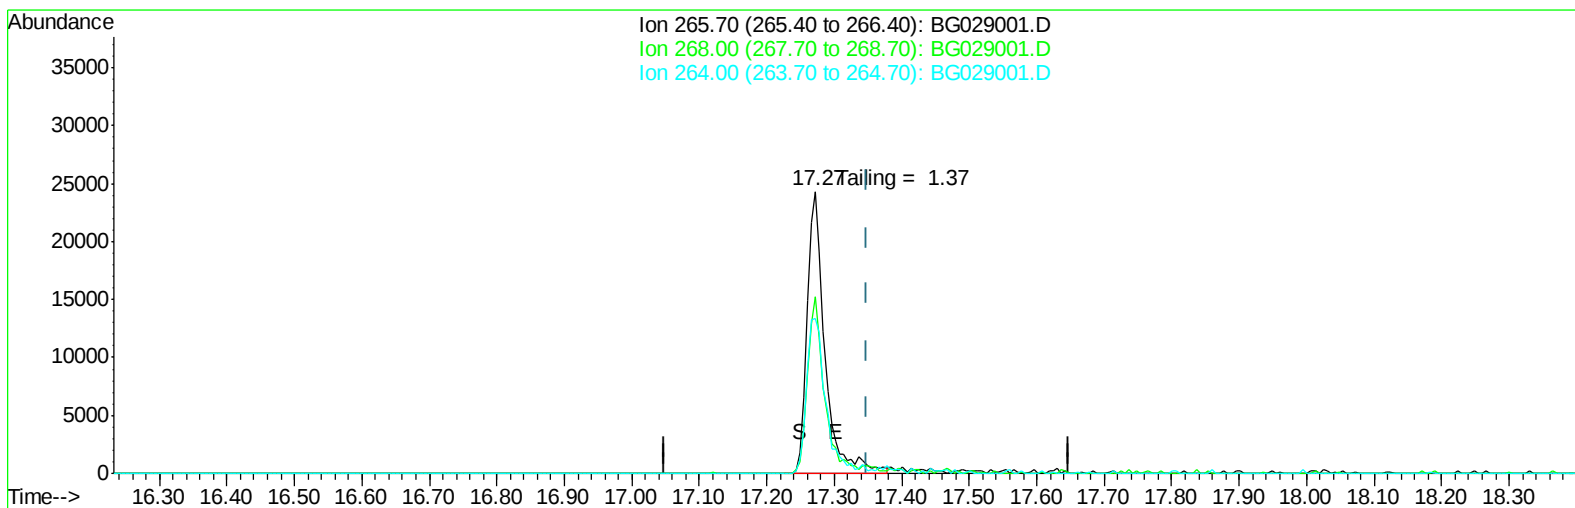

TIC: BG029001.D

(69) Pentachlorophenol (C)



17.272min (-0.076) 76818.60ng

response 42697

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.66
264.00	62.60	54.84
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG100317\
Data File : BG029001.D
Acq On : 3 Oct 2017 11:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 07:56:47 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

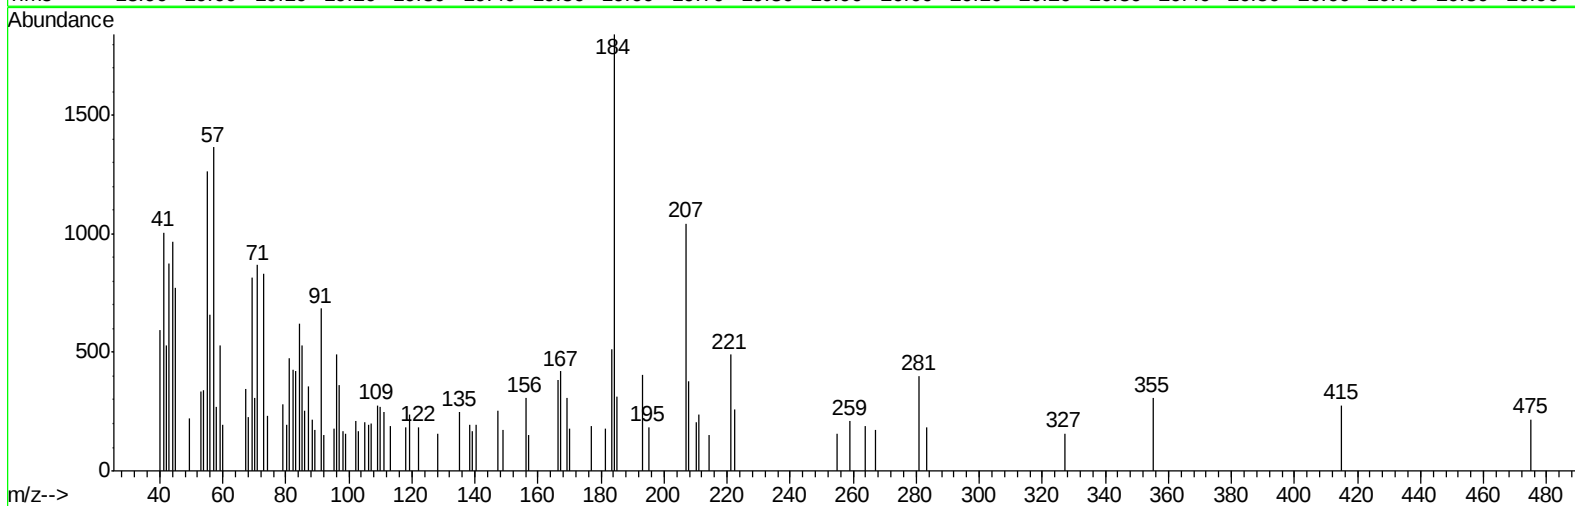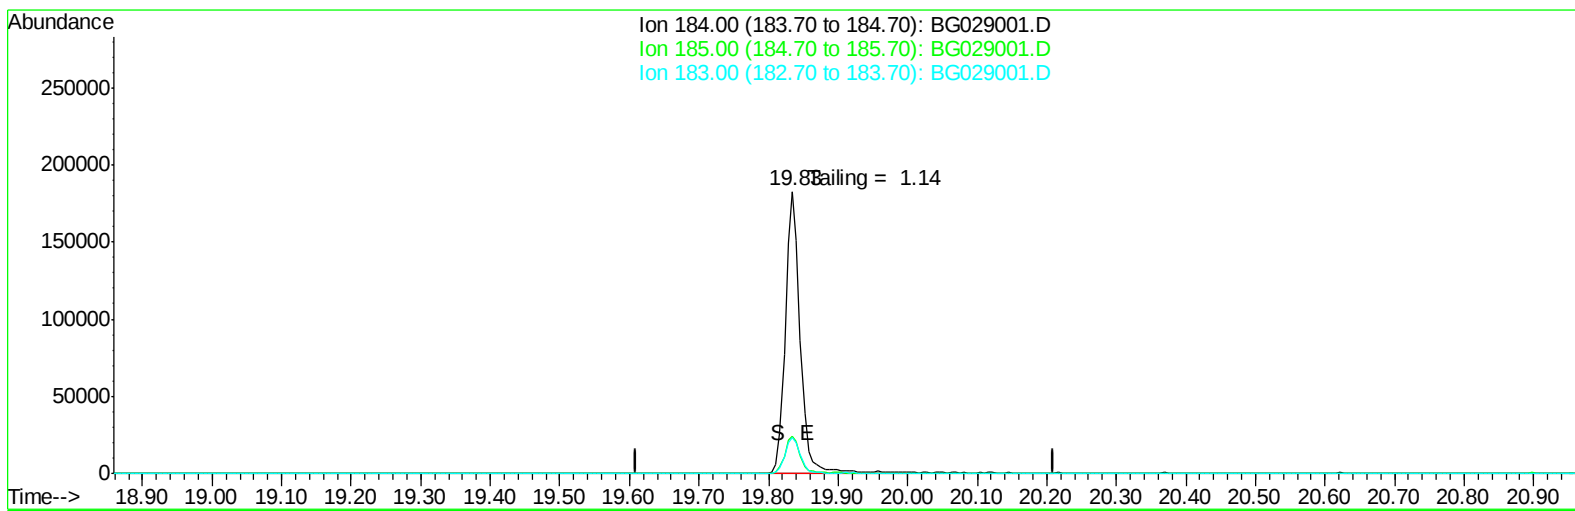

TIC: BG029001.D

(76) Benzidine

19.910min (-19.910) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.30	0.00#
183.00	13.80	0.00#
0.00	0.00	0.00