
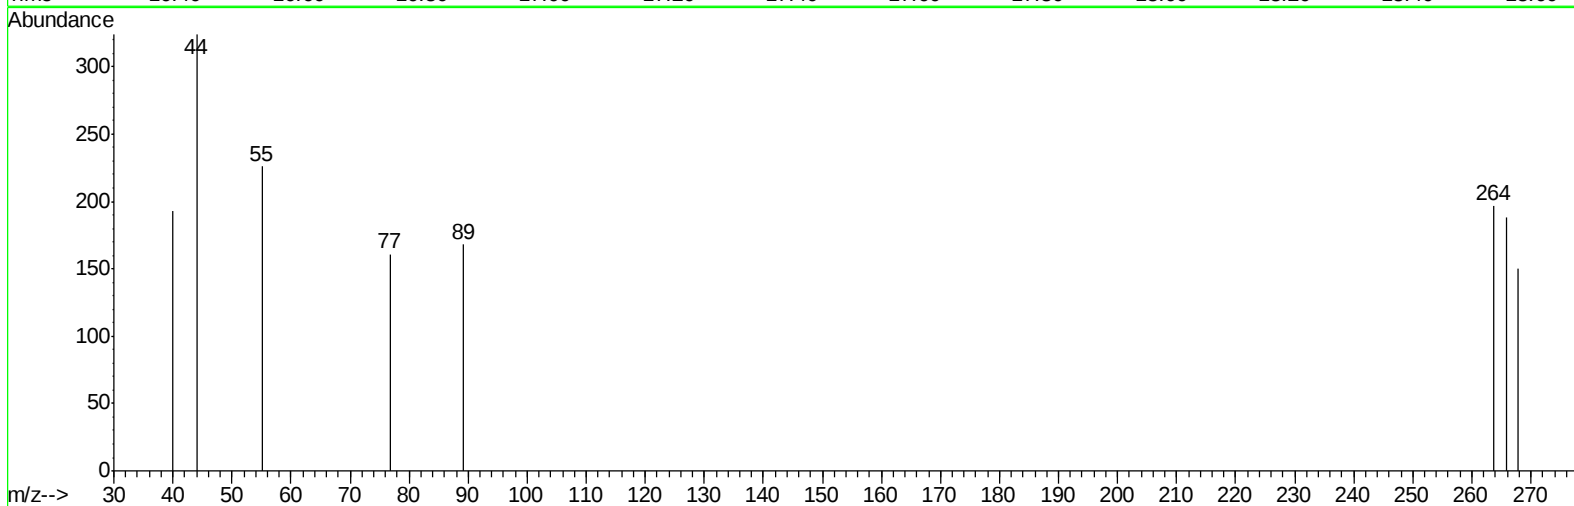


Data Path : Z:\HPCHEM1\BNA G\Data\BG100317\
 Data File : BG029017.D
 Acq On : 3 Oct 2017 22:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 07:58:19 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 16:57:11 2017
 Response via : Initial Calibration

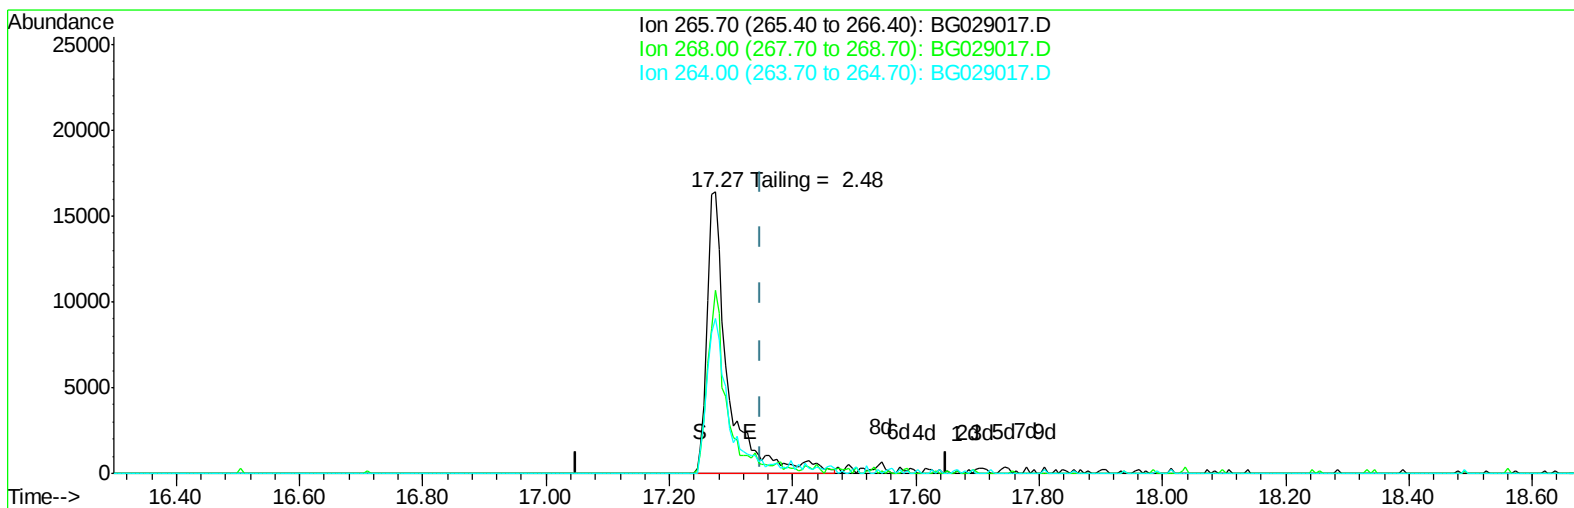

TIC: BG029017.D

(69) Pentachlorophenol (C)



17.668min (+0.319) 29.42ng

response 66

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	79.79#
264.00	62.60	104.79#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG100317\
Data File : BG029017.D
Acq On : 3 Oct 2017 22:38
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 07:58:19 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG091217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 16:57:11 2017
Response via : Initial Calibration

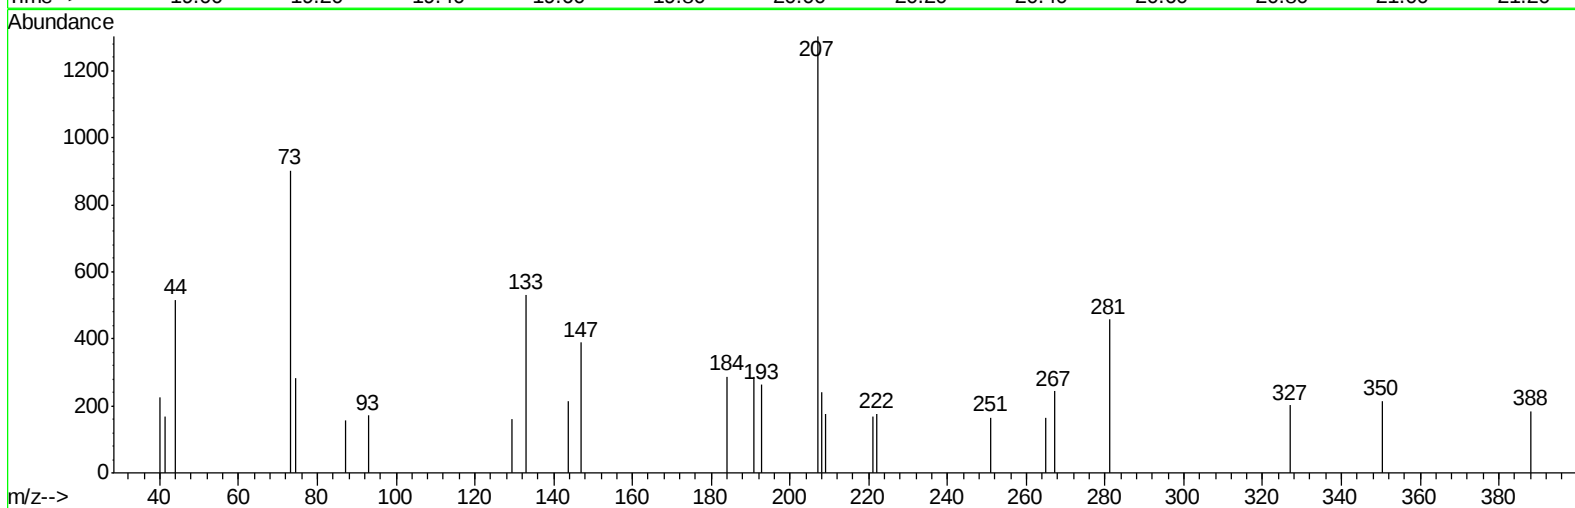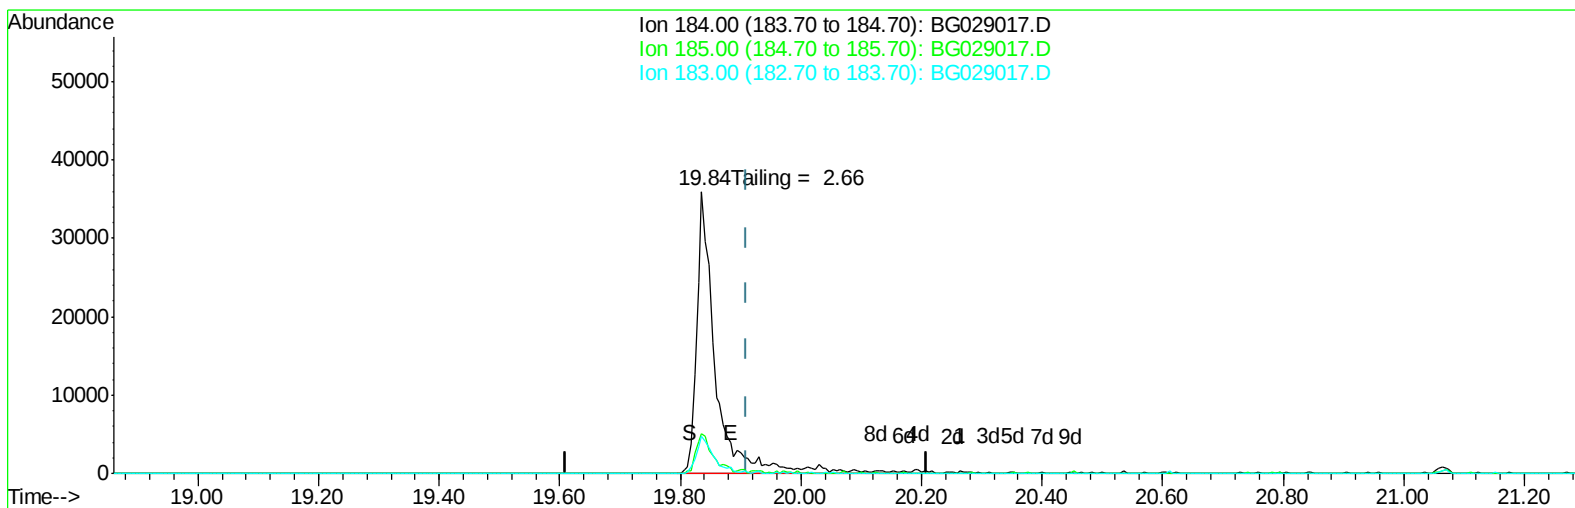

TIC: BG029017.D

(76) Benzidine

20.265min (+0.354) 109.75ng

response 296

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	13.80	0.00#
0.00	0.00	0.00