


Data Path : Z:\HPCHEM1\BNA G\Data\BG100317\
 Data File : BG029001.D
 Acq On : 3 Oct 2017 11:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

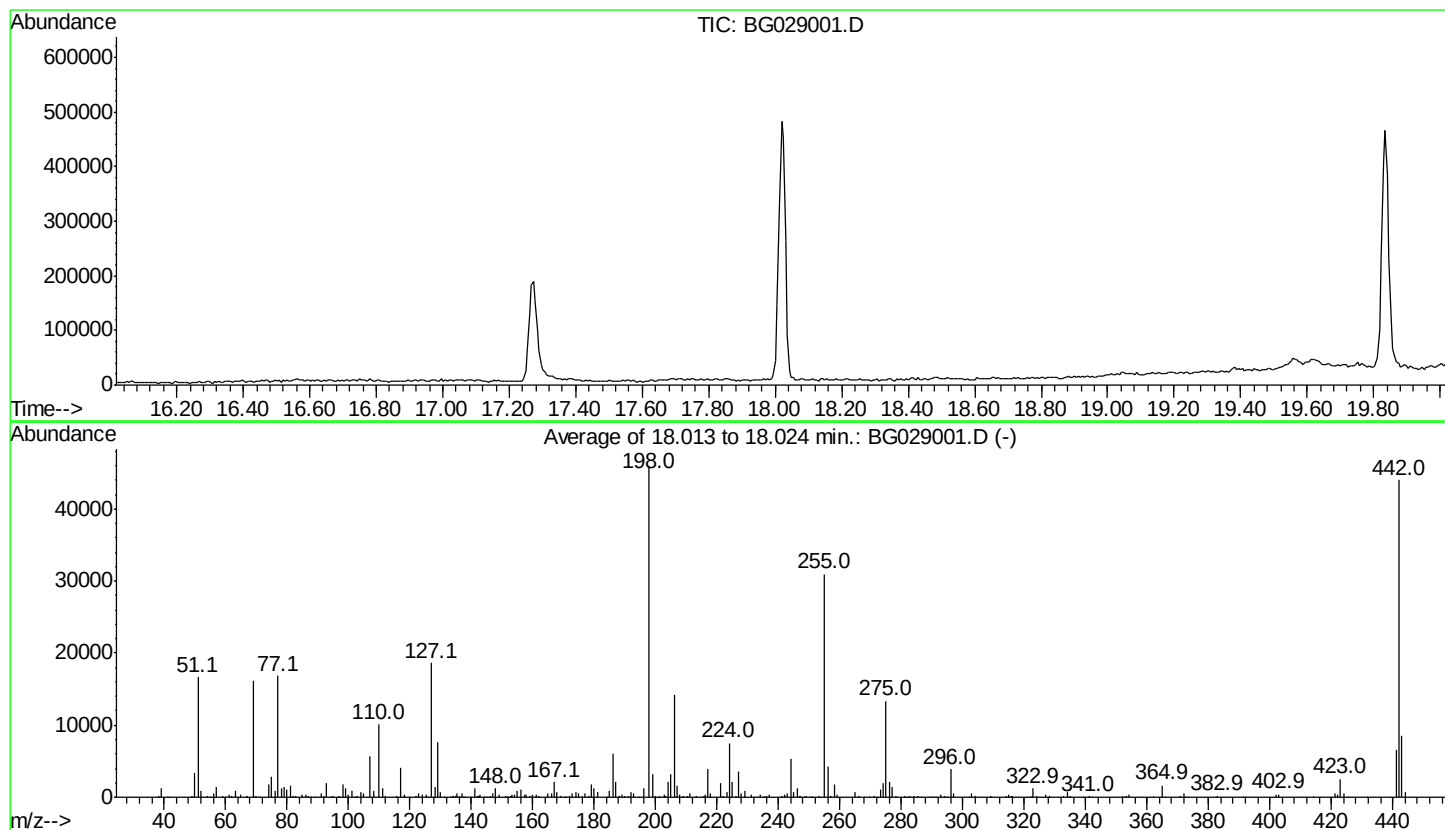

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.2	16632	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.1	16126	PASS
70	69	0.00	2	1.2	199	PASS
127	198	10	80	40.4	18586	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46008	PASS
199	198	5	9	7.0	3237	PASS
275	198	10	60	29.0	13329	PASS
365	198	1	100	3.5	1612	PASS
441	442	0.01	24	15.0	6605	PASS
442	198	50	100	95.7	44026	PASS
443	442	15	24	19.4	8560	PASS