


Data Path : Z:\HPCHEM1\BNA G\Data\BG100317\
 Data File : BG029017.D
 Acq On : 3 Oct 2017 22:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG091217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 16:57:11 2017

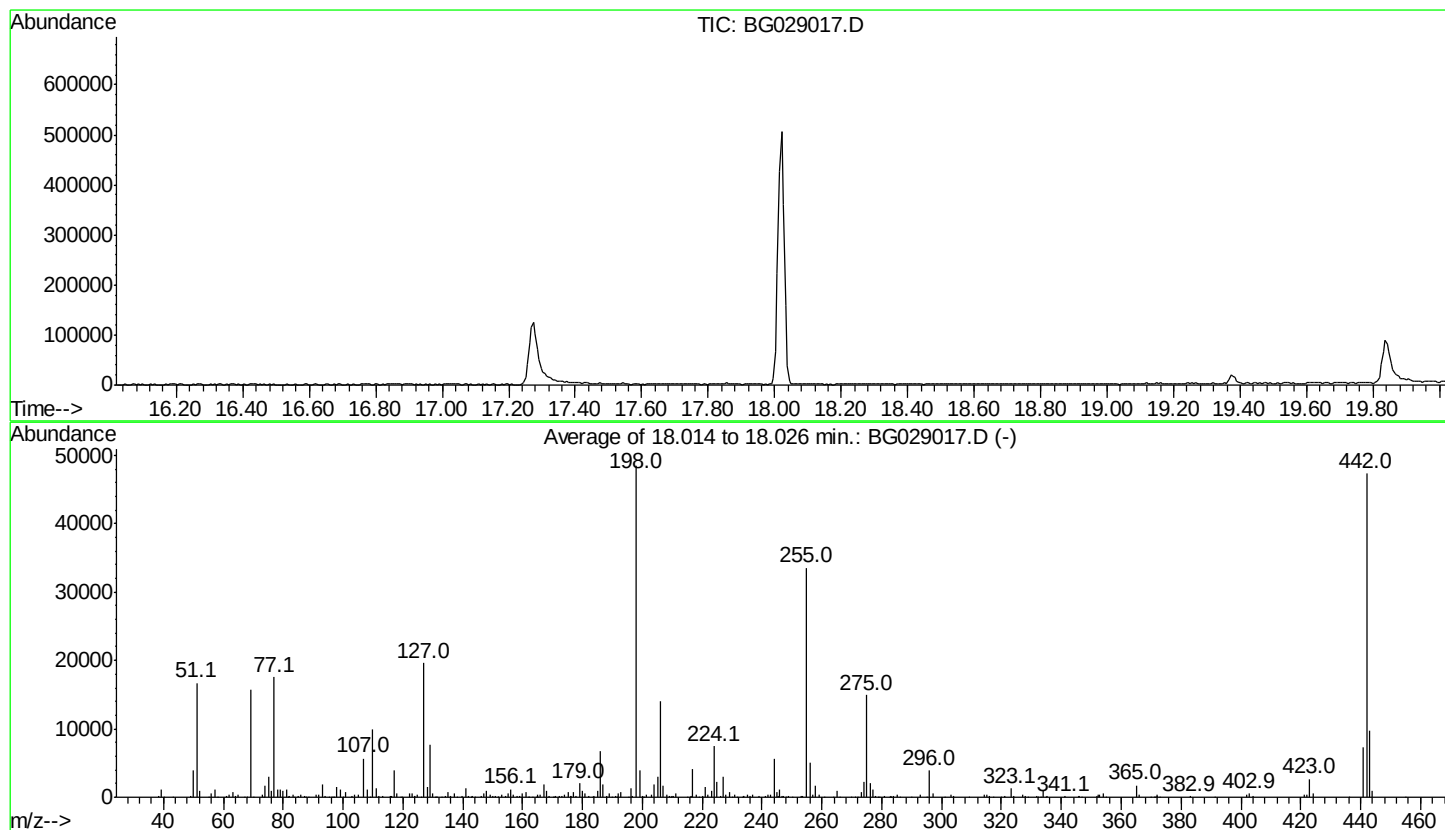

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	16725	PASS
68	69	0.00	2	0.6	97	PASS
69	198	0.00	100	32.4	15691	PASS
70	69	0.00	2	0.5	76	PASS
127	198	10	80	40.5	19610	PASS
197	198	0.00	2	0.3	163	PASS
198	198	100	100	100.0	48474	PASS
199	198	5	9	8.1	3920	PASS
275	198	10	60	30.7	14893	PASS
365	198	1	100	3.6	1730	PASS
441	442	0.01	24	15.5	7329	PASS
442	198	50	100	97.6	47290	PASS
443	442	15	24	20.5	9687	PASS