


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100319\
 Data File : BG043010.D
 Acq On : 3 Oct 2019 13:11
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

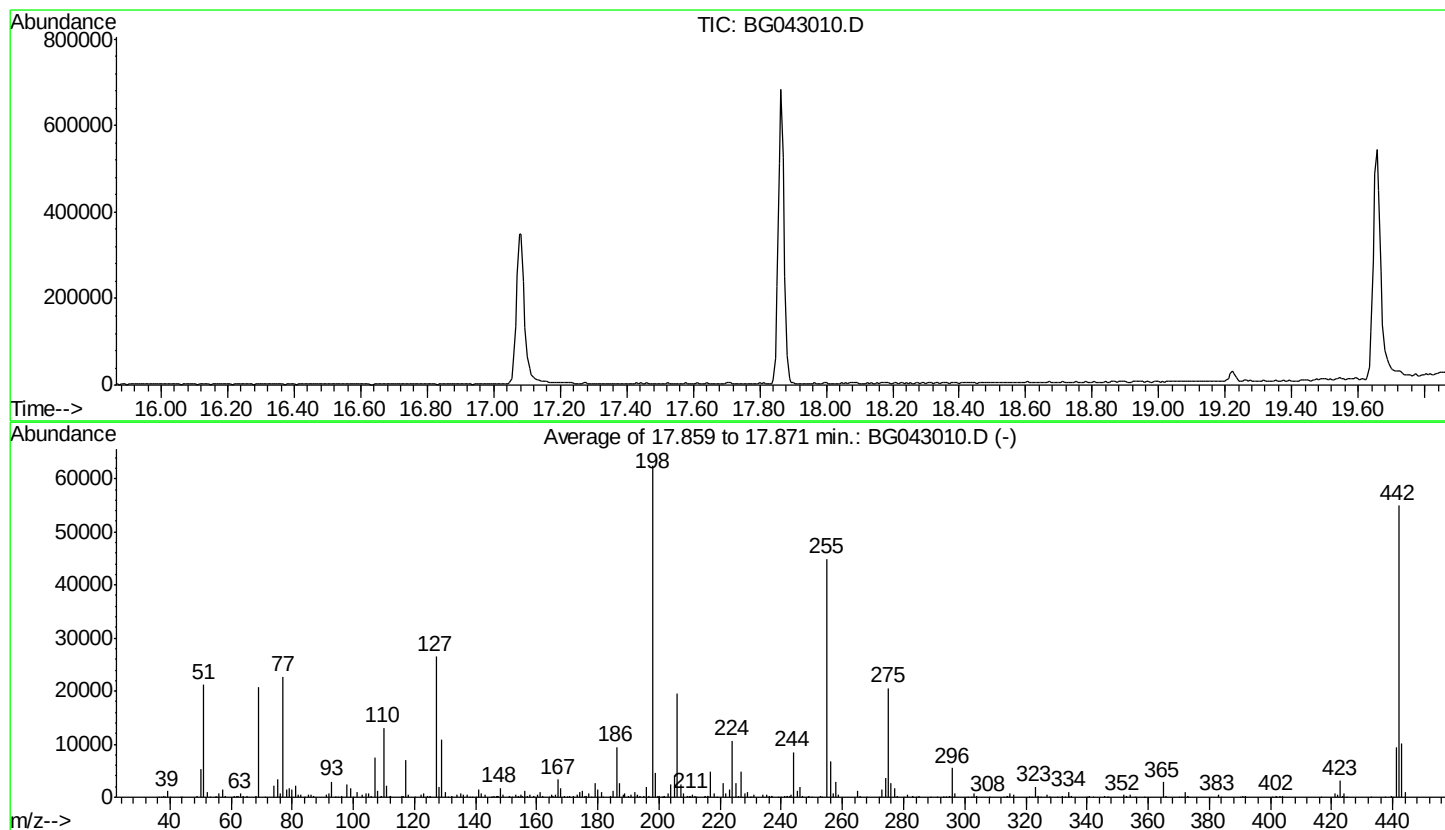

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2508

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	21125	PASS
68	69	0.00	2	1.1	226	PASS
69	198	0.00	100	33.4	20861	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.3	26440	PASS
197	198	0.00	2	0.3	206	PASS
198	198	100	100	100.0	62490	PASS
199	198	5	9	7.2	4474	PASS
275	198	10	60	33.0	20610	PASS
365	198	1	100	4.5	2828	PASS
441	198	0.01	100	15.0	9356	PASS
442	198	50	100	87.9	54922	PASS
443	442	15	24	18.5	10177	PASS