


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100319\
 Data File : BG043019.D
 Acq On : 4 Oct 2019 1:05
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 25 15:35:52 2019

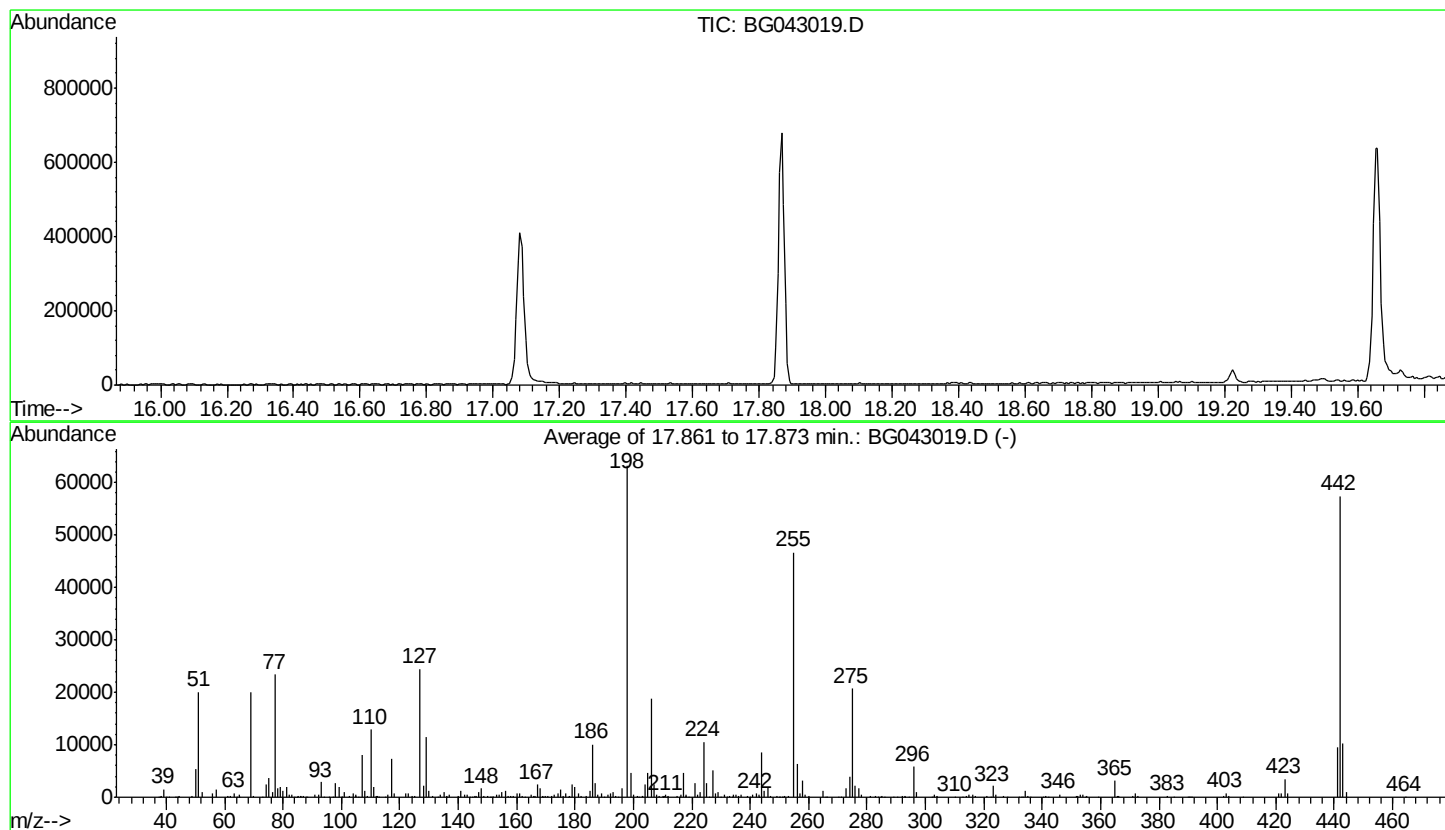

AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.7	20060	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.7	20053	PASS
70	69	0.00	2	0.8	155	PASS
127	198	10	80	38.6	24410	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63226	PASS
199	198	5	9	7.5	4730	PASS
275	198	10	60	32.7	20672	PASS
365	198	1	100	4.9	3077	PASS
441	198	0.01	100	15.2	9602	PASS
442	198	50	100	90.9	57464	PASS
443	442	15	24	18.0	10356	PASS