

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100415\
 Data File : BG019009.D
 Acq On : 4 Oct 2015 17:47
 Operator : UM/NP
 Sample : G3851-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0GG8

Quant Time: Oct 05 01:30:03 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 01:17:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	36166	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	153975	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	94635	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	227421	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	283518	20.00	ng/ul	-0.01
86) Perylene-d12	24.89	264	280148	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.50	96	860	1.07	ng/uL	0.00
5) Phenol-d5	7.20	99	19781	6.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	56723	28.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	54461	23.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	37240	15.19	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	33356	28.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	35207	29.77	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	64506	26.97	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	5183	1.78	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	220491	29.63	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	268899	29.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.83	143	8609	5.81	ng/ul	-0.01
58) Fluorene-d10	15.66	176	195916	29.06	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	32795	27.14	ng/ul	0.00
71) Anthracene-d10	17.51	188	319395	29.68	ng/ul	0.00
79) Pyrene-d10	19.79	212	382467	28.88	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.67	264	424762	29.66	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.12	163	23862	3.14	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100415\
Data File : BG019009.D
Acq On : 4 Oct 2015 17:47
Operator : UM/NP
Sample : G3851-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0GG8

Quant Time: Oct 05 01:30:03 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 01:17:08 2015
Response via : Initial Calibration

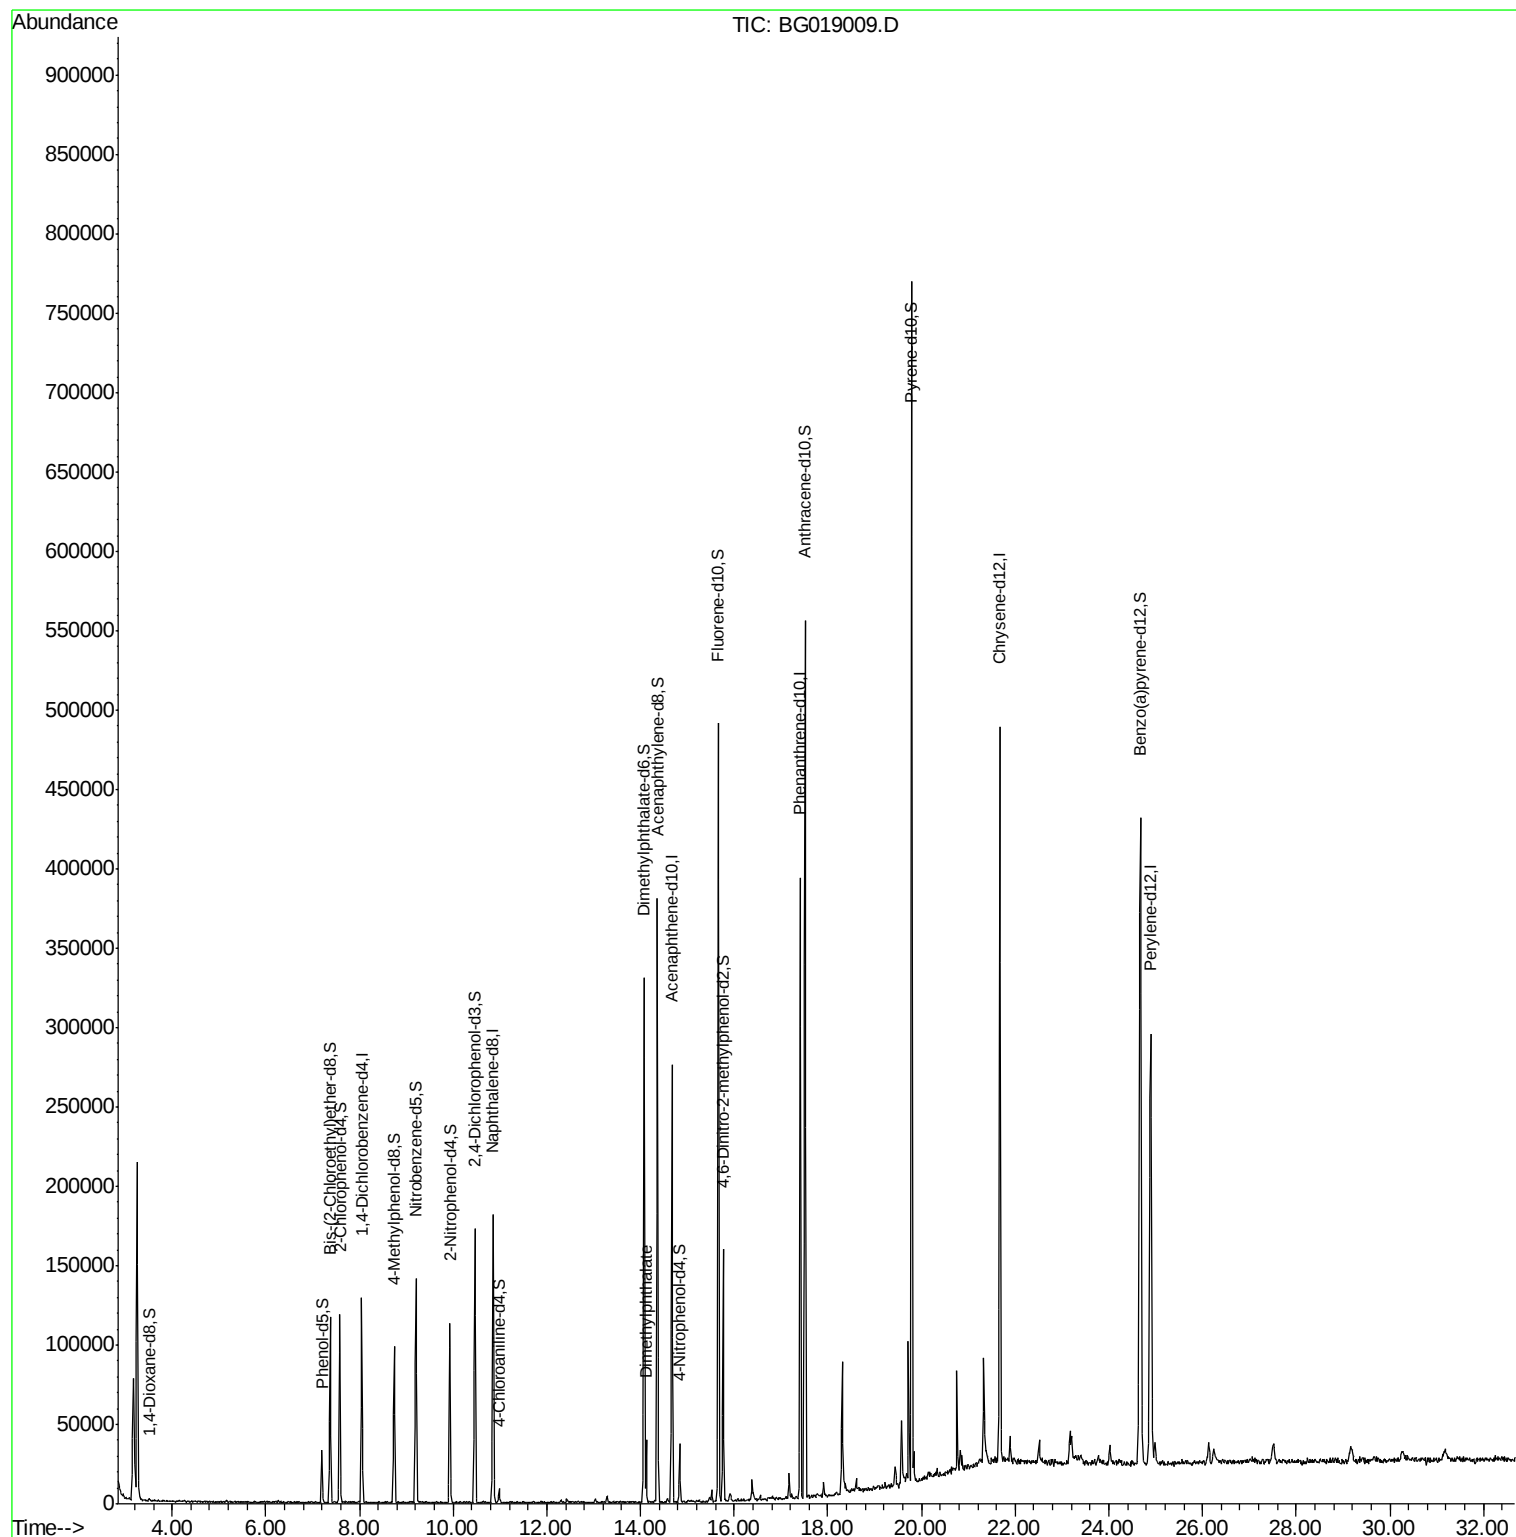


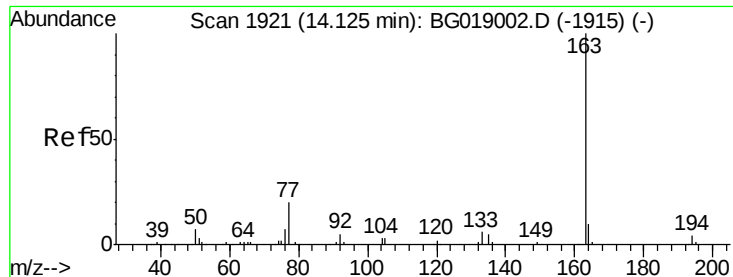

#45
 Dimethylphthalate
 Concen: 3.14 ng/ul
 RT: 14.12 min Scan# 1920
 Delta R.T. -0.00 min
 Lab File: BG019009.D
 Acq: 4 Oct 2015 17:47

Instrument :
 BNA_G
 ClientSampleId :
 C0GG8

Tgt Ion:163 Resp: 23862
 Ion Ratio Lower Upper
 163 100
 194 3.3 3.3 4.9
 164 10.7 8.1 12.1

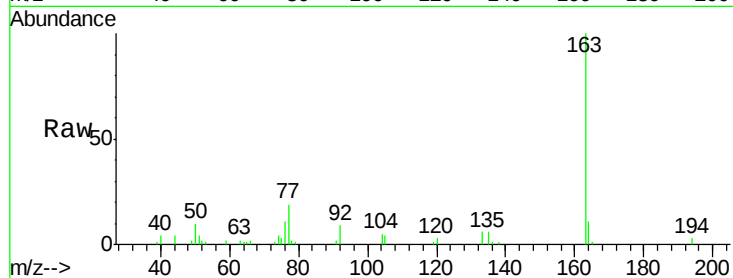

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

