

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100415\
 Data File : BG019010.D
 Acq On : 4 Oct 2015 18:25
 Operator : UM/NP
 Sample : G3851-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0GG9

Quant Time: Oct 05 01:33:17 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 01:17:08 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	37409	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	157808	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	98903	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	234176	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	291754	20.00	ng/ul	0.00
86) Perylene-d12	24.90	264	284465	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.51	96	341	0.41	ng/uL	0.00
5) Phenol-d5	7.20	99	8415	2.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	21747	10.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	21637	8.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	15661	6.17	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	12482	10.51	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	12805	10.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	25173	10.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	1356	0.45	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	86817	11.16	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	102106	10.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	3527	2.28	ng/ul	0.00
58) Fluorene-d10	15.66	176	76607	10.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	11492	9.24	ng/ul	0.00
71) Anthracene-d10	17.51	188	122132	11.02	ng/ul	0.00
79) Pyrene-d10	19.79	212	147703	10.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.67	264	157002	10.80	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.12	163	27154	3.42	ng/ul	99




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100415\
Data File : BG019010.D
Acq On : 4 Oct 2015 18:25
Operator : UM/NP
Sample : G3851-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0GG9

Quant Time: Oct 05 01:33:17 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 01:17:08 2015
Response via : Initial Calibration

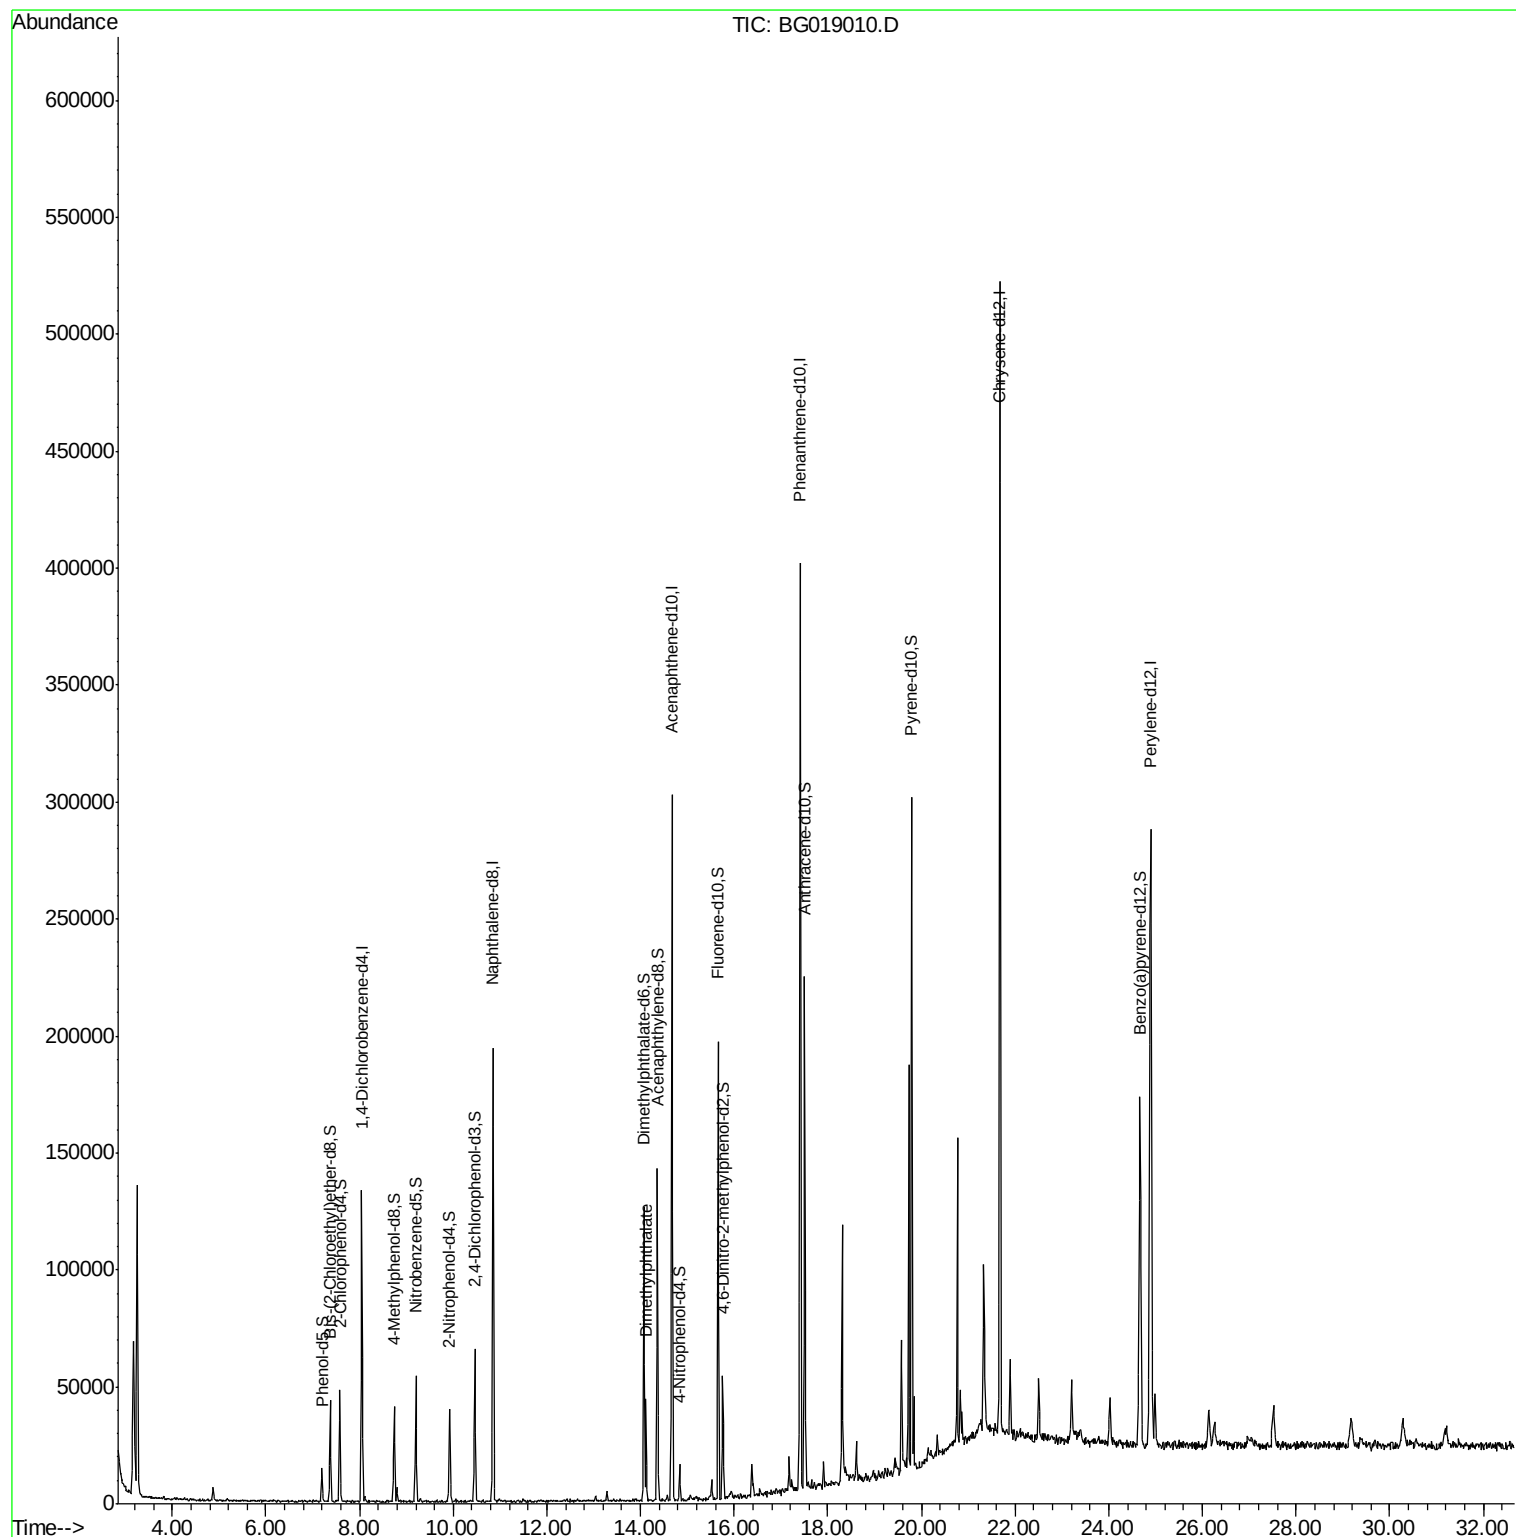

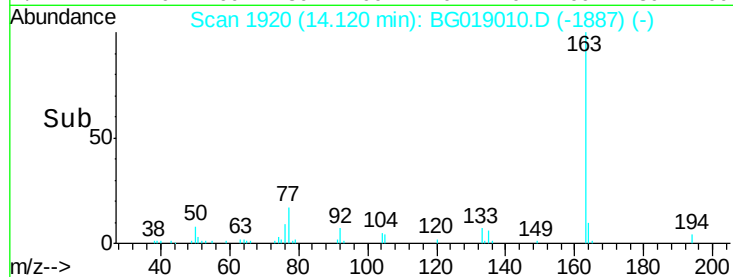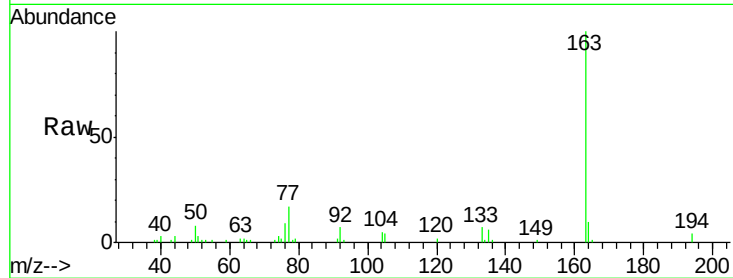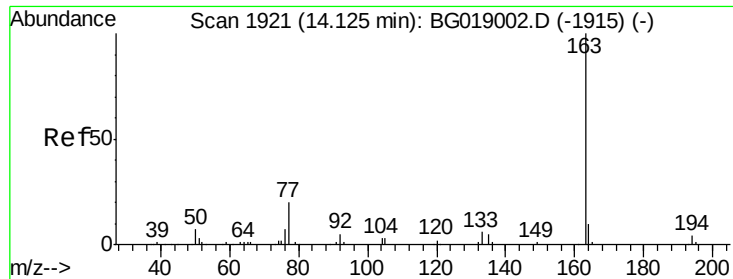

#45

Dimethylphthalate

Concen: 3.42 ng/ul

RT: 14.12 min Scan# 1920

Delta R.T. -0.01 min

Lab File: BG019010.D

Acq: 4 Oct 2015 18:25

Instrument :

BNA_G

ClientSampleId :

C0GG9

Tgt Ion:163 Resp: 27154

Ion Ratio Lower Upper

163 100

194 3.6 3.3 4.9

164 10.0 8.1 12.1

