

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100415\
 Data File : BG019021.D
 Acq On : 5 Oct 2015 1:20
 Operator : UM/NP
 Sample : G3831-08DL 50X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AR5DL

Quant Time: Oct 05 02:26:44 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 05 02:06:27 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	25758	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	106180	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	68133	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	169624	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	218691	20.00	ng/ul	0.00
86) Perylene-d12	24.89	264	208942	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.20	99	128	0.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	830	0.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	619	0.37	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	265	0.15	ng/ul	0.00
19) Nitrobenzene-d5	9.21	128	183	0.23	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	154	0.19	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	836	0.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.86	131	82	0.04	ng/ul	-0.12
44) Dimethylphthalate-d6	14.07	166	2718	0.51	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	3300	0.50	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.66	176	2971	0.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	70	0.08	ng/ul	0.00
71) Anthracene-d10	17.41	188	169624	21.24	ng/ul	-0.10
79) Pyrene-d10	19.79	212	5577	0.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.67	264	5342	0.50	ng/ul	0.00

Target Compounds


						Qvalue
11) 2-Methylphenol	8.40	108	3471	1.99	ng/ul	88
20) Nitrobenzene	9.25	77	40799	20.42	ng/ul	99
30) 4-Chloroaniline	10.95	127	8541	4.10	ng/ul	95
37) 1,2,4,5-Tetrachlorobenzene	12.87	216	2783	1.26	ng/ul	95
73) 1,2,3,4-Tetrachlorobenzene	13.47	216	3161	1.38	ng/uL	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100415\
Data File : BG019021.D
Acq On : 5 Oct 2015 1:20
Operator : UM/NP
Sample : G3831-08DL 50X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AR5DL

Quant Time: Oct 05 02:26:44 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 05 02:06:27 2015
Response via : Initial Calibration

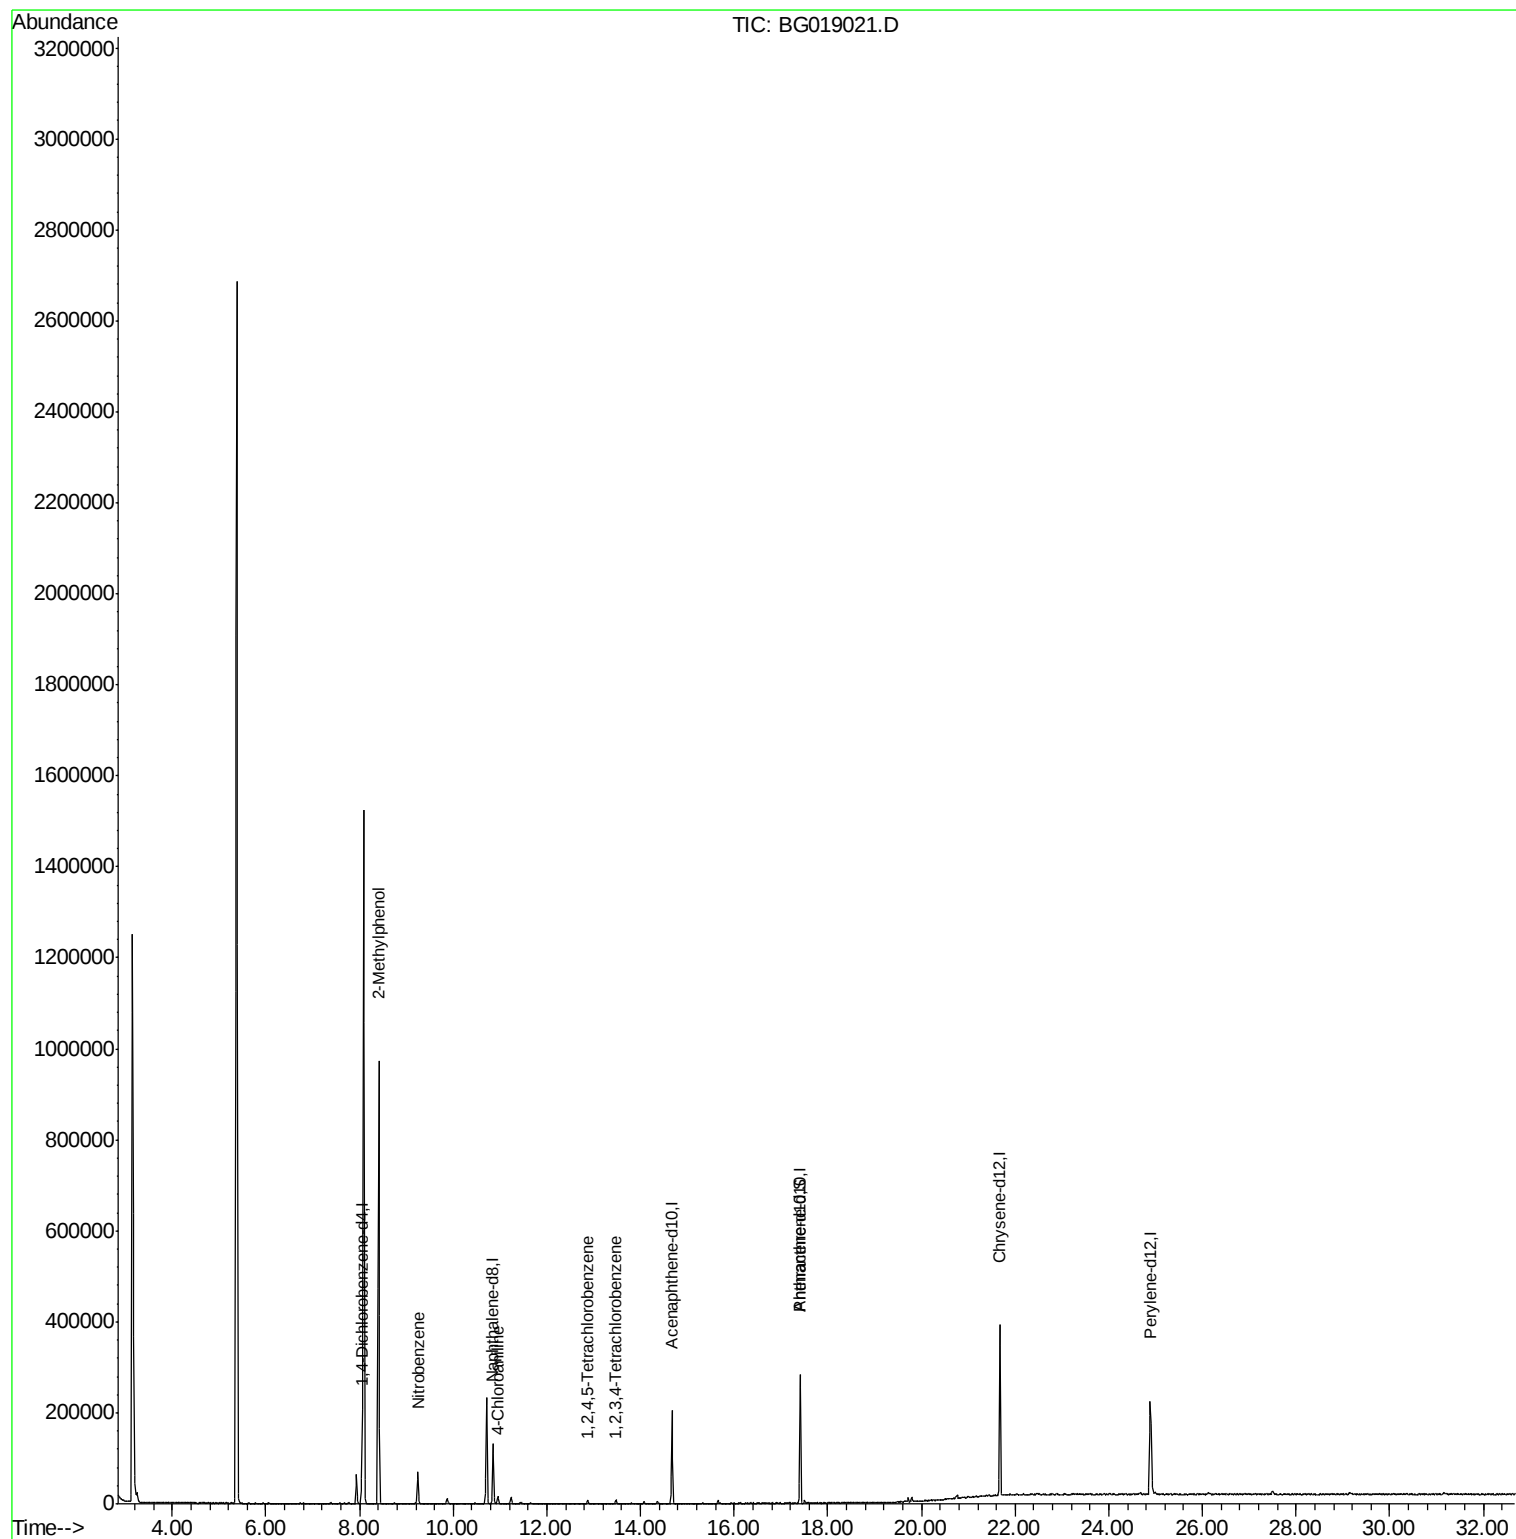


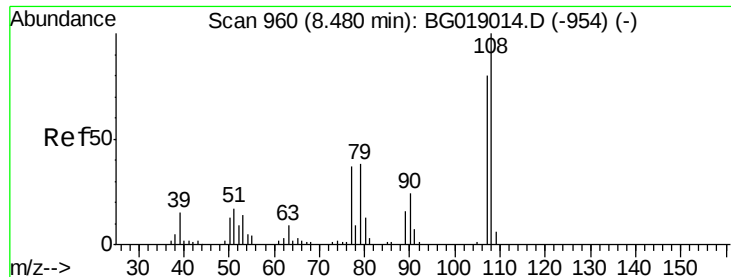




#11
2-Methylphenol
Concen: 1.99 ng/ul
RT: 8.40 min Scan# 947
Delta R.T. -0.08 min
Lab File: BG019021.D
Acq: 5 Oct 2015 1:20

Instrument :
BNA_G
ClientSampleId :
C0AR5DL

Tgt Ion: 108 Resp: 3471
Ion Ratio Lower Upper
108 100
107 84.2 76.7 115.1

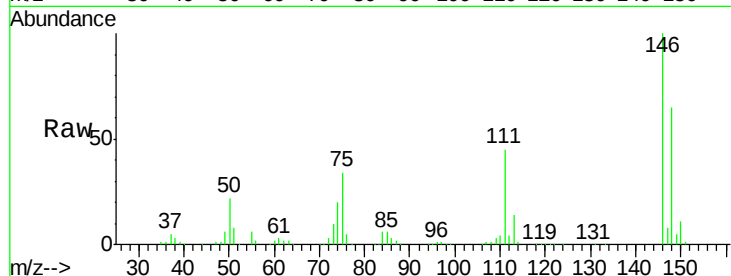


Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E

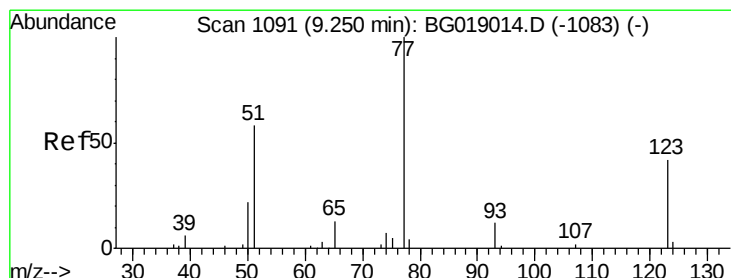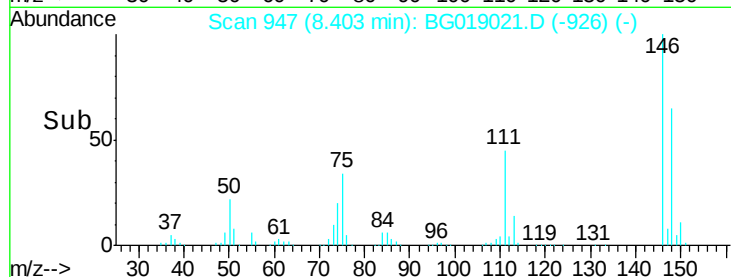
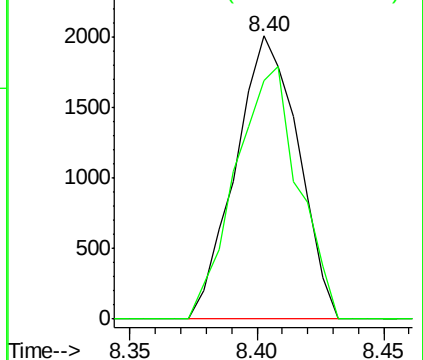



#20
Nitrobenzene
Concen: 20.42 ng/ul
RT: 9.25 min Scan# 1091
Delta R.T. -0.00 min
Lab File: BG019021.D
Acq: 5 Oct 2015 1:20

Tgt Ion: 77 Resp: 40799
Ion Ratio Lower Upper
77 100
123 40.3 32.6 48.8
65 14.0 10.6 15.8

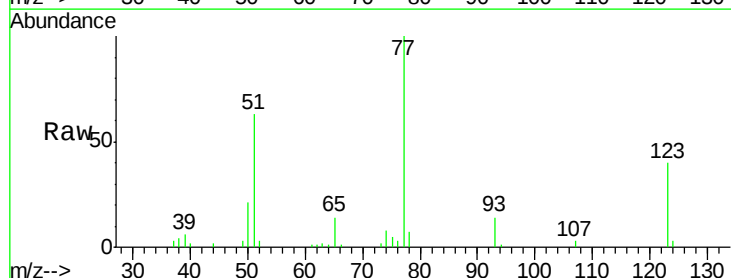

Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 123.00 (122.70 to 123.70): E
Ion 65.00 (64.70 to 65.70): BGC

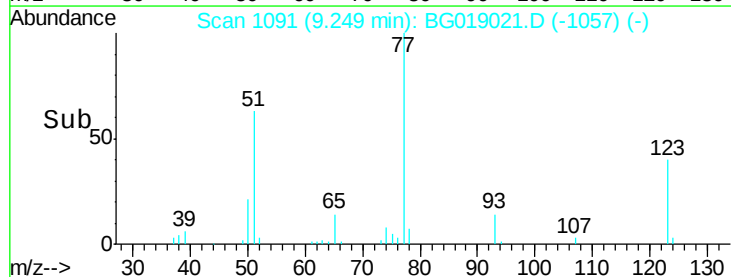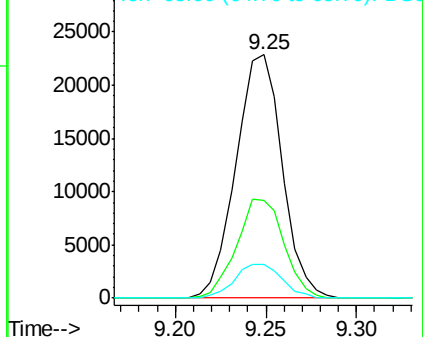


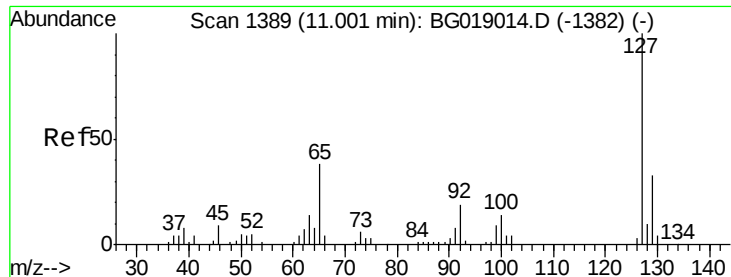


#30
 4-Chloroaniline
 Concen: 4.10 ng/ul
 RT: 10.95 min Scan# 1381
 Delta R.T. -0.05 min
 Lab File: BG019021.D
 Acq: 5 Oct 2015 1:20

Instrument :
 BNA_G
 ClientSampleId :
 C0AR5DL



Tgt Ion:127 Resp: 8541
 Ion Ratio Lower Upper
 127 100
 129 33.2 24.3 36.5

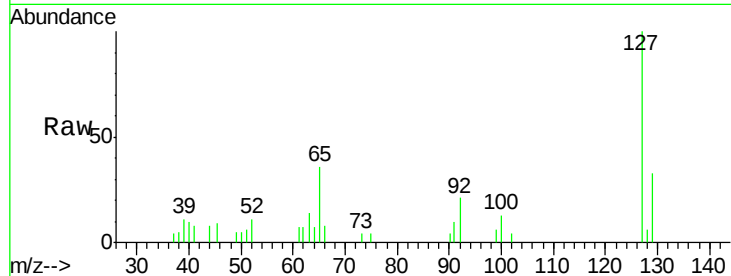

Abundance Ion 127.00 (126.70 to 127.70): E
 Ion 129.00 (128.70 to 129.70): E

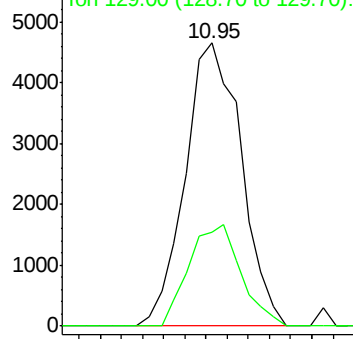


Time-->

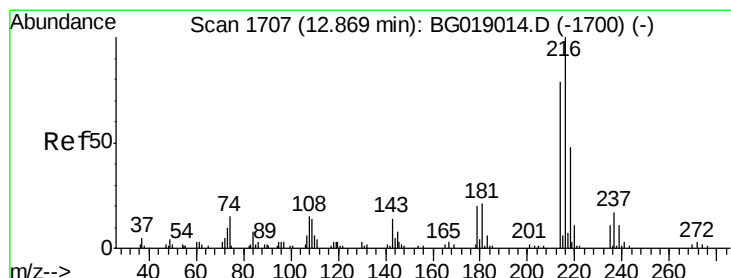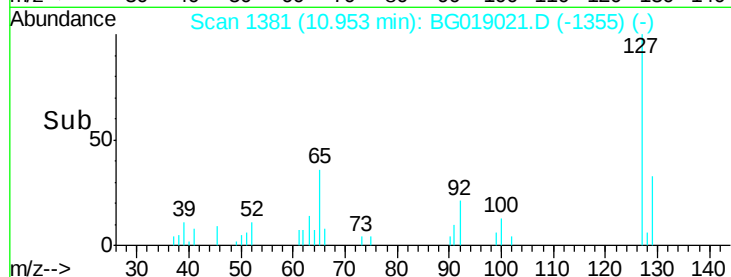


#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 1.26 ng/ul
 RT: 12.87 min Scan# 1707
 Delta R.T. -0.00 min
 Lab File: BG019021.D
 Acq: 5 Oct 2015 1:20


Tgt Ion:216 Resp: 2783
 Ion Ratio Lower Upper
 216 100
 214 82.9 62.6 94.0
 179 18.5 14.6 22.0
 108 18.9 12.9 19.3

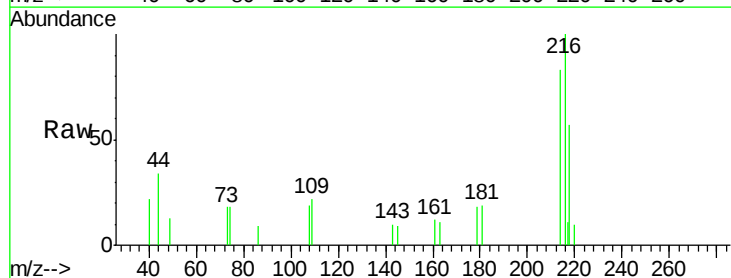


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 108.00 (107.70 to 108.70): E

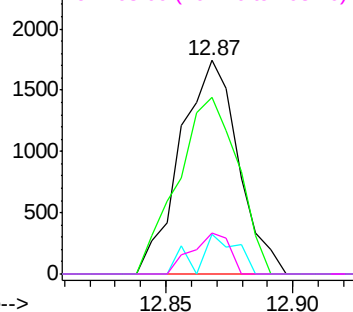

Time-->

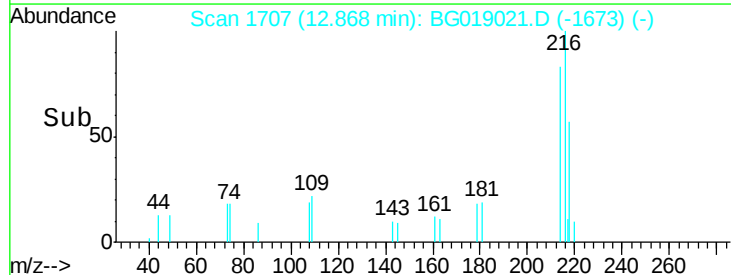

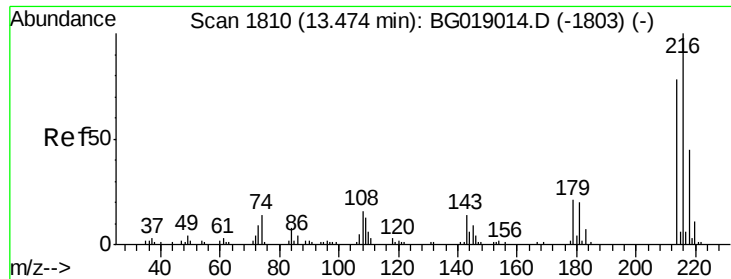

#73

1,2,3,4-Tetrachlorobenzene

Concen: 1.38 ng/uL

RT: 13.47 min Scan# 1809

Delta R.T. -0.01 min

Lab File: BG019021.D


Acq: 5 Oct 2015 1:20

Instrument :

BNA_G

ClientSampleId :

C0AR5DL

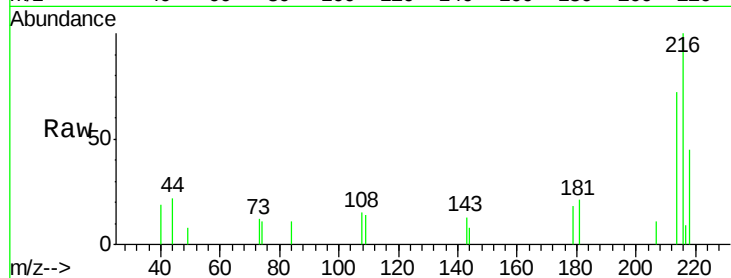


Tgt Ion: 216 Resp: 3161

Ion Ratio Lower Upper

216 100

214 71.9 64.5 96.7

218 45.3 40.4 60.6

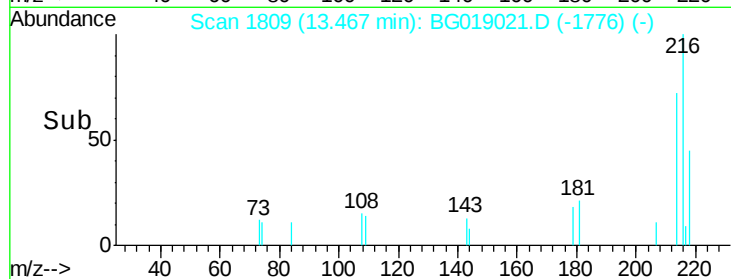

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

