

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050408.D
 Acq On : 4 Oct 2021 10:38
 Operator : CG/JU
 Sample : PB139386BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK386

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.638	20	25	33	rVB2	14797	26454	2.14%	0.187%
2	3.838	58	59	63	rVB4	1552	1295	0.10%	0.009%
3	3.873	63	65	68	rVB3	1213	1371	0.11%	0.010%
4	3.944	75	77	79	rBV3	1080	1244	0.10%	0.009%
5	3.985	82	84	87	rBV3	1018	1325	0.11%	0.009%
6	4.061	92	97	116	rBV	187888	360679	29.15%	2.554%
7	4.214	122	123	128	rVB2	1127	1323	0.11%	0.009%
8	4.396	152	154	155	rVV2	1862	1848	0.15%	0.013%
9	4.408	155	156	160	rVB2	3379	3091	0.25%	0.022%
10	4.602	184	189	193	rBV5	1050	1678	0.14%	0.012%
11	5.213	291	293	298	rVB3	866	1337	0.11%	0.009%
12	6.071	434	439	442	rVB3	819	1616	0.13%	0.011%
13	6.200	456	461	462	rBV2	1007	1317	0.11%	0.009%
14	7.404	659	666	674	rVV	252252	441680	35.70%	3.128%
15	7.586	690	697	705	rBV	182339	312287	25.24%	2.212%
16	7.798	726	733	742	rBV	239120	417827	33.77%	2.959%
17	8.274	807	814	822	rVB	175964	299374	24.20%	2.120%
18	8.961	922	931	946	rVB	285682	519638	42.00%	3.680%
19	9.443	1005	1013	1023	rBV	239349	423571	34.23%	3.000%
20	10.172	1126	1137	1146	rBV	183387	338529	27.36%	2.398%
21	10.706	1219	1228	1237	rBV	283844	512923	41.45%	3.633%
22	11.100	1286	1295	1308	rBV	239954	442380	35.75%	3.133%
23	11.223	1308	1316	1325	rVB	276650	523528	42.31%	3.708%
24	12.663	1554	1561	1567	rVB3	5044	8525	0.69%	0.060%
25	14.284	1830	1837	1844	rVB	482497	713898	57.70%	5.056%
26	14.590	1880	1889	1898	rVB	533973	877677	70.93%	6.216%
27	14.766	1915	1919	1923	rVB2	754	1269	0.10%	0.009%
28	14.807	1923	1926	1928	rBV3	905	1274	0.10%	0.009%
29	14.890	1930	1940	1949	rVB	358081	590883	47.76%	4.185%
30	15.054	1961	1968	1977	rBV	243425	398021	32.17%	2.819%
31	15.877	2101	2108	2115	rBV	678723	1061499	85.79%	7.518%
32	15.982	2120	2126	2135	rBV	142695	219134	17.71%	1.552%
33	16.118	2145	2149	2153	rBV	6780	8965	0.72%	0.063%
34	17.069	2309	2311	2315	rBV4	959	1270	0.10%	0.009%
35	17.416	2367	2370	2375	rBV2	2051	3261	0.26%	0.023%
36	17.633	2400	2407	2417	rVV	441574	688683	55.66%	4.877%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050408.D
 Acq On : 4 Oct 2021 10:38
 Operator : CG/JU
 Sample : PB139386BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK386

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	17.733	2417	2424	2432	rVV	755385	1128129	91.18%	7.990%
38	17.868	2440	2447	2453	rBV5	9475	17573	1.42%	0.124%
39	17.998	2466	2469	2471	rBV2	1464	1521	0.12%	0.011%
40	18.021	2471	2473	2475	rVV	1511	1558	0.13%	0.011%
41	18.121	2488	2490	2494	rVB4	1524	2305	0.19%	0.016%
42	18.162	2494	2497	2499	rBV3	1636	2045	0.17%	0.014%
43	18.609	2567	2573	2575	rBV4	1023	1917	0.15%	0.014%
44	18.767	2599	2600	2602	rBV	1750	1315	0.11%	0.009%
45	18.809	2605	2607	2610	rVV5	1453	1458	0.12%	0.010%
46	18.844	2612	2613	2616	rBV2	1925	2006	0.16%	0.014%
47	18.885	2619	2620	2626	rVV5	1426	1883	0.15%	0.013%
48	19.008	2640	2641	2645	rBV3	1902	2385	0.19%	0.017%
49	19.085	2653	2654	2657	rBV3	2039	1580	0.13%	0.011%
50	19.126	2659	2661	2663	rBV3	1317	1252	0.10%	0.009%
51	19.472	2717	2720	2721	rVB3	2445	1914	0.15%	0.014%
52	19.496	2721	2724	2726	rBV4	2236	2777	0.22%	0.020%
53	19.572	2733	2737	2743	rBV7	8844	13760	1.11%	0.097%
54	19.643	2745	2749	2754	rVB3	10752	15962	1.29%	0.113%
55	19.896	2790	2792	2795	rBV4	3465	3538	0.29%	0.025%
56	20.007	2805	2811	2819	rVB2	846771	1237317	100.00%	8.763%
57	20.448	2884	2886	2889	rBV4	4979	3615	0.29%	0.026%
58	21.940	3133	3140	3147	rVB	376960	666098	53.83%	4.718%
59	25.131	3672	3683	3695	rVB3	383715	1103810	89.21%	7.818%
60	25.371	3714	3724	3735	rVB3	213372	693209	56.03%	4.910%




Sum of corrected areas: 14119601

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050408.D
Acq On : 4 Oct 2021 10:38
Operator : CG/JU
Sample : PB139386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

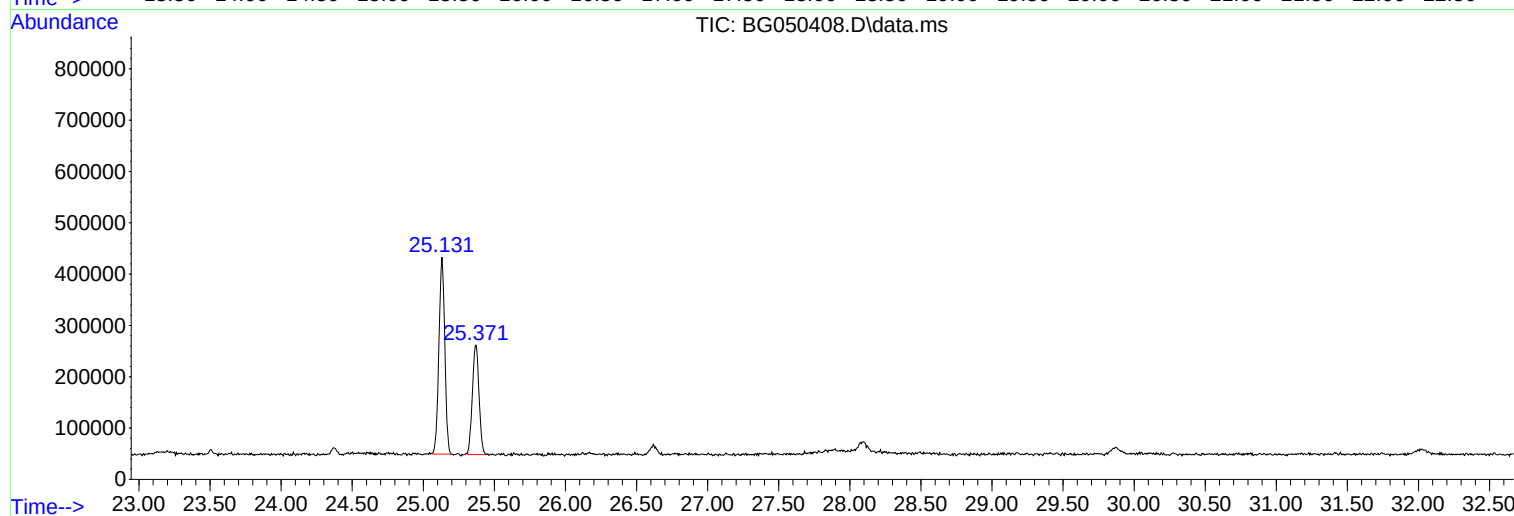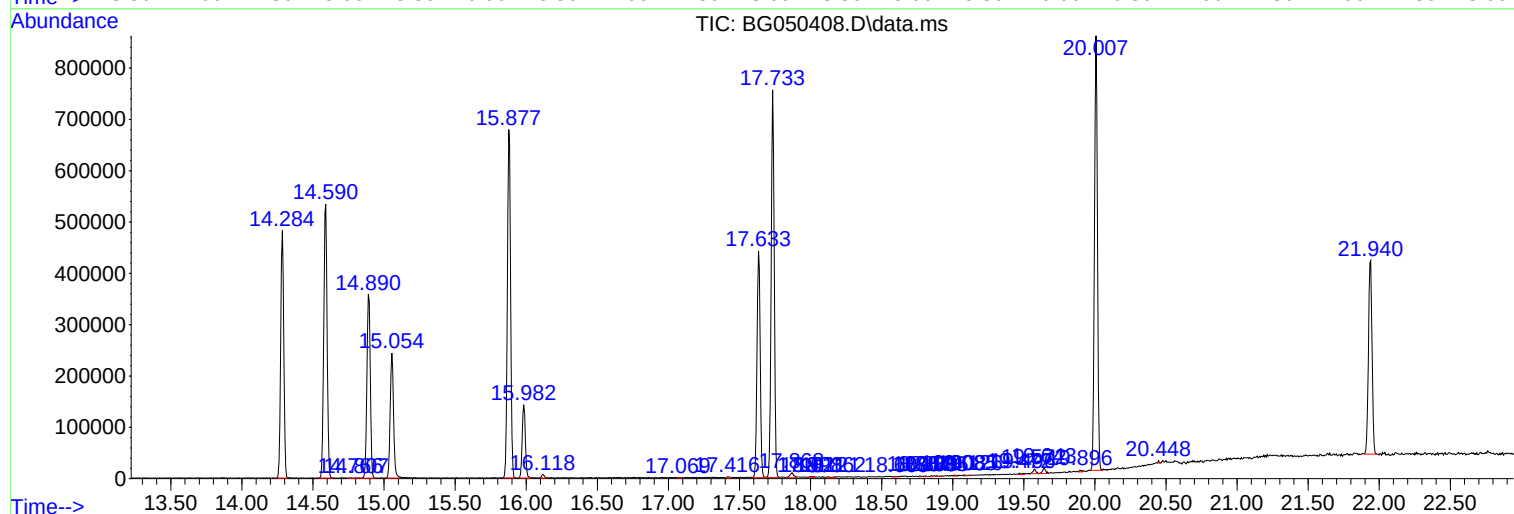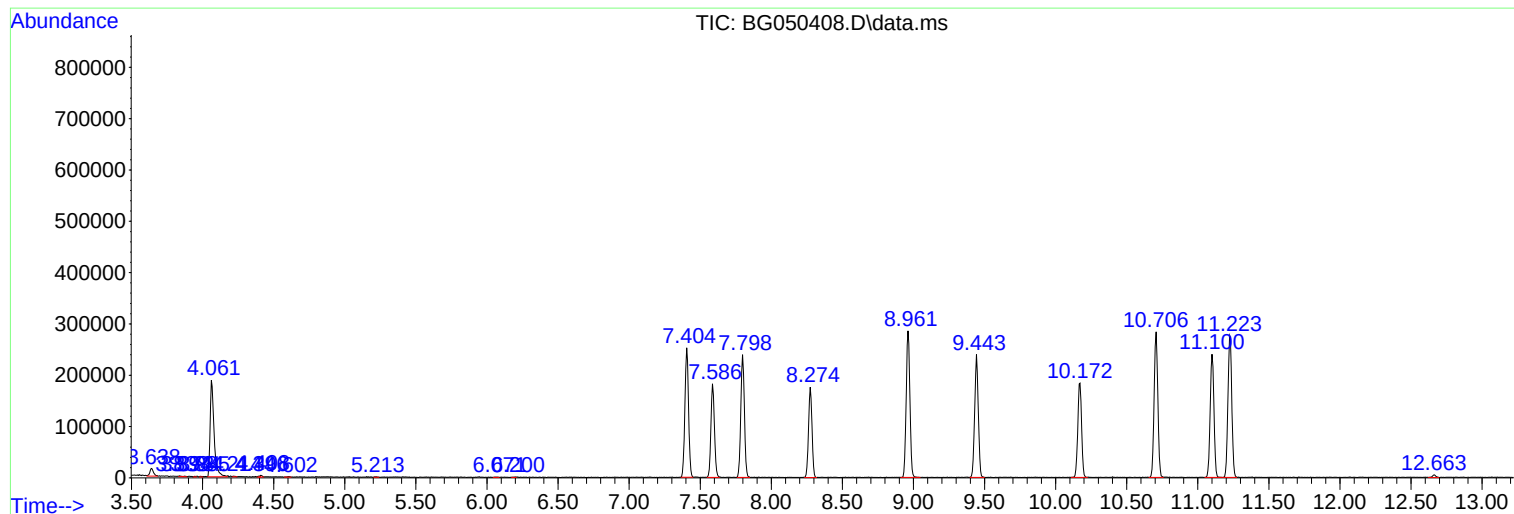

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050408.D
Acq On : 4 Oct 2021 10:38
Operator : CG/JU
Sample : PB139386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050408.D
Acq On : 4 Oct 2021 10:38
Operator : CG/JU
Sample : PB139386BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK386

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------