

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050422.D
 Acq On : 4 Oct 2021 21:03
 Operator : CG/JU
 Sample : PB139387BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK387

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.641	21	26	35	rVB2	16461	32724	2.62%	0.226%
2	4.064	93	98	119	rVV	180782	350504	28.09%	2.424%
3	4.405	153	156	162	rVB3	3857	6042	0.48%	0.042%
4	4.581	184	186	192	rBV4	1306	1809	0.14%	0.013%
5	4.810	224	225	232	rVB3	1104	1656	0.13%	0.011%
6	5.874	402	406	409	rBV3	936	1749	0.14%	0.012%
7	7.184	625	629	634	rVB5	874	1454	0.12%	0.010%
8	7.401	658	666	674	rBV	243085	424844	34.05%	2.938%
9	7.584	690	697	713	rVB	174991	298630	23.93%	2.065%
10	7.795	725	733	743	rBV	220072	396375	31.76%	2.741%
11	8.112	784	787	792	rBV4	784	1658	0.13%	0.011%
12	8.271	807	814	821	rVB	200885	349212	27.98%	2.415%
13	8.958	923	931	940	rVV	273963	494881	39.66%	3.422%
14	9.440	1005	1013	1022	rBV	223640	408231	32.71%	2.823%
15	10.163	1129	1136	1147	rVB	184054	337270	27.03%	2.332%
16	10.698	1219	1227	1235	rVV	271014	487020	39.03%	3.368%
17	11.091	1286	1294	1303	rBV	260039	499366	40.02%	3.453%
18	11.220	1308	1316	1326	rVB	268994	497674	39.88%	3.441%
19	11.608	1379	1382	1385	rBV2	810	1319	0.11%	0.009%
20	12.660	1555	1561	1565	rBV	5621	8311	0.67%	0.057%
21	13.847	1760	1763	1768	rBV2	1037	2016	0.16%	0.014%
22	14.276	1830	1836	1845	rBV	463522	694664	55.67%	4.803%
23	14.352	1845	1849	1852	rVB3	858	1356	0.11%	0.009%
24	14.581	1881	1888	1896	rBV	521511	847532	67.92%	5.860%
25	14.887	1933	1940	1950	rBV	425834	668712	53.59%	4.624%
26	15.045	1961	1967	1981	rBV	245957	401616	32.18%	2.777%
27	15.874	2101	2108	2117	rVB	658585	1024776	82.12%	7.086%
28	15.974	2120	2125	2136	rVB	176737	265427	21.27%	1.835%
29	16.109	2141	2148	2153	rBV3	6530	10494	0.84%	0.073%
30	16.444	2201	2205	2206	rBV2	1025	1304	0.10%	0.009%
31	17.413	2369	2370	2374	rVV2	2431	1457	0.12%	0.010%
32	17.631	2400	2407	2413	rBV	501486	787751	63.13%	5.447%
33	17.725	2416	2423	2431	rBV	681835	1081180	86.64%	7.476%
34	17.872	2442	2448	2452	rBV7	2542	5749	0.46%	0.040%
35	18.629	2574	2577	2579	rBV4	1224	1475	0.12%	0.010%
36	18.782	2600	2603	2604	rBV3	1238	1306	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050422.D
 Acq On : 4 Oct 2021 21:03
 Operator : CG/JU
 Sample : PB139387BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK387

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	18.841	2611	2613	2616	rBV3	1570	1691	0.14%	0.012%
38	18.923	2621	2627	2629	rBV2	1445	2451	0.20%	0.017%
39	19.047	2645	2648	2649	rBV3	1334	1251	0.10%	0.009%
40	19.129	2658	2662	2664	rBV2	2244	1895	0.15%	0.013%
41	19.170	2666	2669	2670	rVB3	1716	1715	0.14%	0.012%
42	19.188	2670	2672	2675	rBV2	1678	2536	0.20%	0.018%
43	19.340	2695	2698	2699	rBV3	1251	1314	0.11%	0.009%
44	19.458	2716	2718	2721	rVB4	1902	2003	0.16%	0.014%
45	19.487	2721	2723	2725	rBV3	2157	1626	0.13%	0.011%
46	19.564	2732	2736	2740	rVV5	8473	12001	0.96%	0.083%
47	19.640	2744	2749	2754	rVB3	9794	15603	1.25%	0.108%
48	19.769	2767	2771	2772	rBV3	2200	2415	0.19%	0.017%
49	19.787	2772	2774	2776	rBV2	1982	2214	0.18%	0.015%
50	19.822	2778	2780	2781	rBV2	2473	1673	0.13%	0.012%
51	19.863	2785	2787	2790	rVV3	2289	2589	0.21%	0.018%
52	19.893	2790	2792	2795	rVB4	3564	4112	0.33%	0.028%
53	19.934	2795	2799	2800	rBV4	2403	3291	0.26%	0.023%
54	19.998	2804	2810	2819	rVB	846431	1247874	100.00%	8.629%
55	20.210	2844	2846	2847	rBV	2809	2131	0.17%	0.015%
56	20.510	2895	2897	2899	rBV3	3230	3394	0.27%	0.023%
57	21.931	3132	3139	3147	rVB2	468439	821015	65.79%	5.677%
58	25.116	3670	3681	3692	rVB2	380674	1103179	88.40%	7.628%
59	25.351	3710	3721	3734	rBV	264472	822706	65.93%	5.689%
60	27.601	4102	4104	4105	rBV2	6877	3916	0.31%	0.027%




Sum of corrected areas: 14462139

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050422.D
Acq On : 4 Oct 2021 21:03
Operator : CG/JU
Sample : PB139387BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

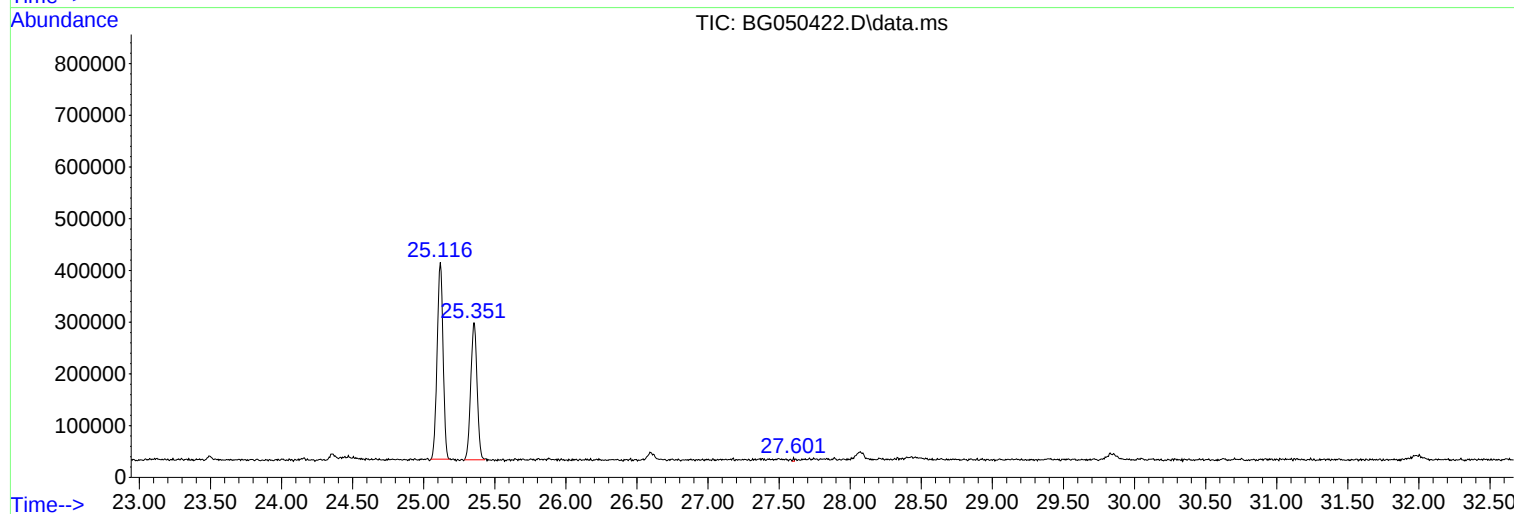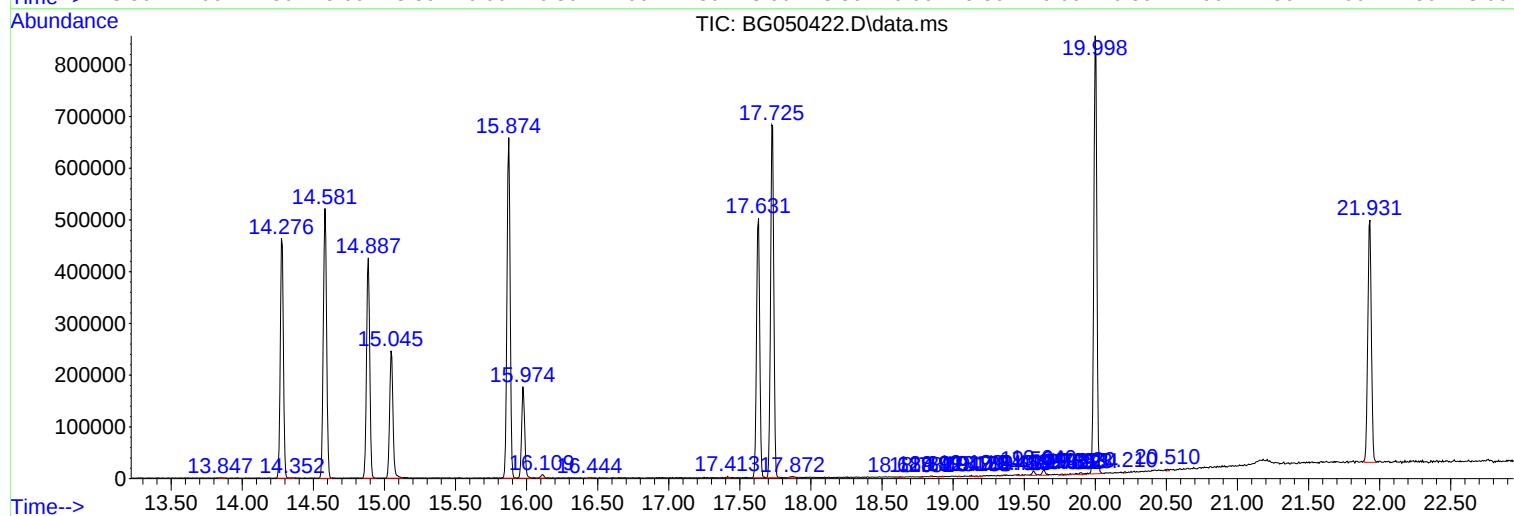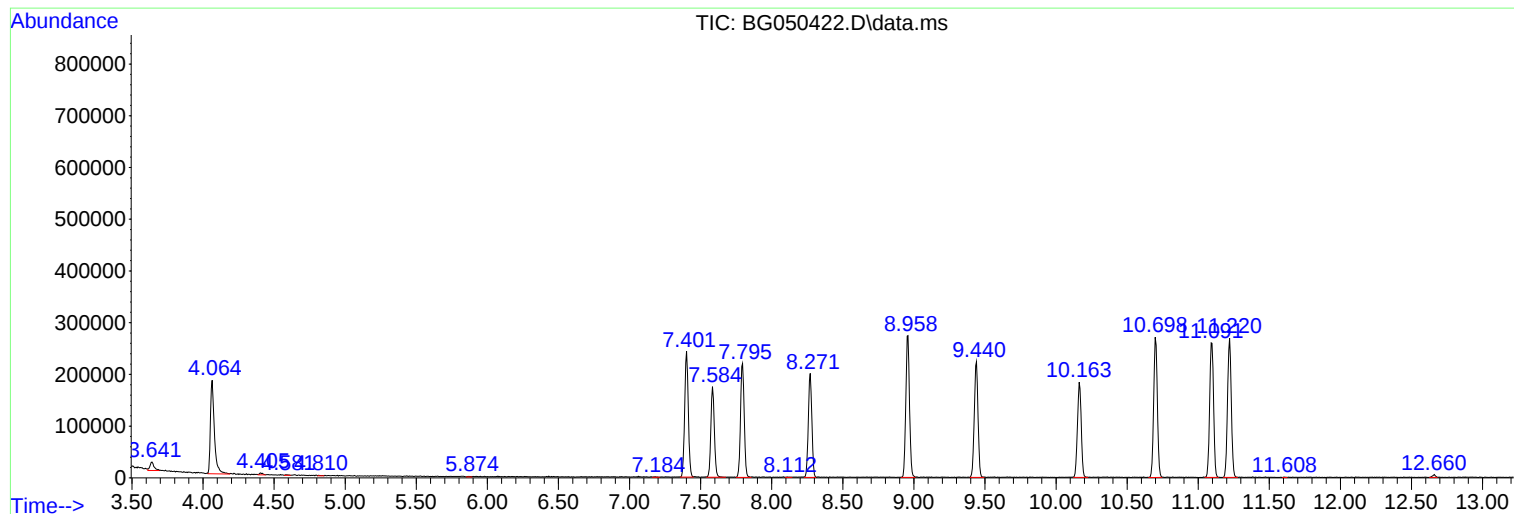

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050422.D
Acq On : 4 Oct 2021 21:03
Operator : CG/JU
Sample : PB139387BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050422.D
Acq On : 4 Oct 2021 21:03
Operator : CG/JU
Sample : PB139387BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK387

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------