

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050438.D
 Acq On : 5 Oct 2021 8:45
 Operator : CG/JU
 Sample : PB139486BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.637	20	25	29	rBV3	14532	23115	1.64%	0.142%
2	3.955	75	79	80	rBV4	1164	1413	0.10%	0.009%
3	4.019	85	90	92	rBV4	1236	1790	0.13%	0.011%
4	4.060	92	97	117	rVV	203524	390789	27.66%	2.401%
5	4.201	119	121	124	rVV	2211	1990	0.14%	0.012%
6	4.248	127	129	133	rVB4	1455	1553	0.11%	0.010%
7	4.401	151	155	162	rVB4	3754	7229	0.51%	0.044%
8	4.718	207	209	214	rBV3	969	1419	0.10%	0.009%
9	7.398	656	665	676	rBV	284356	496786	35.16%	3.052%
10	7.580	689	696	706	rBV	204439	355936	25.19%	2.186%
11	7.791	724	732	740	rBV	262722	459035	32.49%	2.820%
12	8.267	806	813	821	rBV	213271	367142	25.99%	2.255%
13	8.955	923	930	940	rBV2	322062	575486	40.73%	3.535%
14	9.436	1003	1012	1020	rVB	262011	476941	33.76%	2.930%
15	10.165	1128	1136	1144	rVB	212679	400078	28.32%	2.458%
16	10.700	1219	1227	1236	rBV	313562	577508	40.87%	3.547%
17	11.093	1286	1294	1303	rBV	288015	527586	37.34%	3.241%
18	11.217	1307	1315	1325	rVB	309704	584543	41.37%	3.591%
19	12.656	1555	1560	1567	rVB2	4913	8142	0.58%	0.050%
20	13.849	1761	1763	1767	rVB	1339	1615	0.11%	0.010%
21	14.278	1828	1836	1844	rBV	556438	809148	57.27%	4.970%
22	14.577	1879	1887	1896	rBV	596752	988867	69.99%	6.074%
23	14.883	1932	1939	1946	rBV	451422	704920	49.89%	4.330%
24	15.047	1959	1967	1978	rBV	278446	455354	32.23%	2.797%
25	15.870	2100	2107	2115	rVB	773204	1194613	84.55%	7.338%
26	15.976	2119	2125	2132	rBV	195939	306731	21.71%	1.884%
27	16.111	2143	2148	2153	rVB3	8005	10380	0.73%	0.064%
28	17.415	2367	2370	2374	rVB3	1995	2955	0.21%	0.018%
29	17.627	2399	2406	2416	rVB	540728	835224	59.11%	5.131%
30	17.727	2416	2423	2430	rBV2	806638	1249703	88.45%	7.677%
31	17.862	2442	2446	2450	rBV3	2155	3694	0.26%	0.023%
32	17.997	2463	2469	2471	rBV3	1035	1468	0.10%	0.009%
33	18.490	2550	2553	2555	rBV3	1618	1725	0.12%	0.011%
34	18.631	2574	2577	2579	rVB2	1345	1500	0.11%	0.009%
35	18.655	2579	2581	2585	rBV2	958	1521	0.11%	0.009%
36	18.819	2604	2609	2612	rBV2	1651	2171	0.15%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050438.D
 Acq On : 5 Oct 2021 8:45
 Operator : CG/JU
 Sample : PB139486BL
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	19.225	2674	2678	2679	rVV4	1937	1578	0.11%	0.010%
38	19.560	2731	2735	2741	rBV6	9278	16333	1.16%	0.100%
39	19.636	2743	2748	2753	rBV	11104	19034	1.35%	0.117%
40	19.730	2762	2764	2768	rBV4	1619	1709	0.12%	0.010%
41	19.895	2788	2792	2797	rBV6	3953	6069	0.43%	0.037%
42	19.930	2797	2798	2801	rBV3	2027	1551	0.11%	0.010%
43	20.000	2803	2810	2817	rVV	996104	1412888	100.00%	8.679%
44	20.171	2835	2839	2841	rBV4	1893	3023	0.21%	0.019%
45	20.188	2841	2842	2844	rVV2	2175	1516	0.11%	0.009%
46	20.347	2866	2869	2871	rBV4	2561	3382	0.24%	0.021%
47	20.682	2925	2926	2928	rBV2	2851	1787	0.13%	0.011%
48	21.928	3131	3138	3148	rVB	480468	847757	60.00%	5.208%
49	25.112	3670	3680	3692	rVB3	421598	1255230	88.84%	7.711%
50	25.353	3710	3721	3733	rVB2	275838	865546	61.26%	5.317%
51	26.587	3929	3931	3932	rBV	8502	6431	0.46%	0.040%
52	28.026	4174	4176	4177	rBV2	7707	5569	0.39%	0.034%




Sum of corrected areas: 16279473

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050438.D
Acq On : 5 Oct 2021 8:45
Operator : CG/JU
Sample : PB139486BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

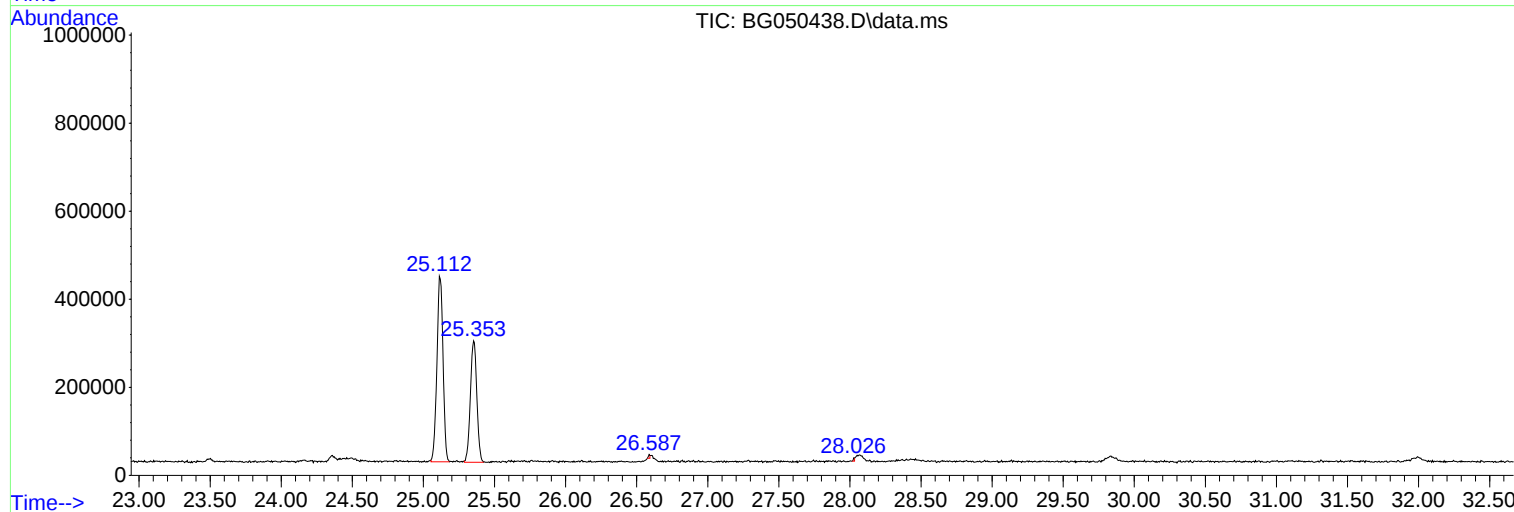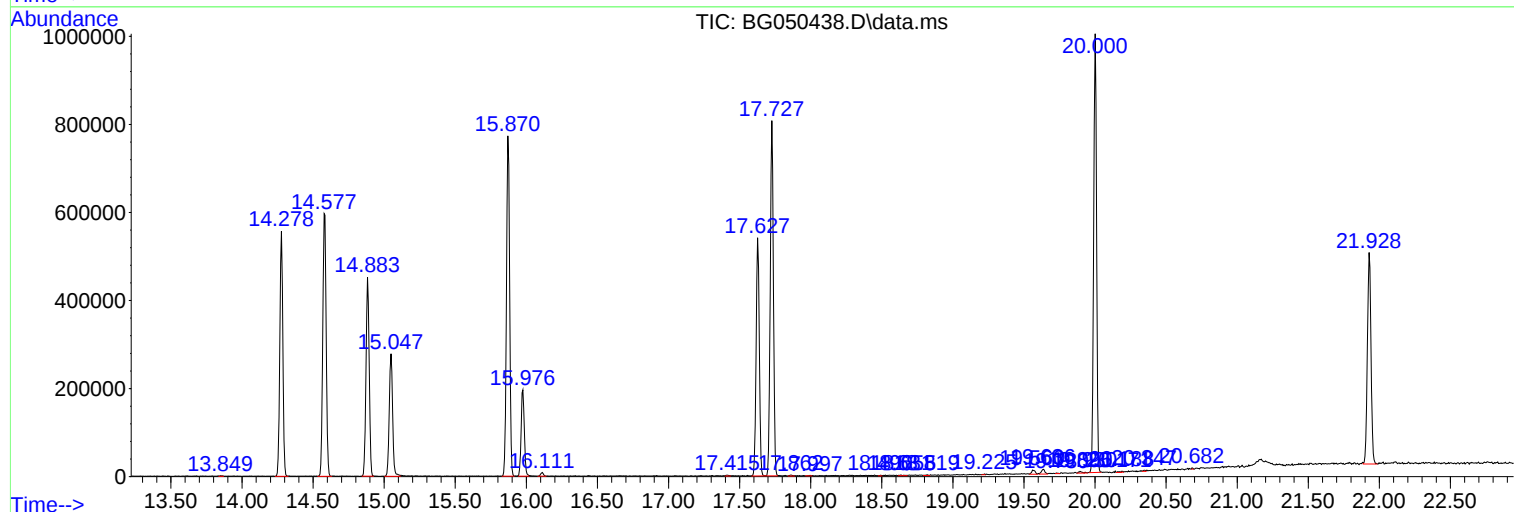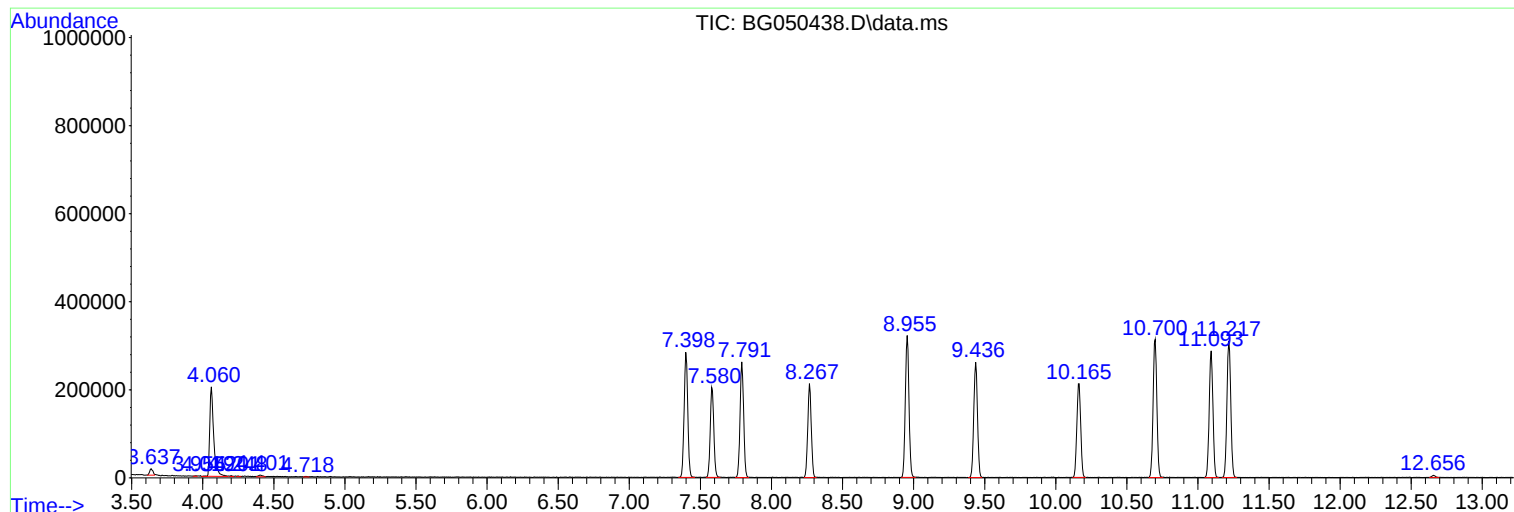

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050438.D
Acq On : 5 Oct 2021 8:45
Operator : CG/JU
Sample : PB139486BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050438.D
Acq On : 5 Oct 2021 8:45
Operator : CG/JU
Sample : PB139486BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------