

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050448.D
 Acq On : 5 Oct 2021 18:23
 Operator : CG/JU
 Sample : PB139632BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK632

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.640	22	26	32	rVB2	15250	25224	1.98%	0.184%
2	4.058	92	97	110	rBV	168490	329275	25.83%	2.403%
3	4.216	123	124	126	rVB2	2738	1279	0.10%	0.009%
4	4.398	151	155	161	rVB6	5146	8614	0.68%	0.063%
5	4.445	161	163	166	rBB3	1339	1350	0.11%	0.010%
6	4.510	172	174	177	rVB2	2046	1790	0.14%	0.013%
7	4.616	190	192	196	rVB4	2282	2453	0.19%	0.018%
8	5.115	275	277	281	rVB3	1303	1425	0.11%	0.010%
9	7.395	657	665	675	rBV	234076	416026	32.64%	3.036%
10	7.583	690	697	712	rVB	169504	295267	23.17%	2.155%
11	7.700	712	717	718	rBV3	1256	1443	0.11%	0.011%
12	7.788	725	732	742	rVB	211410	379552	29.78%	2.770%
13	7.935	755	757	760	rBV2	1150	1347	0.11%	0.010%
14	8.270	806	814	823	rVB	162580	287511	22.56%	2.098%
15	8.341	823	826	830	rBV4	1114	1485	0.12%	0.011%
16	8.952	923	930	940	rVV	273094	478918	37.58%	3.495%
17	9.434	1003	1012	1020	rBV	215958	391329	30.70%	2.856%
18	10.162	1128	1136	1144	rBV	179484	320130	25.12%	2.336%
19	10.697	1219	1227	1240	rBV	258385	471744	37.01%	3.443%
20	11.090	1287	1294	1302	rVB	230159	416626	32.69%	3.040%
21	11.220	1308	1316	1324	rBV	262303	482703	37.87%	3.522%
22	12.659	1556	1561	1566	rVB	5656	7449	0.58%	0.054%
23	14.275	1829	1836	1842	rBV	466256	674818	52.95%	4.924%
24	14.580	1881	1888	1895	rVB	500522	809324	63.50%	5.906%
25	14.880	1933	1939	1946	rVB	341357	561794	44.08%	4.100%
26	15.045	1960	1967	1980	rBV	237493	386234	30.30%	2.819%
27	15.867	2101	2107	2115	rBV	624710	993987	77.99%	7.254%
28	15.973	2118	2125	2136	rBV	163872	254023	19.93%	1.854%
29	16.114	2143	2149	2152	rBV2	6970	9512	0.75%	0.069%
30	17.401	2365	2368	2370	rBV2	1152	1373	0.11%	0.010%
31	17.624	2399	2406	2415	rVB	437755	681014	53.43%	4.970%
32	17.724	2415	2423	2433	rBV	725538	1107008	86.85%	8.078%
33	18.417	2538	2541	2543	rBV	1140	1303	0.10%	0.010%
34	18.770	2600	2601	2606	rBV4	1164	1287	0.10%	0.009%
35	18.952	2629	2632	2635	rBV3	986	1415	0.11%	0.010%
36	19.381	2702	2705	2706	rBV3	1291	1393	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050448.D
 Acq On : 5 Oct 2021 18:23
 Operator : CG/JU
 Sample : PB139632BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK632

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	19.563	2733	2736	2740	rBV4	7309	9546	0.75%	0.070%
38	19.633	2743	2748	2751	rVV2	9619	13060	1.02%	0.095%
39	19.745	2765	2767	2771	rBV3	1498	2171	0.17%	0.016%
40	19.827	2777	2781	2782	rBV4	2637	2734	0.21%	0.020%
41	19.998	2803	2810	2819	rBV	889609	1274549	100.00%	9.301%
42	20.139	2830	2834	2835	rBV4	2334	2727	0.21%	0.020%
43	20.262	2853	2855	2858	rVB3	2291	2072	0.16%	0.015%
44	20.291	2858	2860	2862	rBV2	2094	2625	0.21%	0.019%
45	20.391	2875	2877	2878	rBV2	2344	1662	0.13%	0.012%
46	21.079	2992	2994	2995	rBV2	3198	2080	0.16%	0.015%
47	21.837	3121	3123	3126	rBV4	4572	5200	0.41%	0.038%
48	21.925	3131	3138	3147	rVB	394933	712624	55.91%	5.200%
49	23.864	3466	3468	3469	rBV2	4052	2013	0.16%	0.015%
50	25.109	3669	3680	3691	rVB2	394172	1140088	89.45%	8.320%
51	25.344	3709	3720	3734	rVB	232688	711324	55.81%	5.191%
52	29.774	4472	4474	4477	rBV4	5035	5538	0.43%	0.040%
53	30.955	4673	4675	4679	rBV3	4116	4173	0.33%	0.030%
54	30.991	4679	4681	4682	rVV2	4093	1905	0.15%	0.014%




Sum of corrected areas: 13703516

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050448.D
Acq On : 5 Oct 2021 18:23
Operator : CG/JU
Sample : PB139632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

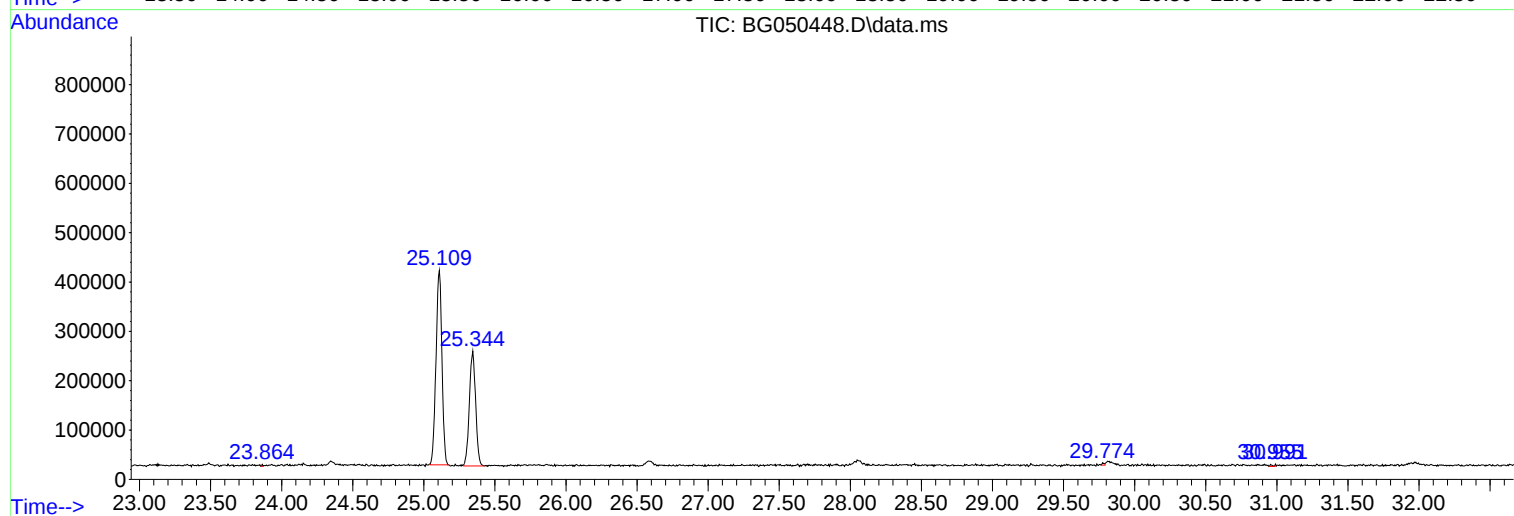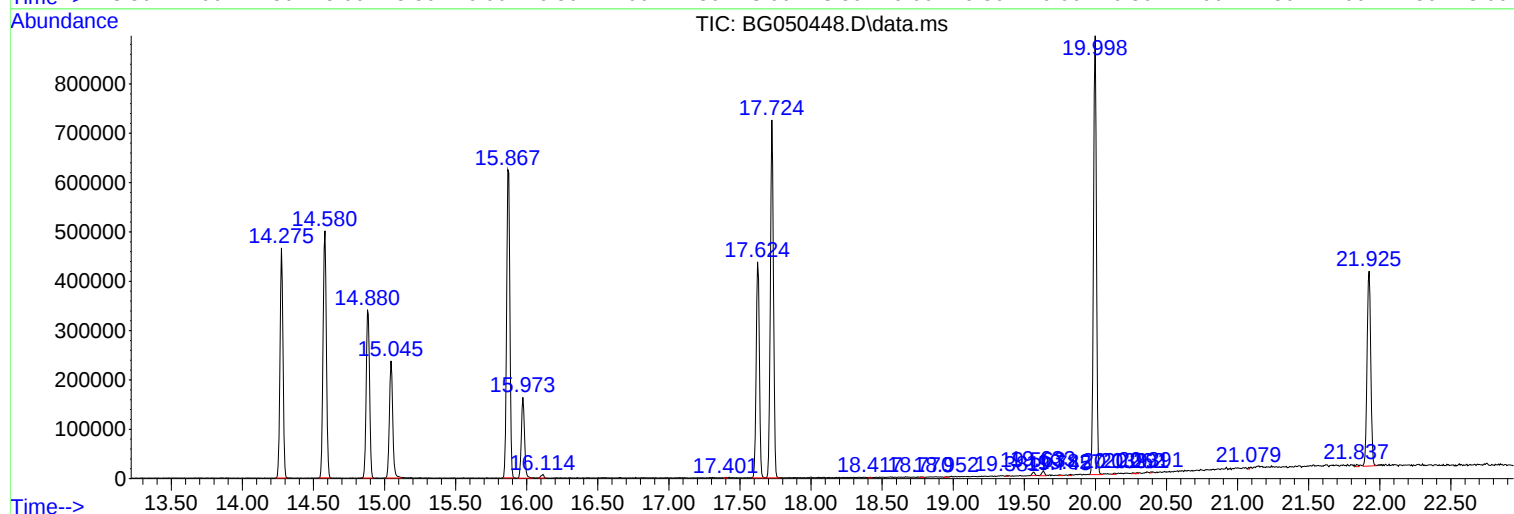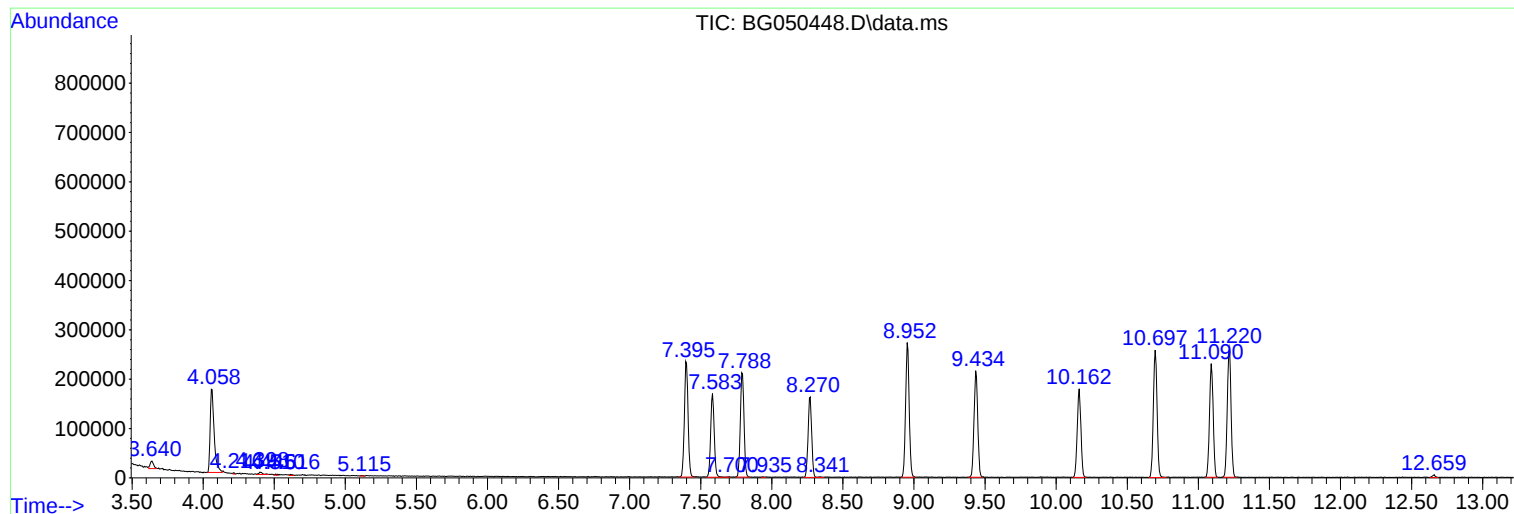

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050448.D
Acq On : 5 Oct 2021 18:23
Operator : CG/JU
Sample : PB139632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050448.D
Acq On : 5 Oct 2021 18:23
Operator : CG/JU
Sample : PB139632BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK632

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------