

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050449.D
 Acq On : 5 Oct 2021 19:04
 Operator : CG/JU
 Sample : PB139634BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK634

Integration Parameters: LSCINT.P

Integrator: RTE

Smothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

Signal : TIC: BG050449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.635	22	25	31	rVB2	16580	22476	1.79%	0.163%
2	4.058	92	97	110	rBV	174841	333424	26.56%	2.415%
3	4.398	153	155	161	rBV4	3555	4640	0.37%	0.034%
4	4.622	192	193	196	rBV2	1181	1323	0.11%	0.010%
5	6.508	509	514	515	rBV3	974	1274	0.10%	0.009%
6	7.395	658	665	676	rBV	227291	411387	32.77%	2.980%
7	7.583	688	697	705	rBV	168931	292864	23.33%	2.121%
8	7.789	725	732	740	rBV	212622	378587	30.16%	2.742%
9	8.265	807	813	822	rVB	173864	305756	24.35%	2.215%
10	8.952	923	930	940	rVV	264782	471190	37.53%	3.413%
11	9.434	1005	1012	1023	rVB	216802	388684	30.96%	2.815%
12	10.162	1127	1136	1144	rBV	177323	321207	25.59%	2.327%
13	10.697	1220	1227	1235	rBV	258270	457633	36.45%	3.315%
14	11.091	1285	1294	1303	rVB	243002	447305	35.63%	3.240%
15	11.220	1308	1316	1324	rBV	252169	475844	37.90%	3.447%
16	12.659	1556	1561	1565	rBV3	4370	6916	0.55%	0.050%
17	14.275	1829	1836	1843	rBV	461171	672469	53.57%	4.871%
18	14.581	1879	1888	1894	rBV	505662	805926	64.20%	5.838%
19	14.880	1932	1939	1947	rVB	384462	601032	47.87%	4.354%
20	15.045	1960	1967	1975	rBV	228457	375242	29.89%	2.718%
21	15.867	2100	2107	2119	rBV	623888	984982	78.46%	7.135%
22	15.973	2119	2125	2132	rBV	162852	247458	19.71%	1.792%
23	16.108	2141	2148	2152	rVB3	7000	10075	0.80%	0.073%
24	17.413	2366	2370	2374	rBV3	1835	2556	0.20%	0.019%
25	17.624	2400	2406	2415	rVB	473996	719546	57.31%	5.212%
26	17.724	2416	2423	2430	rVV	716841	1087958	86.66%	7.881%
27	19.093	2652	2656	2657	rBV3	1534	1585	0.13%	0.011%
28	19.252	2681	2683	2686	rBV4	1287	1668	0.13%	0.012%
29	19.322	2693	2695	2698	rBV2	1419	1514	0.12%	0.011%
30	19.563	2732	2736	2743	rVB5	7484	11905	0.95%	0.086%
31	19.634	2743	2748	2752	rBV2	9289	15260	1.22%	0.111%
32	19.739	2764	2766	2769	rVB4	2102	2110	0.17%	0.015%
33	19.892	2789	2792	2793	rBV3	2799	3019	0.24%	0.022%
34	19.998	2803	2810	2816	rBV	867389	1255425	100.00%	9.094%
35	20.168	2838	2839	2841	rBV2	2438	1431	0.11%	0.010%
36	20.327	2865	2866	2868	rBV2	2106	1535	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
 Data File : BG050449.D
 Acq On : 5 Oct 2021 19:04
 Operator : CG/JU
 Sample : PB139634BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK634

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
 Title : SVOA CALIBRATION

37	20.433	2882	2884	2885	rVB2	2457	1439	0.11%	0.010%
38	20.450	2885	2887	2888	rBV2	2458	1446	0.12%	0.010%
39	20.497	2893	2895	2896	rVB2	2445	1349	0.11%	0.010%
40	20.521	2896	2899	2900	rBV2	2651	2670	0.21%	0.019%
41	20.644	2918	2920	2921	rBV2	2954	1952	0.16%	0.014%
42	21.925	3131	3138	3147	rVB2	426150	753331	60.01%	5.457%
43	22.048	3158	3159	3163	rBV4	4728	5525	0.44%	0.040%
44	22.965	3313	3315	3316	rBV2	4017	2302	0.18%	0.017%
45	24.352	3547	3551	3556	rVB7	8432	15443	1.23%	0.112%
46	25.110	3668	3680	3692	rVB2	385800	1129961	90.01%	8.185%
47	25.345	3709	3720	3733	rVB3	245976	764727	60.91%	5.539%
48	29.687	4457	4459	4460	rVB2	4351	2251	0.18%	0.016%




Sum of corrected areas: 13805602

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050449.D
Acq On : 5 Oct 2021 19:04
Operator : CG/JU
Sample : PB139634BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK634

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

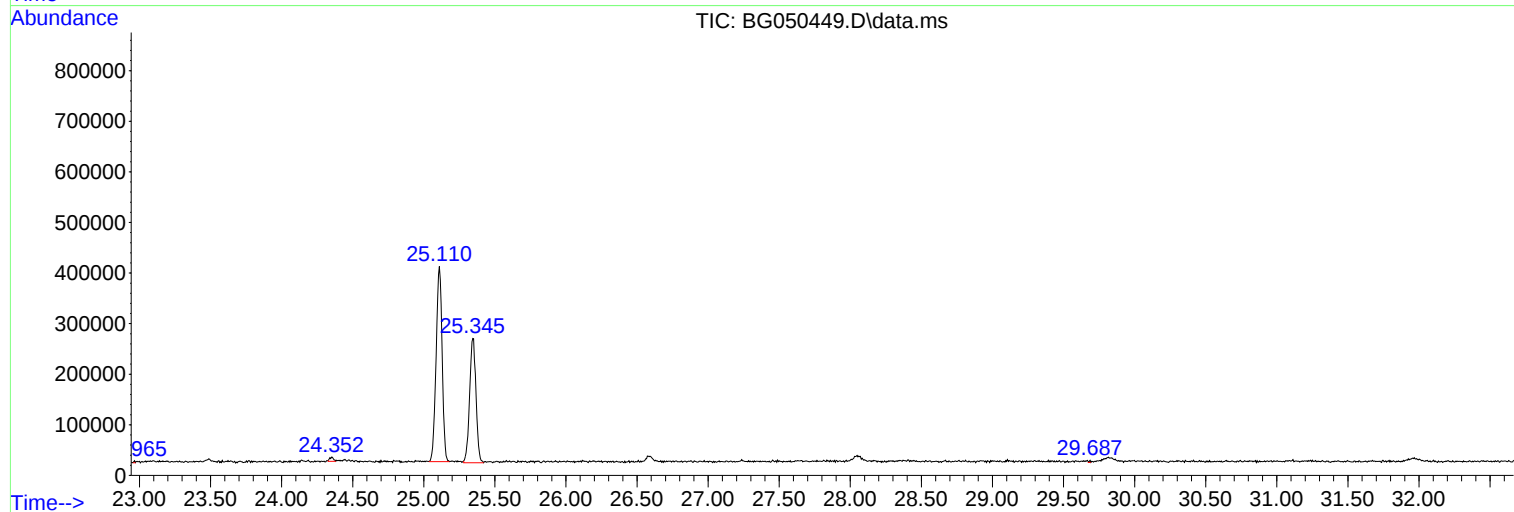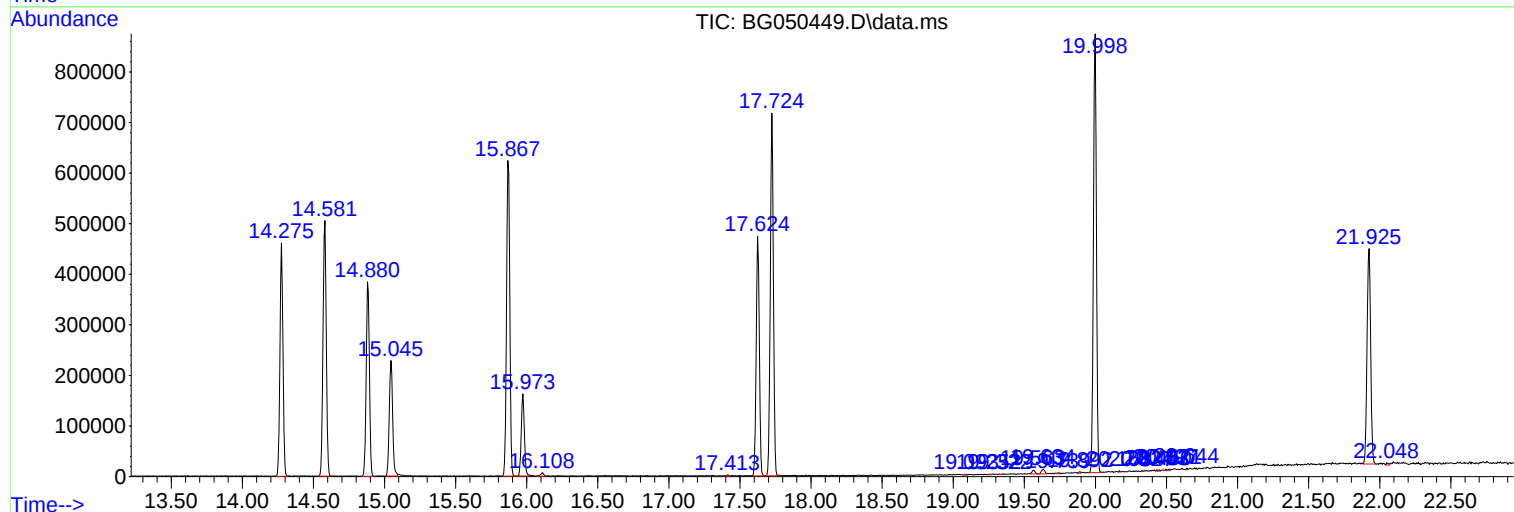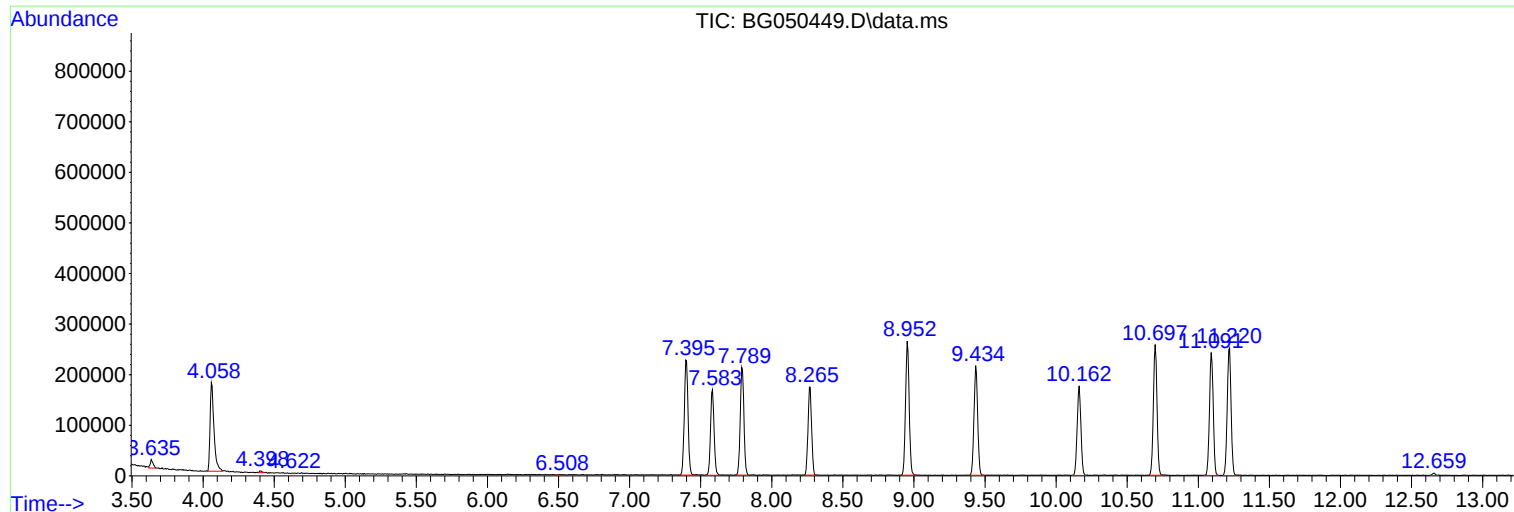

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050449.D
Acq On : 5 Oct 2021 19:04
Operator : CG/JU
Sample : PB139634BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK634

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100421\
Data File : BG050449.D
Acq On : 5 Oct 2021 19:04
Operator : CG/JU
Sample : PB139634BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK634

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG093021.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
