

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100515\
 Data File : BG019034.D
 Acq On : 5 Oct 2015 19:35
 Operator : UM/NP
 Sample : G3900-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AA0

Quant Time: Oct 06 04:27:57 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 04:27:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	31227	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	141446	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	92260	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	227985	20.00	ng/ul	0.00
78) Chrysene-d12	21.67	240	258801	20.00	ng/ul	0.00
86) Perylene-d12	24.89	264	255016	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.50	96	2954	4.27	ng/uL	0.00
5) Phenol-d5	7.20	99	74998	27.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	51129	29.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	57667	28.55	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	58859	27.82	ng/ul	0.00
19) Nitrobenzene-d5	9.21	128	30094	28.14	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	32138	29.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	62429	28.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	57665	21.47	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	209624	28.82	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	252140	28.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.84	143	36514	24.85	ng/ul	0.00
58) Fluorene-d10	15.66	176	192419	29.22	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	27218	22.01	ng/ul	0.00
71) Anthracene-d10	17.51	188	301708	28.10	ng/ul	0.00
79) Pyrene-d10	19.79	212	352872	29.44	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.67	264	381695	29.25	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.12	163	114219	15.38	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100515\
Data File : BG019034.D
Acq On : 5 Oct 2015 19:35
Operator : UM/NP
Sample : G3900-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AA0

Quant Time: Oct 06 04:27:57 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 04:27:31 2015
Response via : Initial Calibration

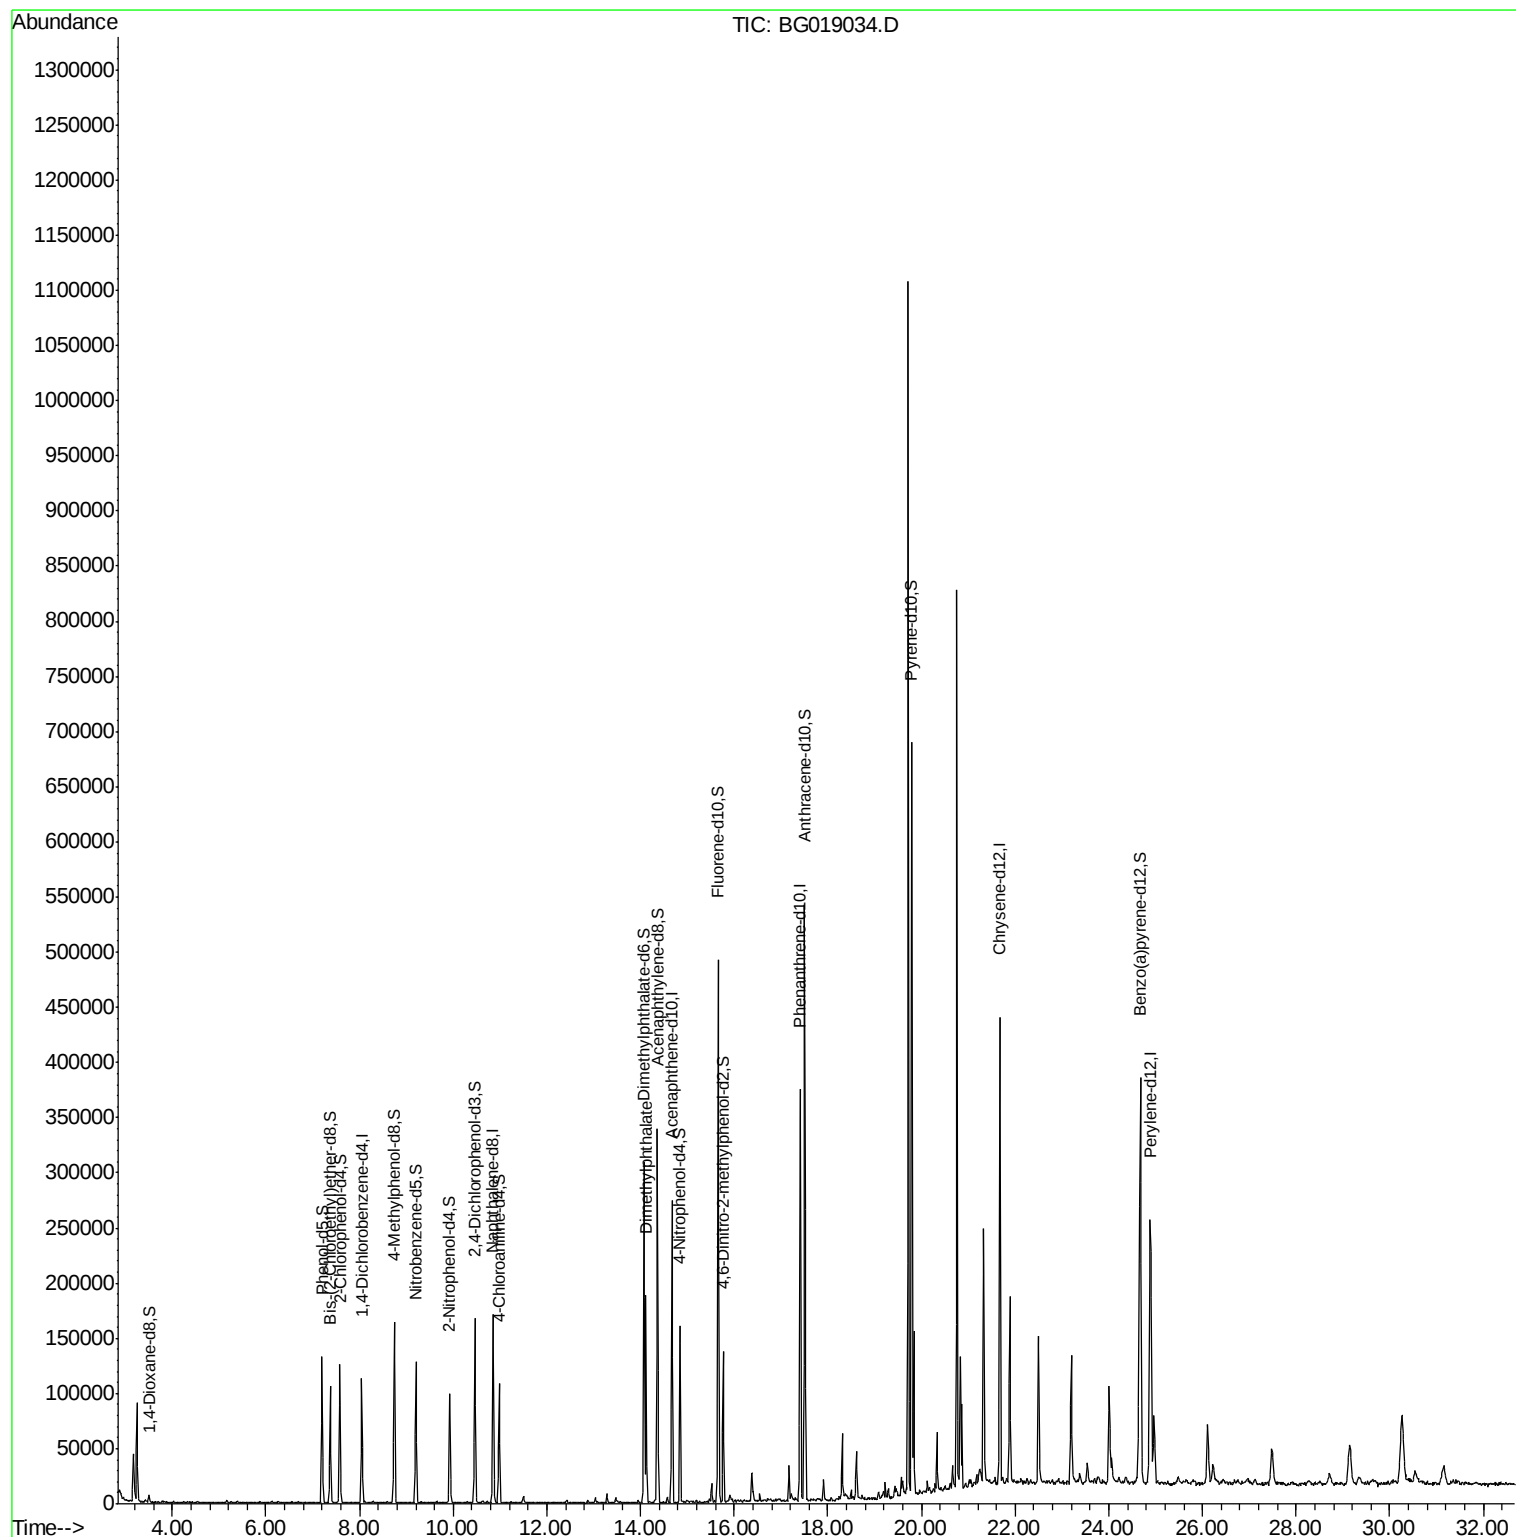

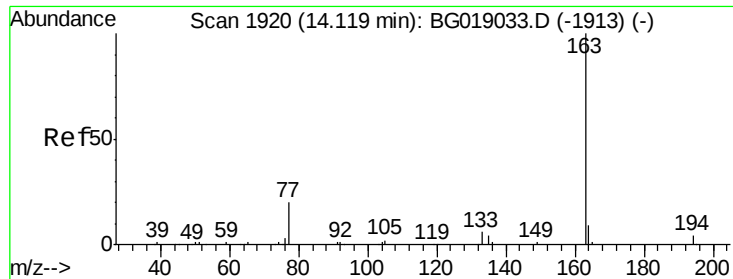

#45

Dimethylphthalate

Concen: 15.38 ng/ul

RT: 14.12 min Scan# 1920

Delta R.T. -0.00 min

Lab File: BG019034.D


Acq: 5 Oct 2015 19:35

Instrument :

BNA_G

ClientSampleId :

C0AA0

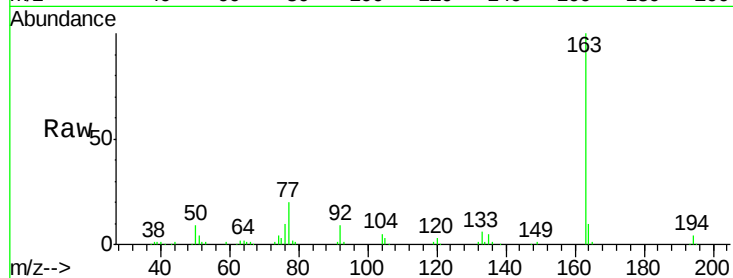


Tgt Ion:163 Resp: 114219

Ion Ratio Lower Upper

163 100

194 3.8 3.3 4.9

164 10.2 8.1 12.1

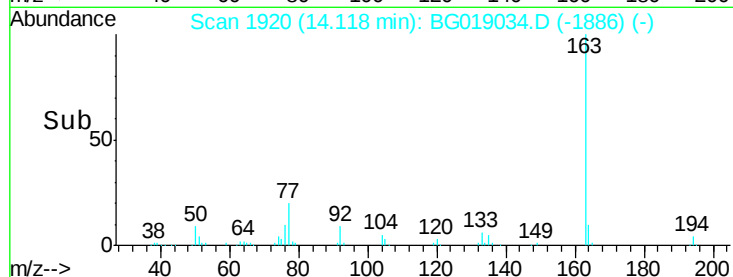

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

