

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100515\
 Data File : BG019045.D
 Acq On : 6 Oct 2015 2:32
 Operator : UM/NP
 Sample : G3865-15
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5MZ1

Quant Time: Oct 06 04:30:16 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 04:27:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	64646	20.00	ng/ul	0.01
18) Naphthalene-d8	10.86	136	291360	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.68	164	175460	20.00	ng/ul	0.01
62) Phenanthrene-d10	17.42	188	348879	20.00	ng/ul	0.01
78) Chrysene-d12	21.69	240	366373	20.00	ng/ul	0.02
86) Perylene-d12	24.94	264	359665	20.00	ng/ul	0.04

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.50	96	3512	2.45	ng/uL	0.00
5) Phenol-d5	7.22	99	104390	18.74	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.38	67	72286	20.05	ng/ul	0.01
9) 2-Chlorophenol-d4	7.59	132	82667	19.77	ng/ul	0.01
13) 4-Methylphenol-d8	8.76	113	78420	17.91	ng/ul	0.02
19) Nitrobenzene-d5	9.21	128	45246	20.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	49398	21.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	91180	20.10	ng/ul	0.02
29) 4-Chloroaniline-d4	10.99	131	68505	12.38	ng/ul	0.01
44) Dimethylphthalate-d6	14.08	166	282102	20.39	ng/ul	0.01
47) Acenaphthylene-d8	14.37	160	347815	20.33	ng/ul	0.01
52) 4-Nitrophenol-d4	14.87	143	30852	11.04	ng/ul	0.02
58) Fluorene-d10	15.67	176	243021	19.40	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	15.78	200	16995	8.98	ng/ul	0.00
71) Anthracene-d10	17.52	188	346008	21.06	ng/ul	0.01
79) Pyrene-d10	19.81	212	348391	20.53	ng/ul	0.02
90) Benzo(a)pyrene-d12	24.71	264	380826	20.69	ng/ul	0.03


Target Compounds						Qvalue
45) Dimethylphthalate	14.13	163	160851	11.39	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100515\
Data File : BG019045.D
Acq On : 6 Oct 2015 2:32
Operator : UM/NP
Sample : G3865-15
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5MZ1

Quant Time: Oct 06 04:30:16 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 04:27:31 2015
Response via : Initial Calibration

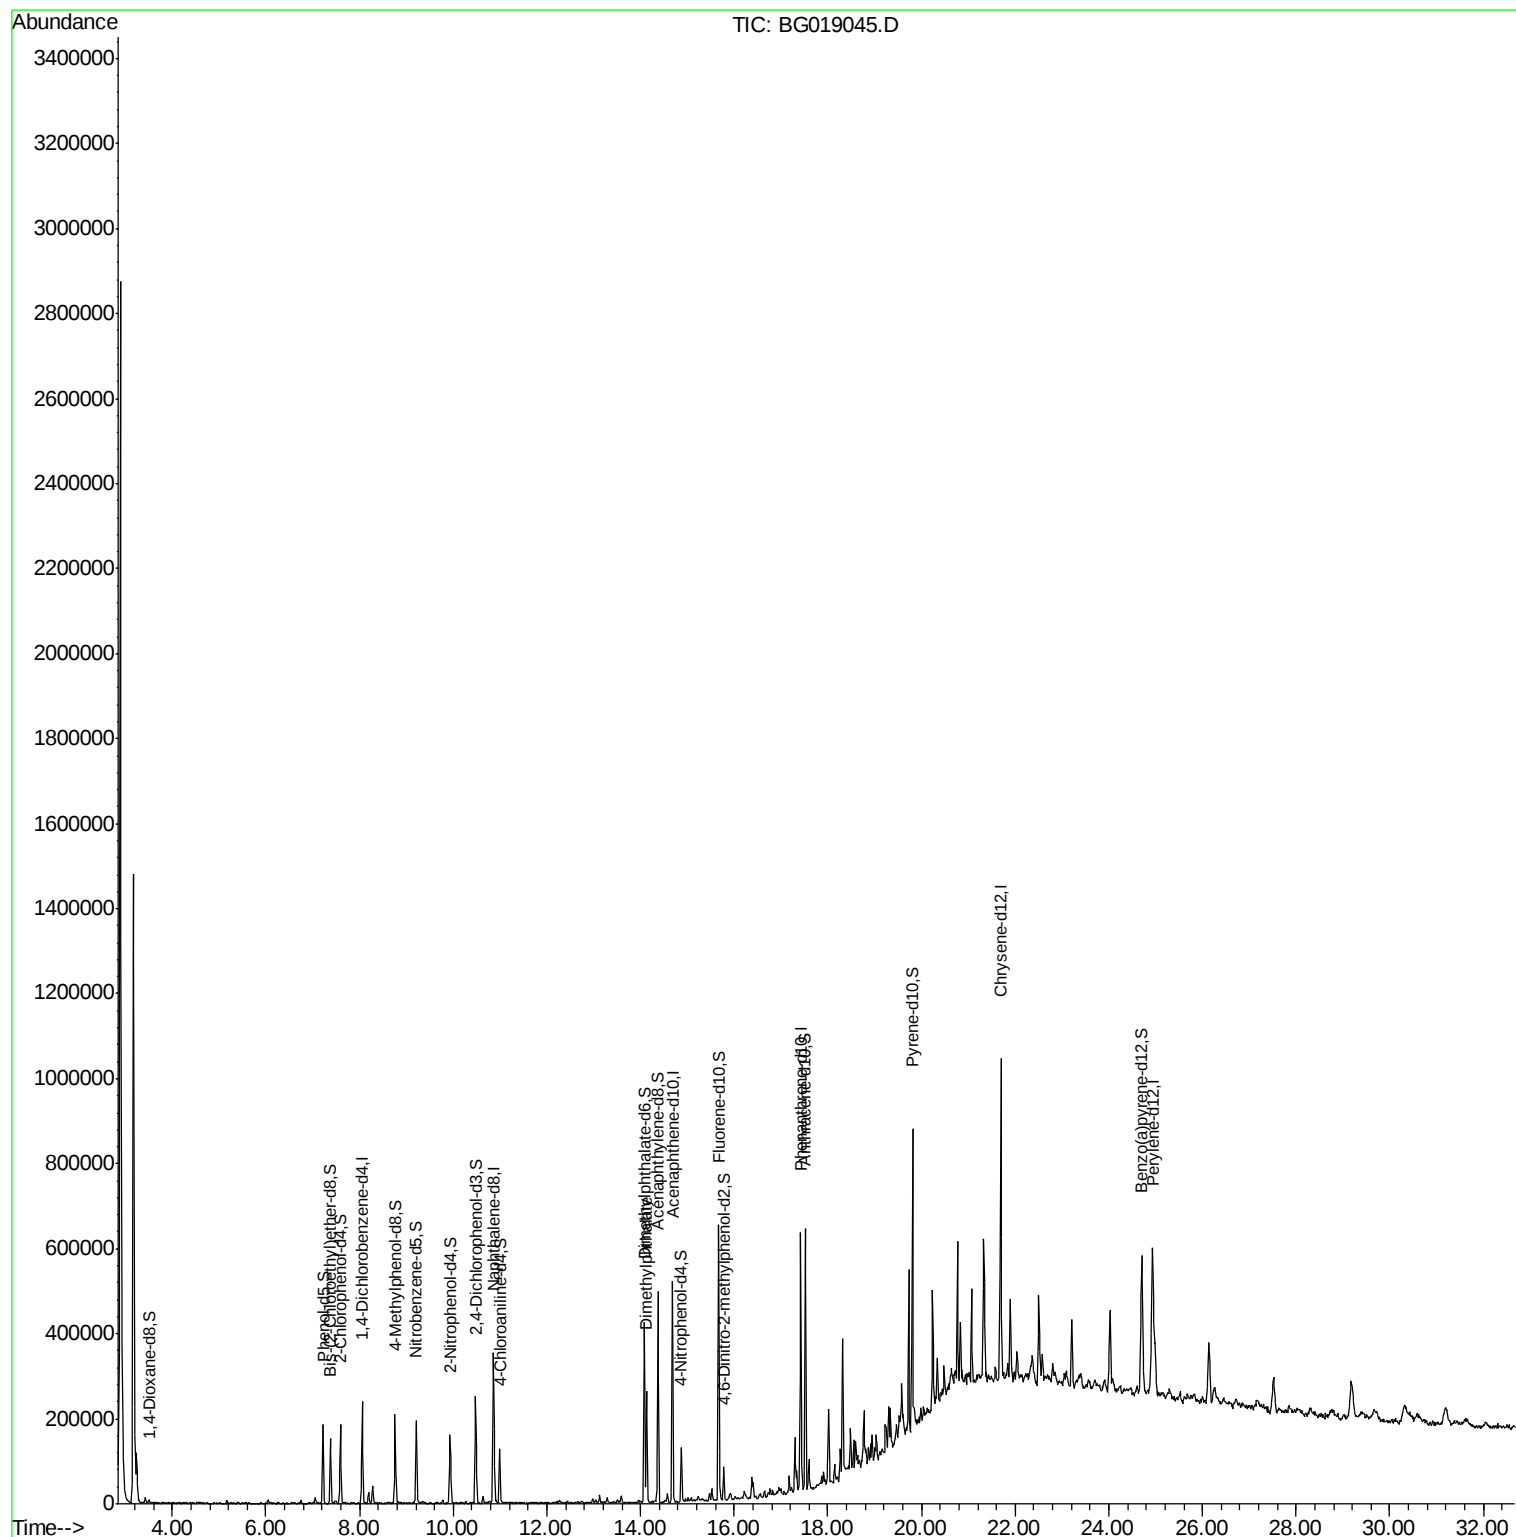

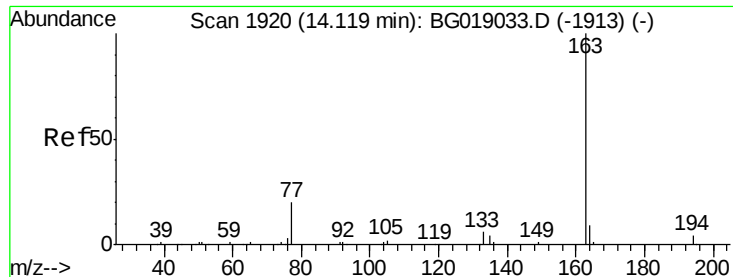

#45

Dimethylphthalate

Concen: 11.39 ng/ul

RT: 14.13 min Scan# 1922

Delta R.T. 0.01 min

Lab File: BG019045.D

Acq: 6 Oct 2015 2:32

Instrument :

BNA_G

ClientSampleId :

E5MZ1


Tgt Ion:163 Resp: 160851

Ion Ratio Lower Upper

163 100

194 4.3 3.3 4.9

164 11.0 8.1 12.1

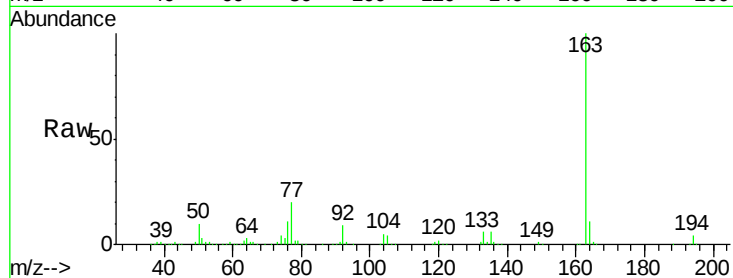

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

