

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100515\
 Data File : BG019046.D
 Acq On : 6 Oct 2015 3:10
 Operator : UM/NP
 Sample : G3865-14
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5MZ0

Quant Time: Oct 06 04:30:27 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 04:27:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	54557	20.00	ng/ul	0.01
18) Naphthalene-d8	10.86	136	244152	20.00	ng/ul	0.01
36) Acenaphthene-d10	14.68	164	148181	20.00	ng/ul	0.01
62) Phenanthrene-d10	17.42	188	301968	20.00	ng/ul	0.01
78) Chrysene-d12	21.69	240	318981	20.00	ng/ul	0.02
86) Perylene-d12	24.93	264	307974	20.00	ng/ul	0.03

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.50	96	3791	3.14	ng/uL	0.00
5) Phenol-d5	7.22	99	80523	17.13	ng/ul	0.02
7) Bis-(2-Chloroethyl)ether-d	7.38	67	71683	23.56	ng/ul	0.01
9) 2-Chlorophenol-d4	7.59	132	76429	21.66	ng/ul	0.01
13) 4-Methylphenol-d8	8.76	113	52399	14.18	ng/ul	0.02
19) Nitrobenzene-d5	9.21	128	44969	24.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	50248	26.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	86839	22.85	ng/ul	0.02
29) 4-Chloroaniline-d4	10.99	131	141731	30.58	ng/ul	0.01
44) Dimethylphthalate-d6	14.08	166	283319	24.25	ng/ul	0.01
47) Acenaphthylene-d8	14.38	160	349809	24.21	ng/ul	0.02
52) 4-Nitrophenol-d4	14.88	143	25332	10.73	ng/ul	0.03
58) Fluorene-d10	15.67	176	244418	23.11	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	15.78	200	11436	6.98	ng/ul	0.01
71) Anthracene-d10	17.52	188	348249	24.49	ng/ul	0.01
79) Pyrene-d10	19.80	212	354224	23.98	ng/ul	0.01
90) Benzo(a)pyrene-d12	24.71	264	384252	24.38	ng/ul	0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.13	163	168621	14.13	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100515\
Data File : BG019046.D
Acq On : 6 Oct 2015 3:10
Operator : UM/NP
Sample : G3865-14
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5MZ0

Quant Time: Oct 06 04:30:27 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 04:27:31 2015
Response via : Initial Calibration

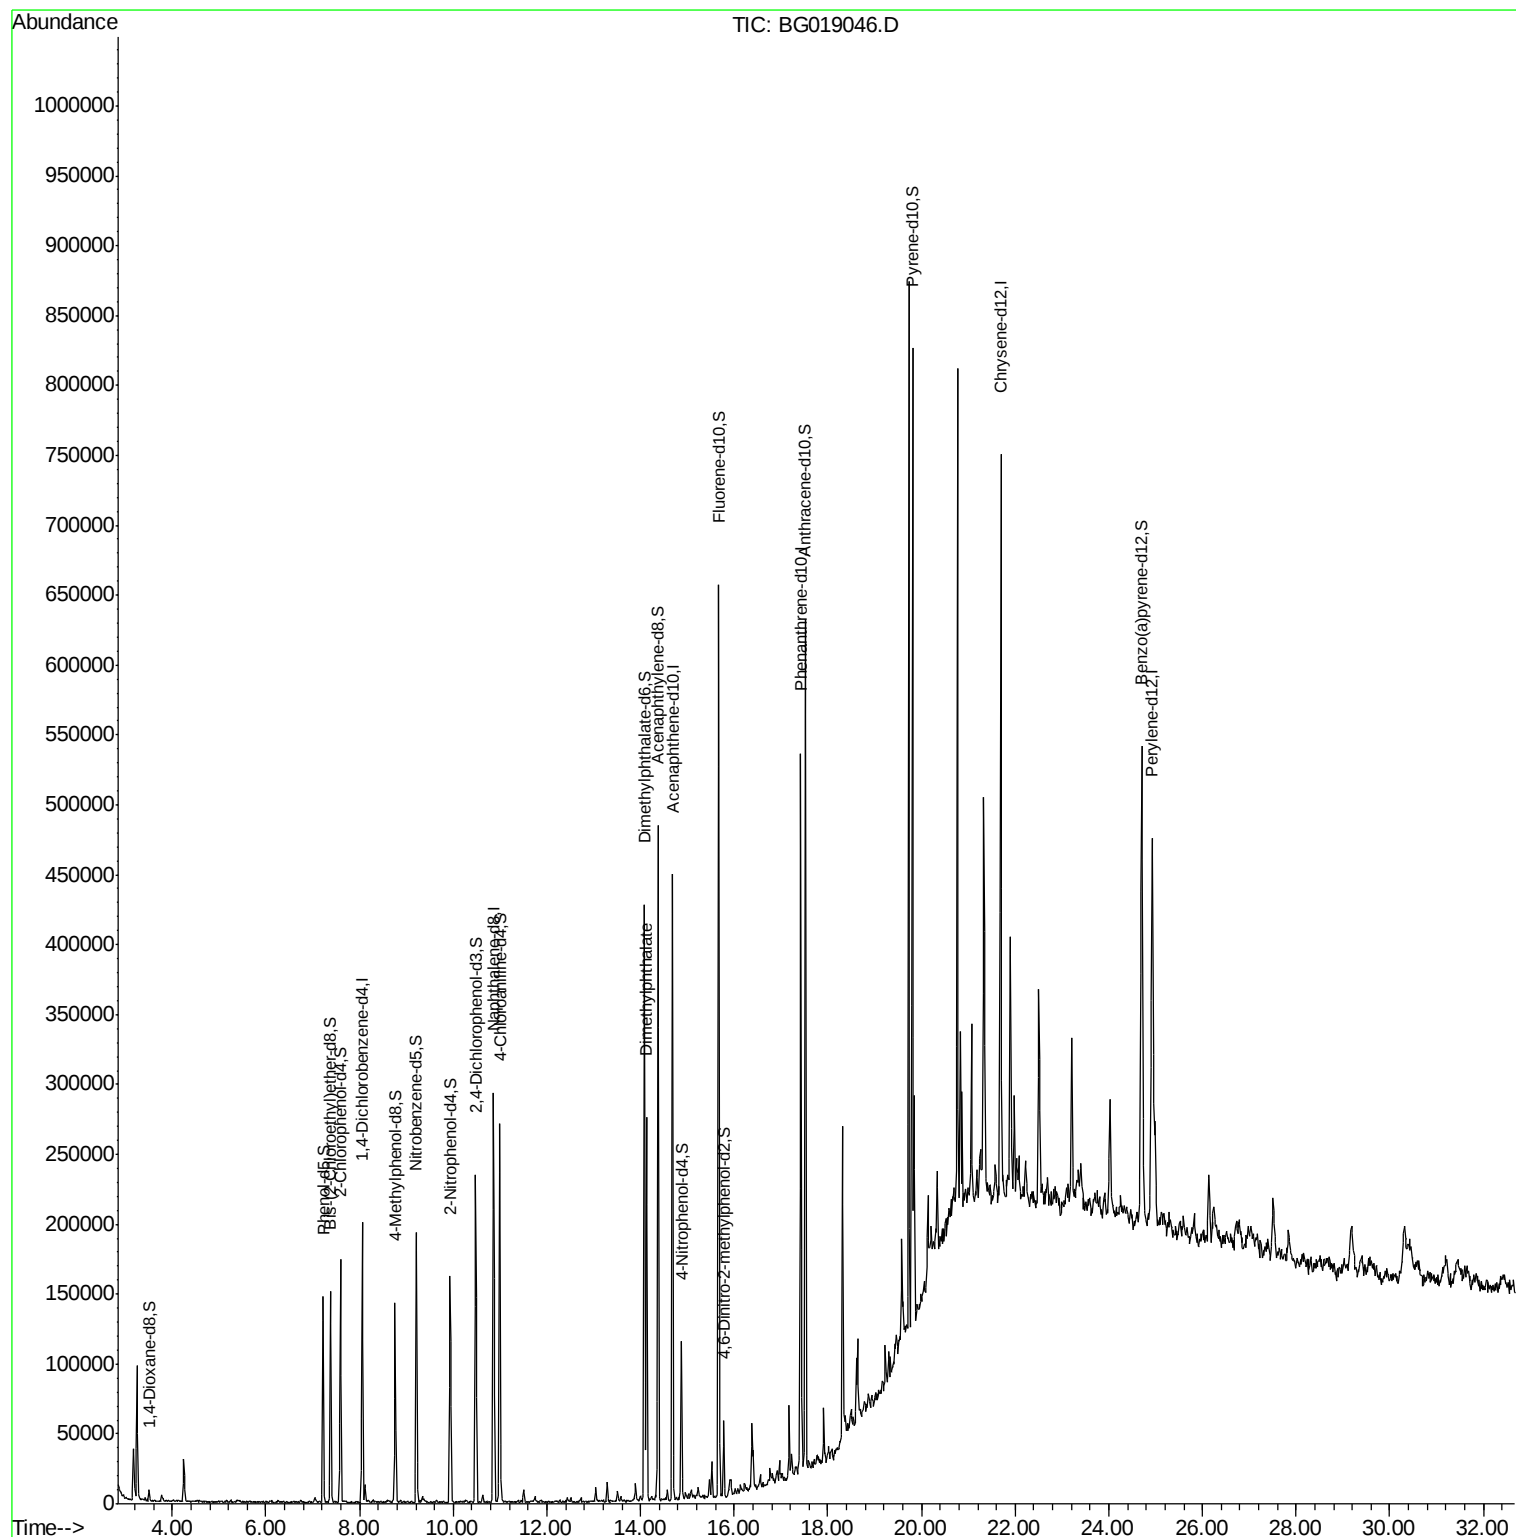

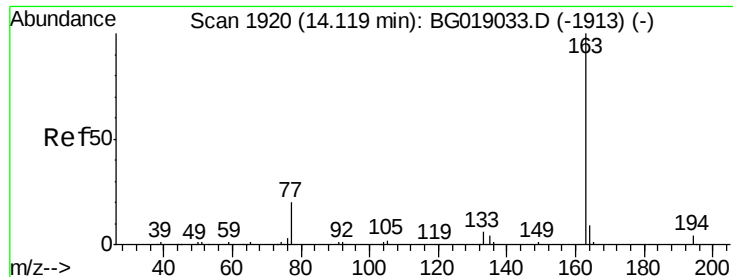

#45

Dimethylphthalate

Concen: 14.13 ng/ul

RT: 14.13 min Scan# 1922

Delta R.T. 0.01 min

Lab File: BG019046.D

Acq: 6 Oct 2015 3:10

Instrument :

BNA_G

ClientSampleId :

E5MZ0


Tgt Ion:163 Resp: 168621

Ion Ratio Lower Upper

163 100

194 4.2 3.3 4.9

164 10.4 8.1 12.1

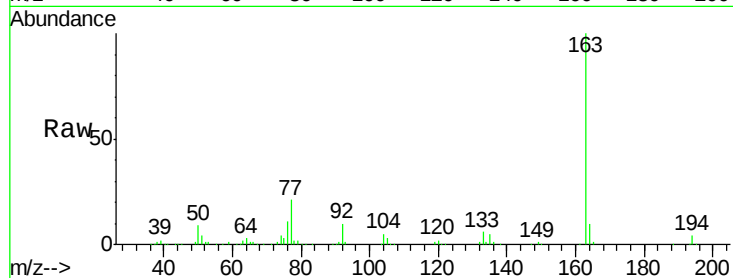

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

