

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100515\
 Data File : BG019042.D
 Acq On : 6 Oct 2015 00:39
 Operator : UM/NP
 Sample : G3865-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5MY2

Manual Integrations
 APPROVED

MMDadoda
 10/6/2015 5:55:06 PM

Quant Time: Oct 06 09:41:18 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 06 04:27:31 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	46967	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	220094	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	144182	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	317635	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	347221	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	343855	20.00	ng/ul	0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.51	96	3261	3.14	ng/uL	0.00
5) Phenol-d5	7.21	99	82479	20.38	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	7.37	67	57540	21.97	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	65156	21.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.76	113	60967	19.16	ng/ul	0.01
19) Nitrobenzene-d5	9.21	128	36325	21.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	41835	24.44	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	75687	22.09	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	74223	17.76	ng/ul	0.00
44) Dimethylphthalate-d6	14.08	166	252224	22.19	ng/ul	0.00
47) Acenaphthylene-d8	14.37	160	313284	22.28	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	30522	13.29	ng/ul	0.01
58) Fluorene-d10	15.66	176	225577	21.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.77	200	24351	14.13	ng/ul	0.00
71) Anthracene-d10	17.51	188	339030	22.67	ng/ul	0.00
79) Pyrene-d10	19.80	212	358852	22.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.69	264	398984	22.68	ng/ul	0.01

Target Compounds

						Ovalue
34) 2-Methylnaphthalene	12.51	142	12497	1.46	ng/ul	99
35) 1-Methylnaphthalene	12.72	142	9789	1.17	ng/ul	91
45) Dimethylphthalate	14.12	163	149830	12.91	ng/ul	98
70) Phenanthrene	17.46	178	39436	2.20	ng/ul	97
77) Fluoranthene	19.46	202	41748	2.00	ng/ul	98
80) Pyrene	19.82	202	36176	1.73	ng/ul#	96
83) Benzo(a)anthracene	21.66	228	20868	1.04	ng/ul	97
88) Benzo(b)fluoranthene	23.88	252	22245m	1.10	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG100515\
Data File : BG019042.D
Acq On : 6 Oct 2015 00:39
Operator : UM/NP
Sample : G3865-03
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
E5MY2

Manual Integrations
APPROVED

MMDadoda
10/6/2015 5:55:06 PM

Quant Time: Oct 06 09:41:18 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 06 04:27:31 2015
Response via : Initial Calibration

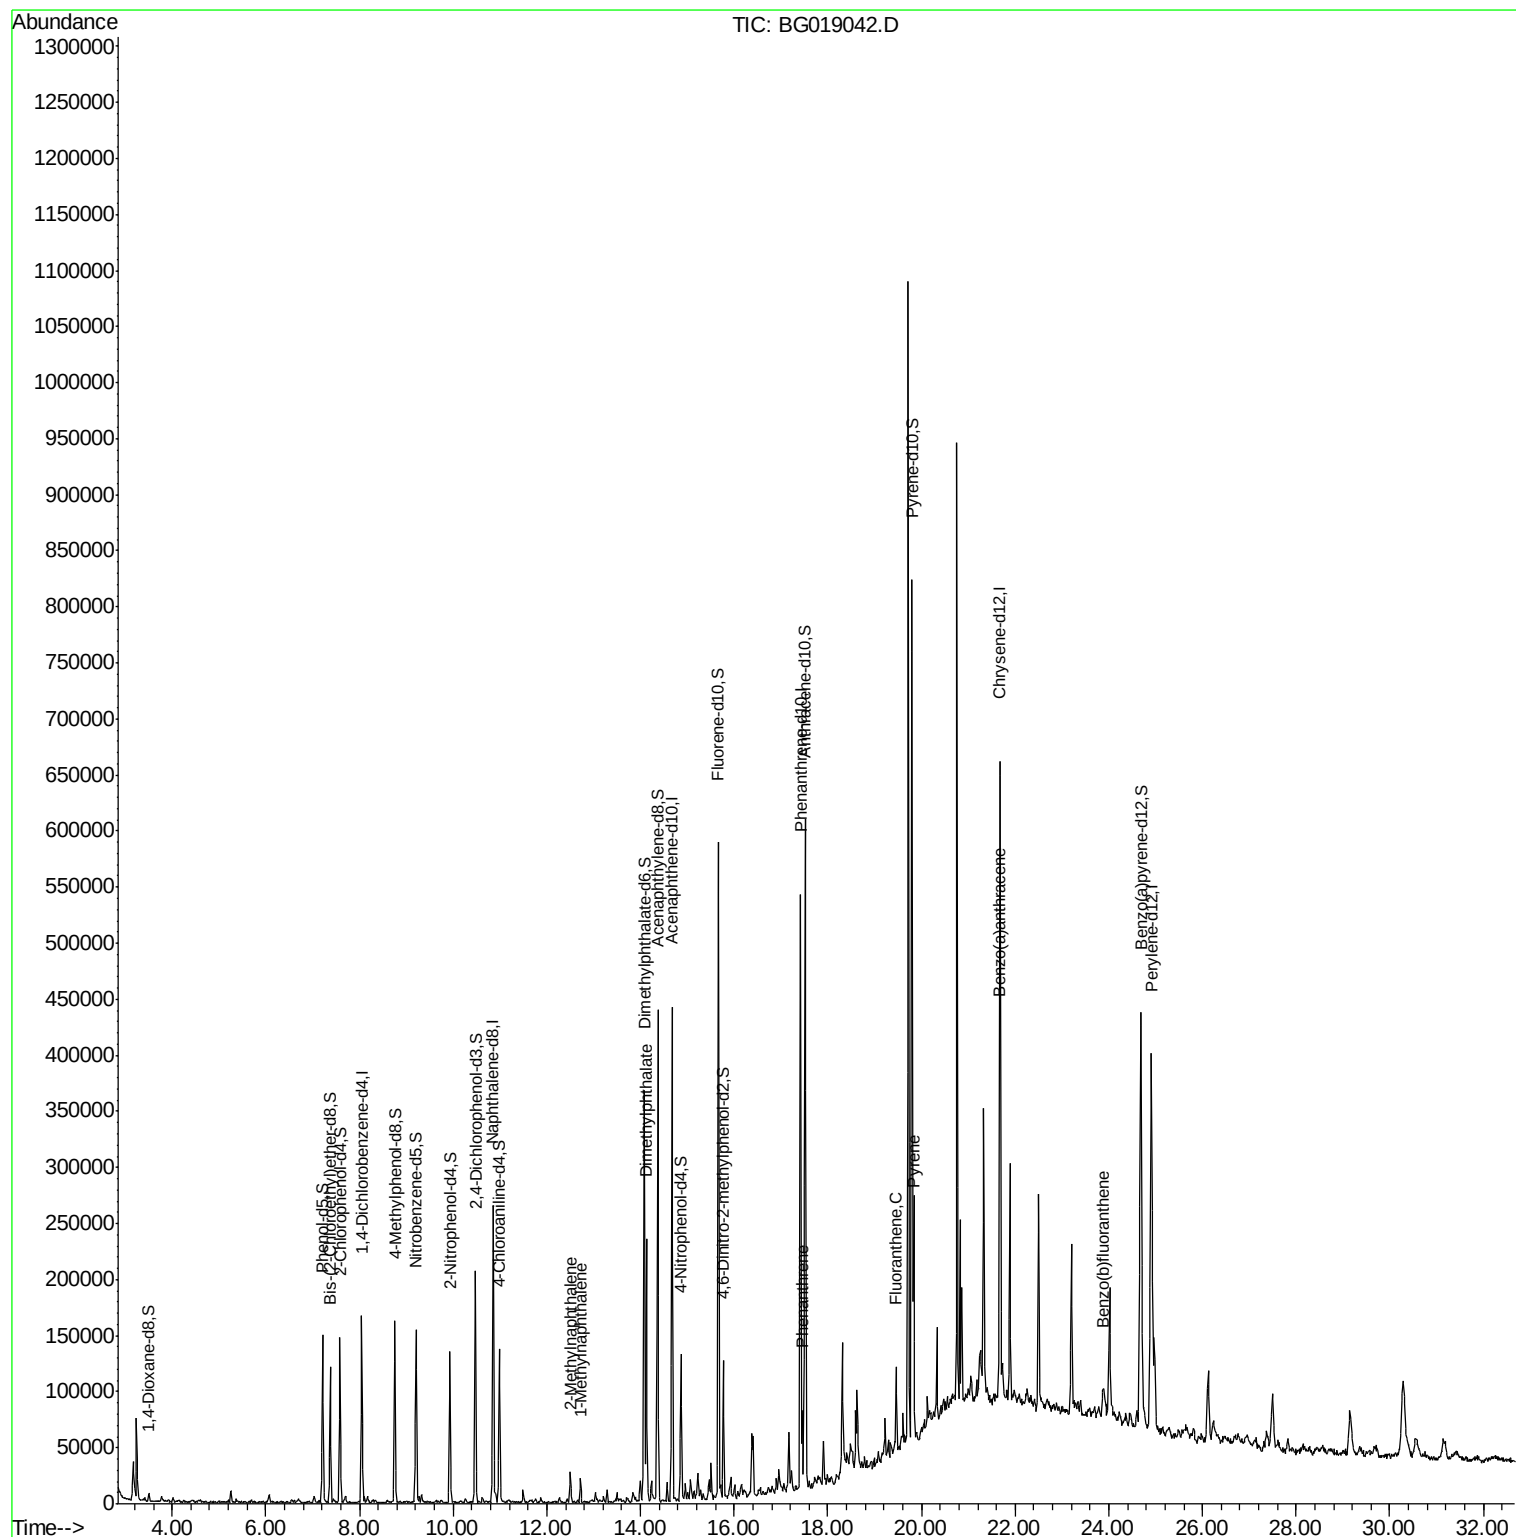

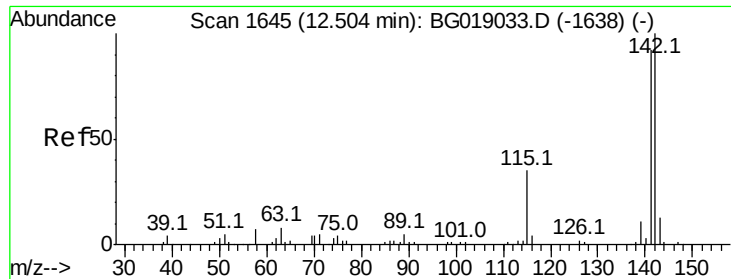


#34
 2-Methylnaphthalene
 Concen: 1.46 ng/ul
 RT: 12.51 min Scan# 1645
 Delta R.T. 0.00 min
 Lab File: BG019042.D
 Acq: 6 Oct 2015 00:39

Instrument :
 BNA_G
 ClientSampleId :
 E5MY2




Tot Ion:142 Resp: 12497
 Ion Ratio Lower Upper
 142 100
 141 91.0 73.4 110.0

Manual Integrations
 APPROVED

MMDadoda
 10/6/2015 5:55:06 PM

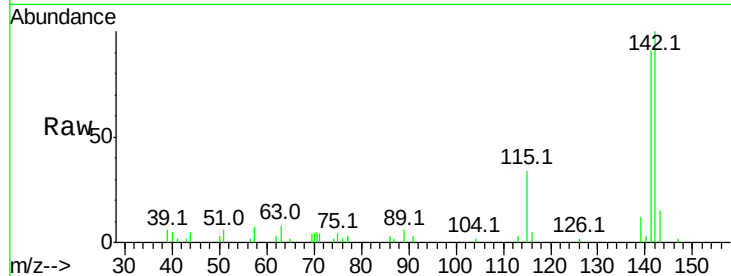


Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E

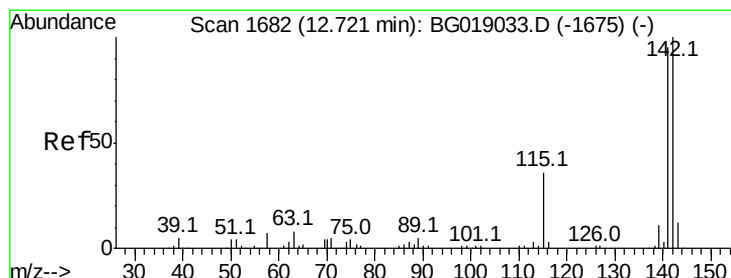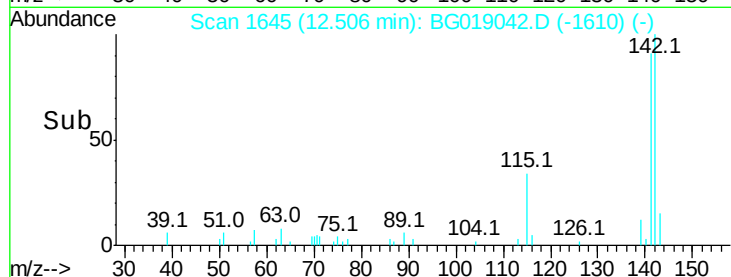
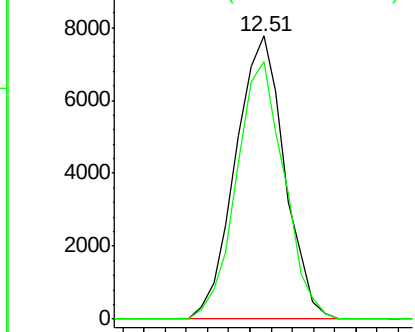



#35
 1-Methylnaphthalene
 Concen: 1.17 ng/ul
 RT: 12.72 min Scan# 1682
 Delta R.T. 0.00 min
 Lab File: BG019042.D
 Acq: 6 Oct 2015 00:39

Tgt Ion:142 Resp: 9789
 Ion Ratio Lower Upper
 142 100
 141 84.7 74.8 112.2
 116 4.4 3.2 4.8

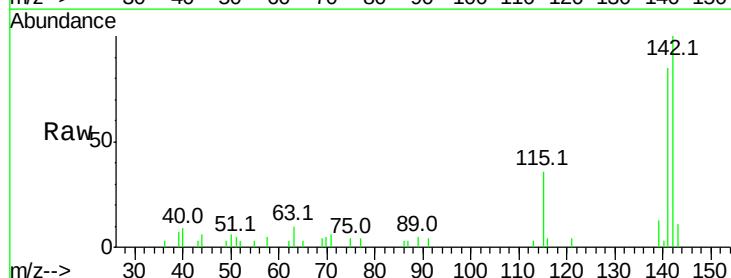

Abundance Ion 142.00 (141.70 to 142.70): E
 Ion 141.00 (140.70 to 141.70): E
 Ion 116.00 (115.70 to 116.70): E

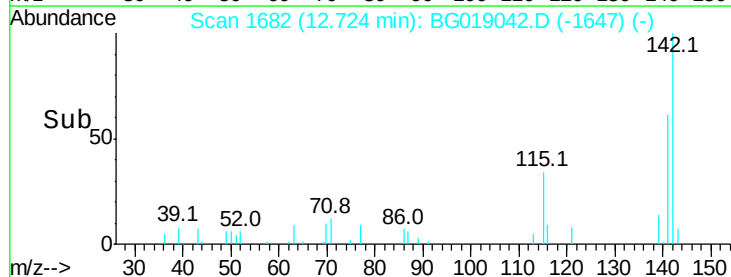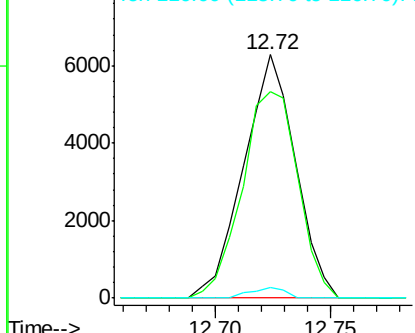

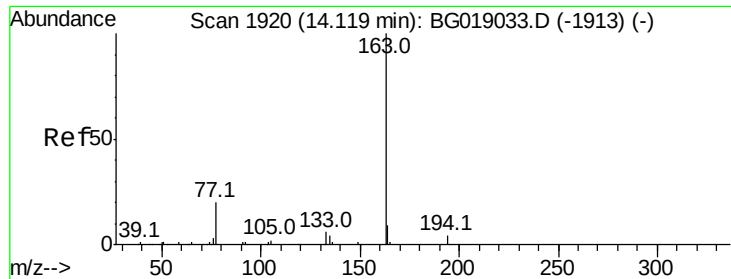





#45
Dimethylphthalate
Concen: 12.91 ng/ul
RT: 14.12 min Scan# 1920
Delta R.T. 0.00 min
Lab File: BG019042.D
Acq: 6 Oct 2015 00:39

Instrument :
BNA_G
ClientSampled :
E5MY2

Tot Ion	Ratio	Resp	Lower	Upper
163	100	149830		
194	3.5		3.3	4.9
164	10.7		8.1	12.1




Manual Integrations
APPROVED


MMDadoda
10/6/2015 5:55:06 PM

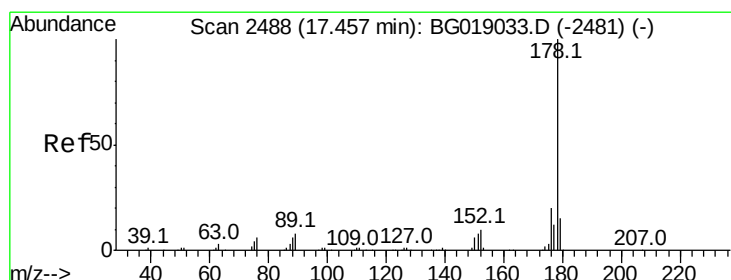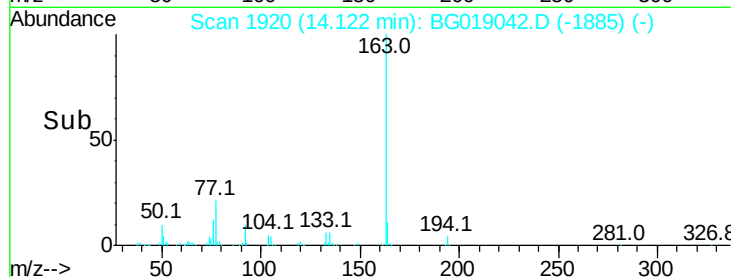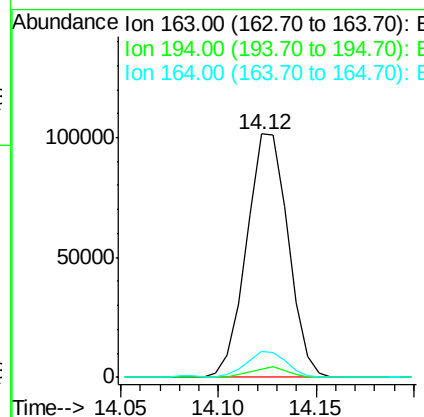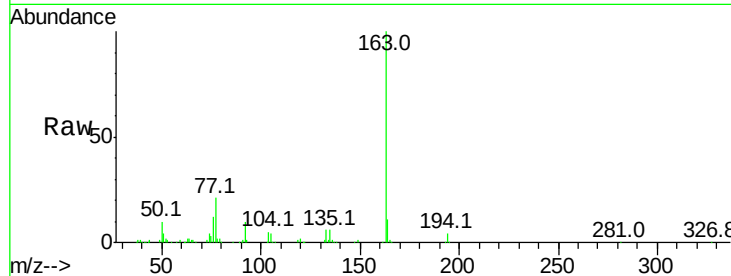

#70
Phenanthrene
Concen: 2.20 ng/ul
RT: 17.46 min Scan# 2488
Delta R.T. 0.00 min
Lab File: BG019042.D
Acq: 6 Oct 2015 00:39

Tgt Ion	Ratio	Resp	Lower	Upper
178	100	39436		
179	16.9		12.5	18.7
176	18.1		15.4	23.0

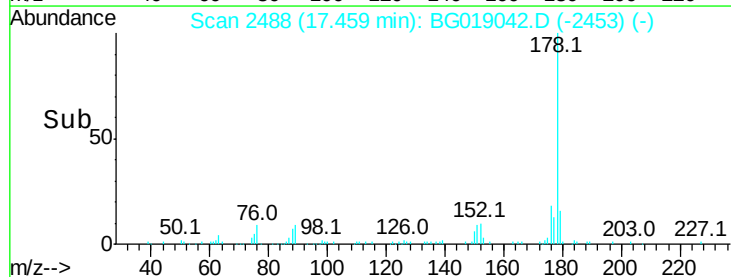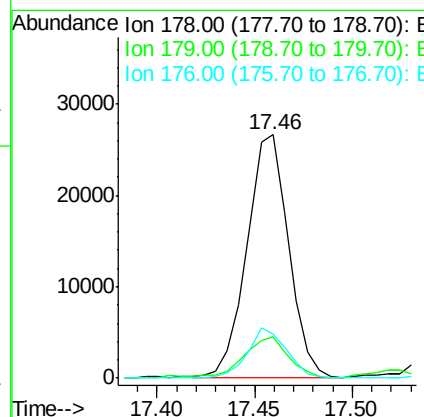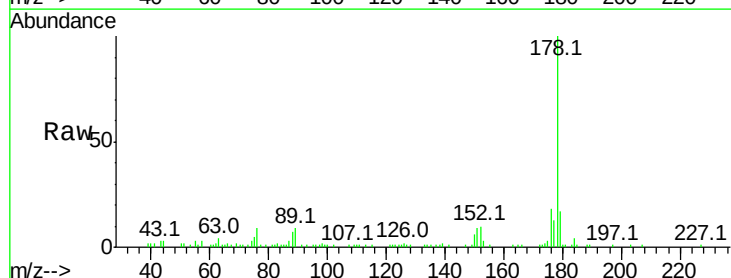

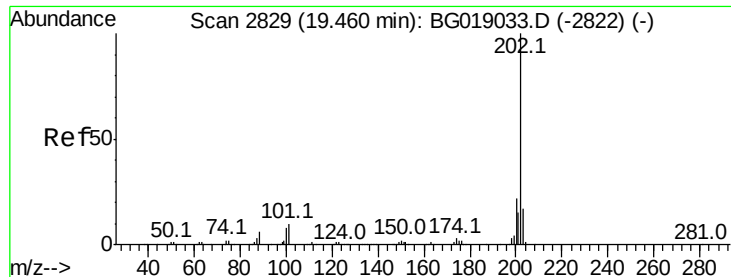





#77
Fluoranthene
 Concen: 2.00 ng/ul
 RT: 19.46 min Scan# 2829
 Delta R.T. 0.00 min
 Lab File: BG019042.D
 Acq: 6 Oct 2015 00:39

Instrument :
 BNA_G
 ClientSampleId :
 E5MY2

Tot Ion:	202	Resp:	41748
Ion Ratio	Lower	Upper	
202	100		
101	10.0	9.0	13.4
100	8.9	6.9	10.3




Manual Integrations
 APPROVED


MMDadoda
 10/6/2015 5:55:06 PM

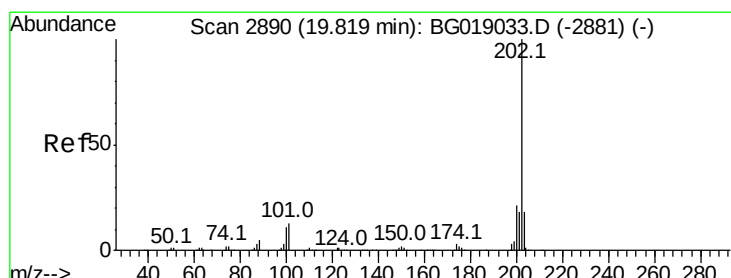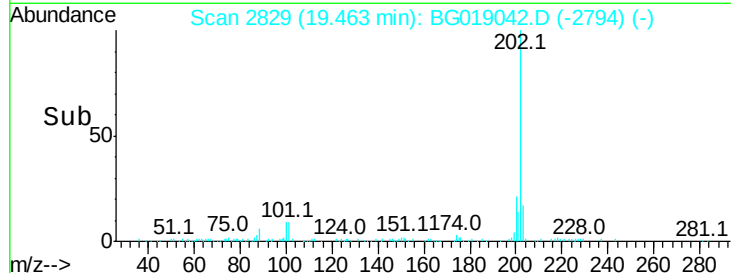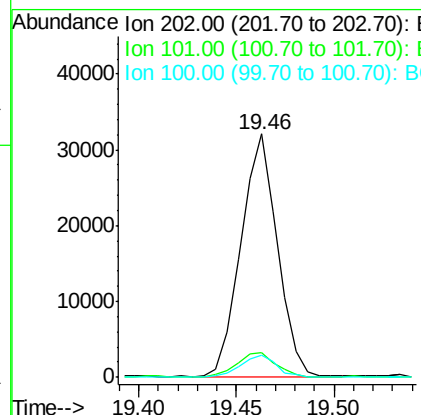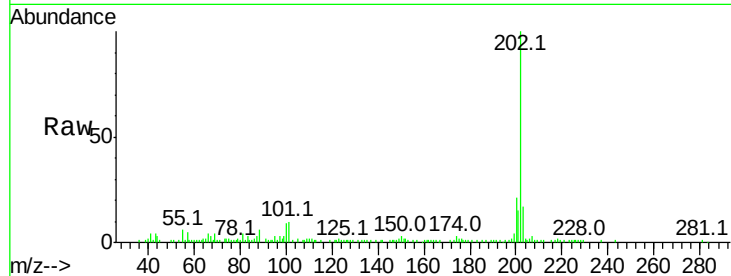

#80
Pyrene
 Concen: 1.73 ng/ul
 RT: 19.82 min Scan# 2890
 Delta R.T. 0.00 min
 Lab File: BG019042.D
 Acq: 6 Oct 2015 00:39

Tgt Ion:	202	Resp:	36176
Ion Ratio	Lower	Upper	
202	100		
101	10.1	10.2	15.2#
100	9.9	8.5	12.7

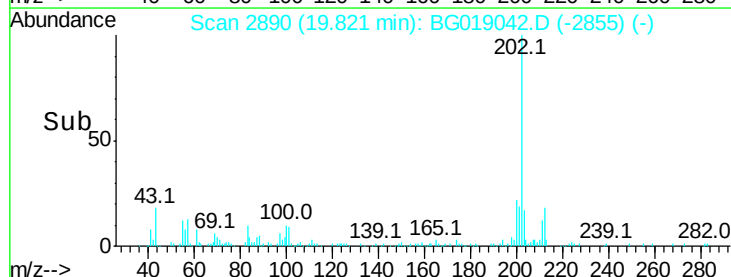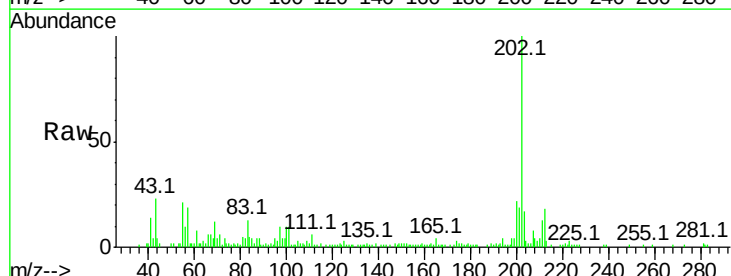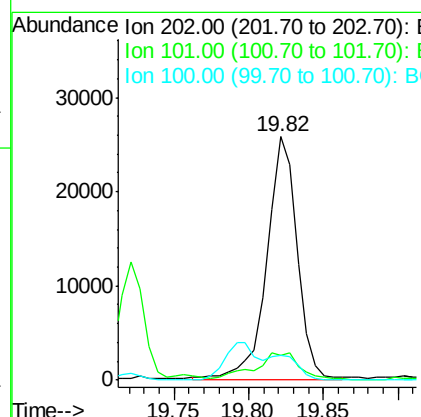

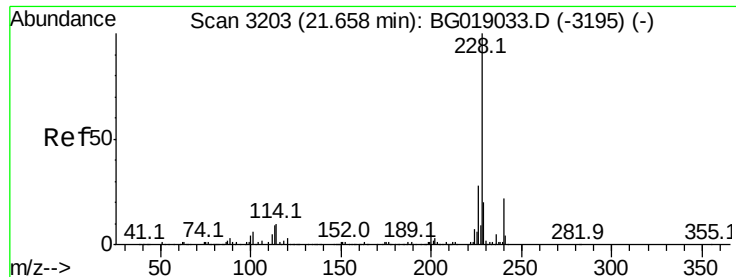





#83
Benzo(a)anthracene
Concen: 1.04 ng/ul
RT: 21.66 min Scan# 3203
Delta R.T. 0.00 min
Lab File: BG019042.D
Acq: 6 Oct 2015 00:39

Instrument :
BNA_G
ClientSampleId :
E5MY2

Tot Ion	Ratio	Lower	Upper
228	100		
229	23.2	16.6	24.8
226	28.8	22.8	34.2

Manual Integrations
APPROVED

MMDadoda
10/6/2015 5:55:06 PM

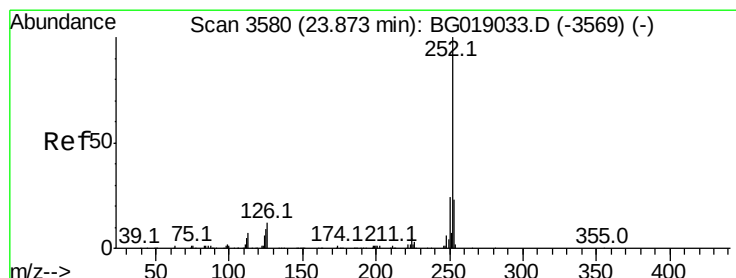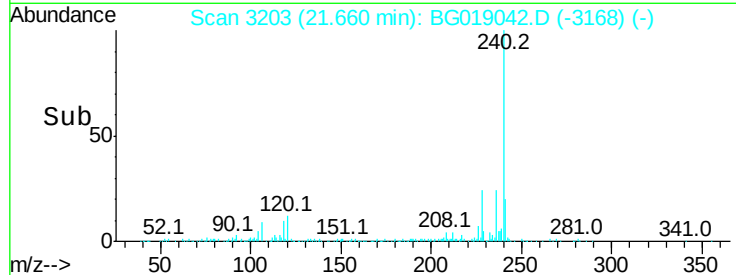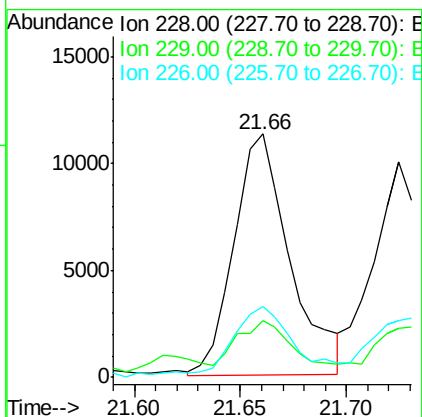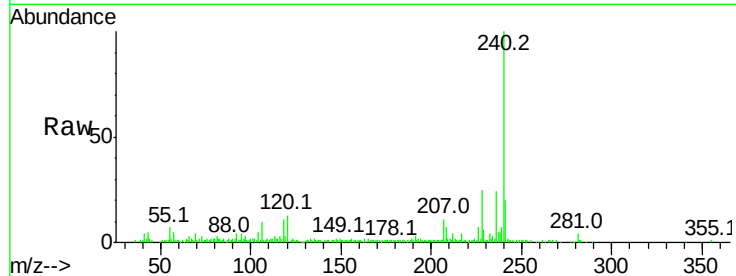

#88
Benzo(b)fluoranthene
Concen: 1.10 ng/ul m
RT: 23.88 min Scan# 3581
Delta R.T. 0.01 min
Lab File: BG019042.D
Acq: 6 Oct 2015 00:39

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.7	17.4	26.2
125	15.4	8.1	12.1#

