

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100518\
 Data File : BG037178.D
 Acq On : 5 Oct 2018 7:22
 Operator : JU/SJ
 Sample : J5241-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 100218-DBRI-E-U-S

Quant Time: Oct 05 08:51:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	44767	20.00	ng	-0.02
21) Naphthalene-d8	10.83	136	181275	20.00	ng	-0.02
38) Acenaphthene-d10	14.65	164	118973	20.00	ng	-0.02
63) Phenanthrene-d10	17.40	188	315443	20.00	ng	-0.02
75) Chrysene-d12	21.67	240	327593	20.00	ng	-0.02
86) Perylene-d12	24.86	264	327155	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	117038	50.14	ng	-0.02
7) Phenol-d6	7.20	99	97607	27.03	ng	-0.02
23) Nitrobenzene-d5	9.19	82	384409	113.56	ng	-0.02
41) 2,4,6-Tribromophenol	16.15	330	163959	115.19	ng	-0.02
44) 2-Fluorobiphenyl	13.28	172	794014	99.40	ng	-0.02
78) Terphenyl-d14	20.01	244	1467505	117.79	ng	-0.02
Target Compounds						
49) Dimethylphthalate	14.11	163	61856	6.459	ng	Qvalue # 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100518\
Data File : BG037178.D
Acq On : 5 Oct 2018 7:22
Operator : JU/SJ
Sample : J5241-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
100218-DBRI-E-U-S

Quant Time: Oct 05 08:51:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

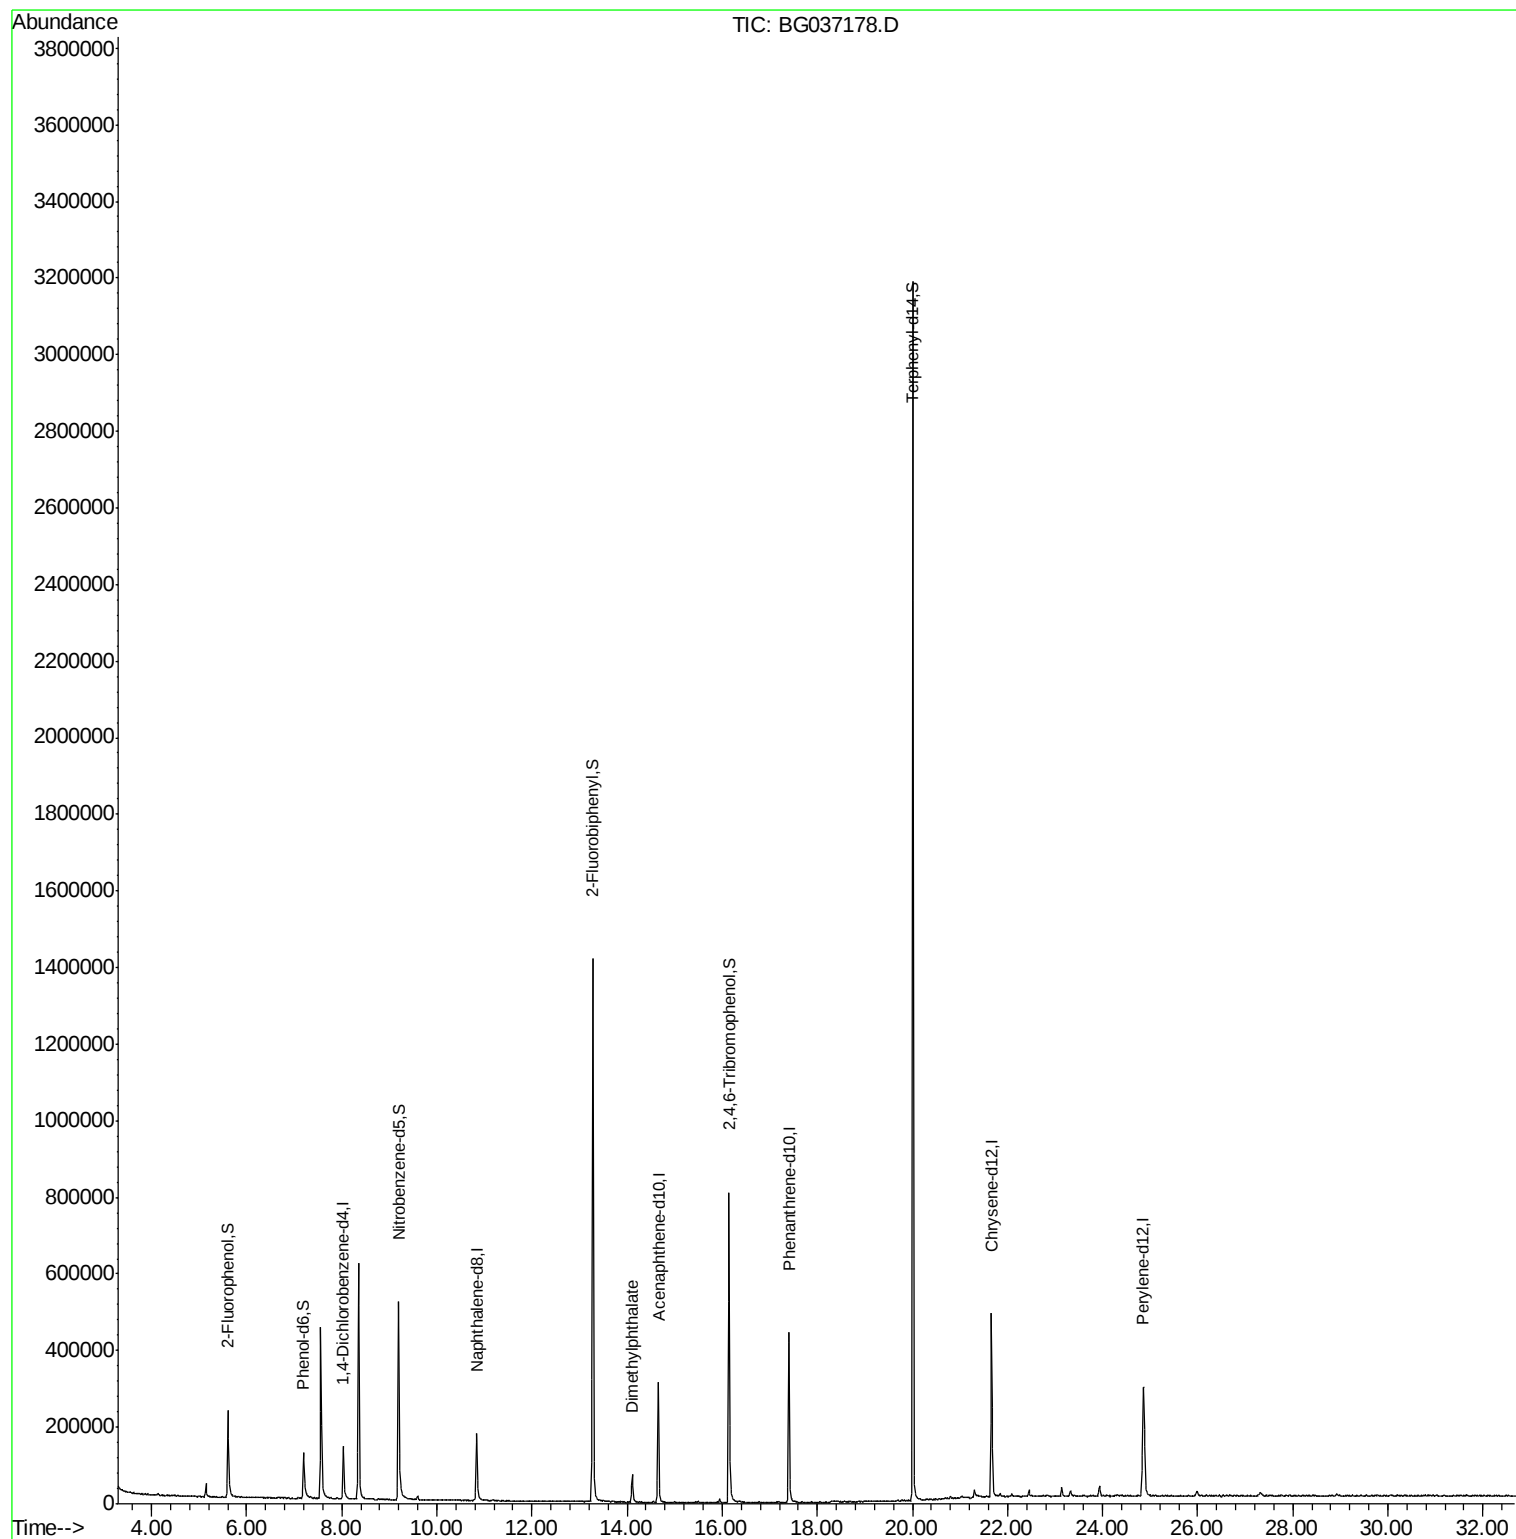

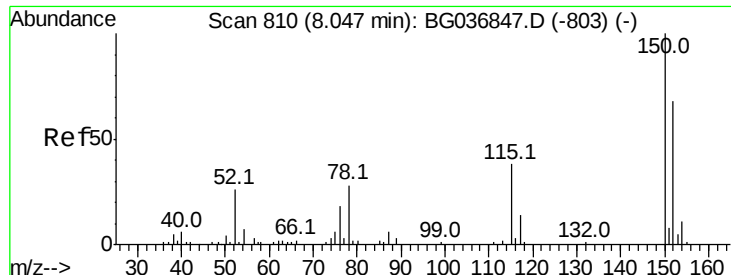


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 807
Delta R.T. -0.02 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22

Instrument :
BNA_G
ClientSampleId :
100218-DBRI-E-U-S

Tot Ion	Ratio	Lower	Upper
152	100		
150	151.9	119.5	179.3
115	62.2	44.5	66.7



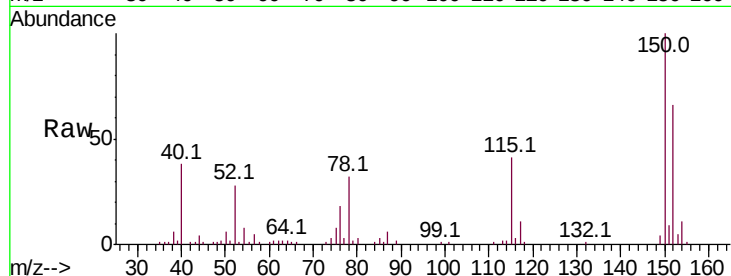


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

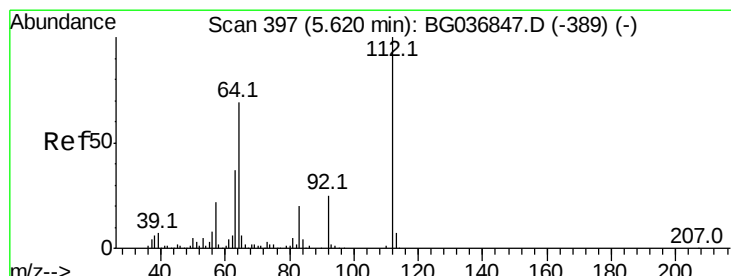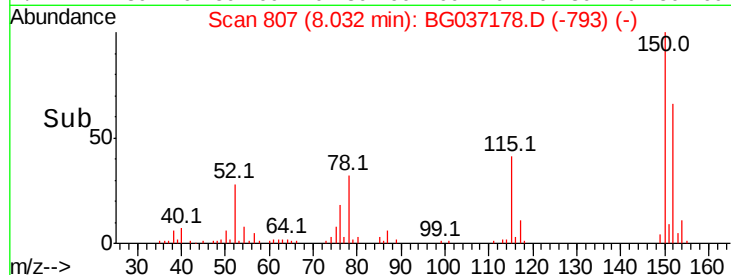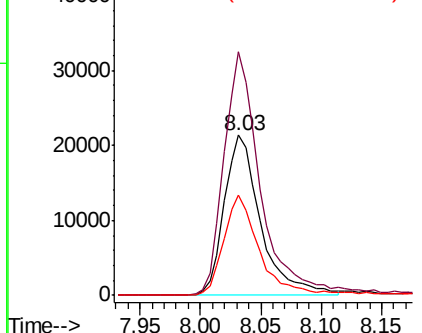

#5

2-Fluorophenol
Concen: 50.138 ng
RT: 5.60 min Scan# 394
Delta R.T. -0.02 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22

Tgt Ion	Ratio	Lower	Upper
112	100		
64	70.6	57.2	85.8
63	38.6	30.8	46.2


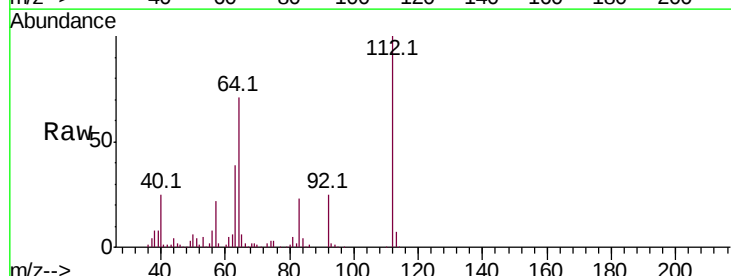


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

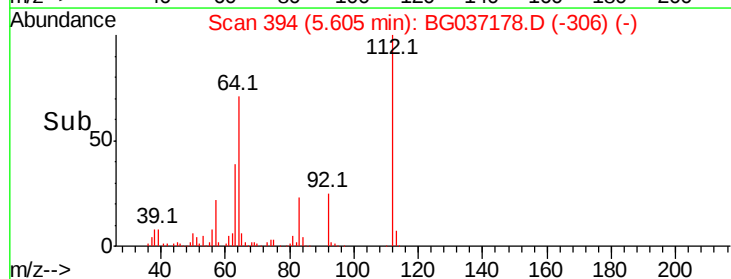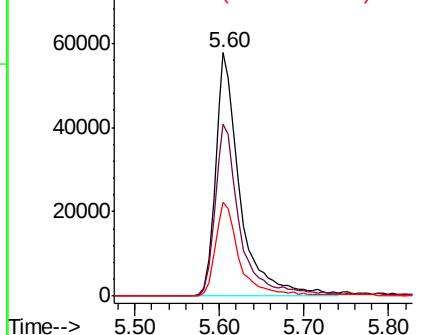



#7

Phenol-d6

Concen: 27.026 ng

RT: 7.20 min Scan# 665

Delta R.T. -0.02 min

Lab File: BG037178.D

Acq: 5 Oct 2018 7:22

Instrument :

BNA_G

ClientSampleId :

100218-DBRI-E-U-S


Tot Ion: 99 Resp: 97607

Ion Ratio Lower Upper

99 100

42 21.3 16.5 24.7

71 36.3 29.4 44.2


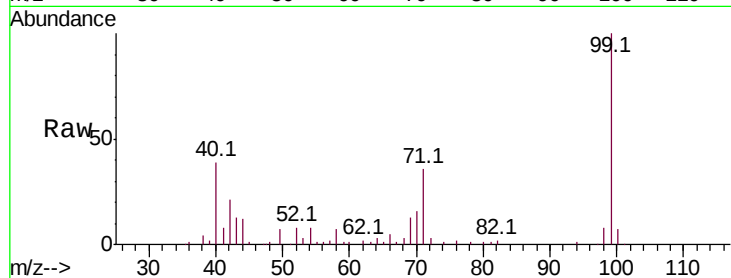


Abundance

Ion 99.00 (98.70 to 99.70): BGC

Ion 42.00 (41.70 to 42.70): BGC

Ion 71.00 (70.70 to 71.70): BGC

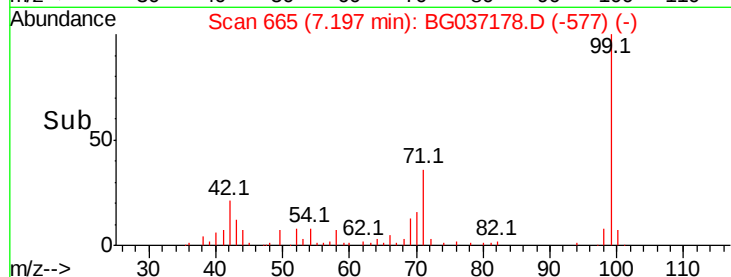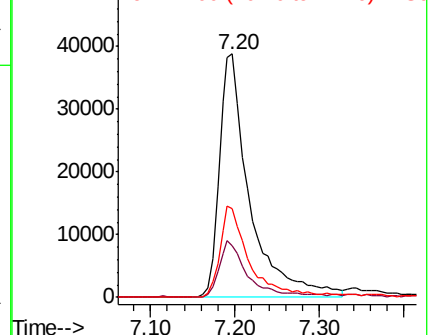

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.83 min Scan# 1284

Delta R.T. -0.02 min

Lab File: BG037178.D

Acq: 5 Oct 2018 7:22

Tgt Ion: 136 Resp: 181275


Ion Ratio Lower Upper

136 100

137 12.0 8.8 13.2

54 10.4 9.2 13.8

68 6.8 5.8 8.6

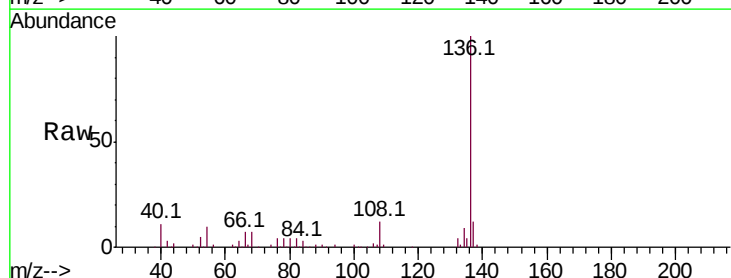



Abundance


Ion 136.00 (135.70 to 136.70): BGC

Ion 137.00 (136.70 to 137.70): BGC

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

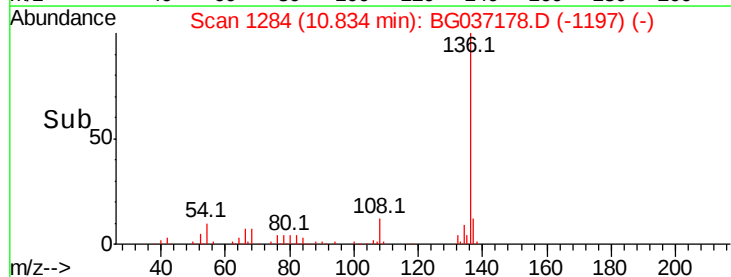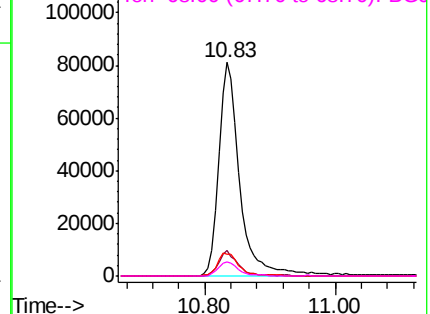


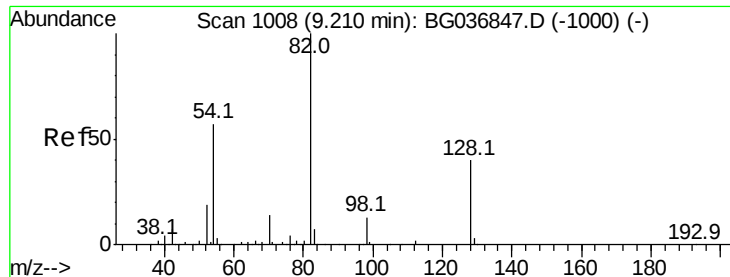




#23
Nitrobenzene-d5
Concen: 113.559 ng
RT: 9.19 min Scan# 1005
Delta R.T. -0.02 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22

Instrument :
BNA_G
ClientSampleId :
100218-DBRI-E-U-S

Tot Ion	Ratio	Lower	Upper
82	100		
128	40.1	33.3	49.9
54	57.3	45.1	67.7

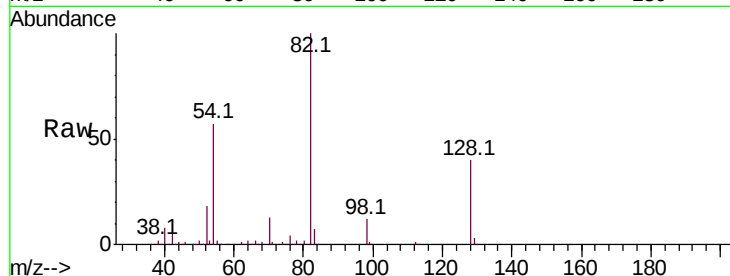


Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

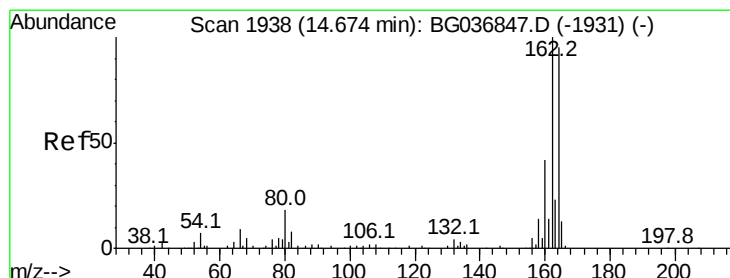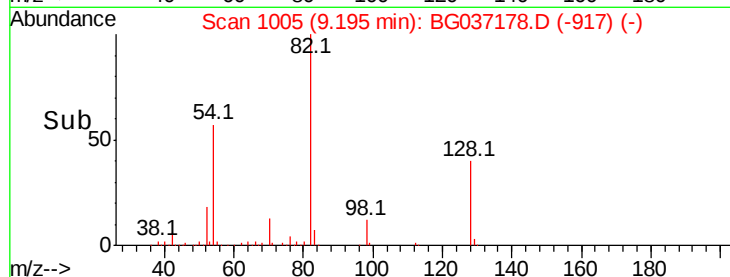
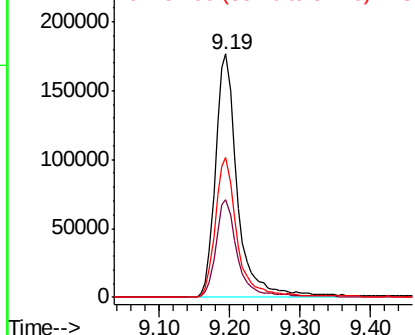


#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.65 min Scan# 1934
Delta R.T. -0.02 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.8	80.7	121.1
160	44.1	35.3	52.9

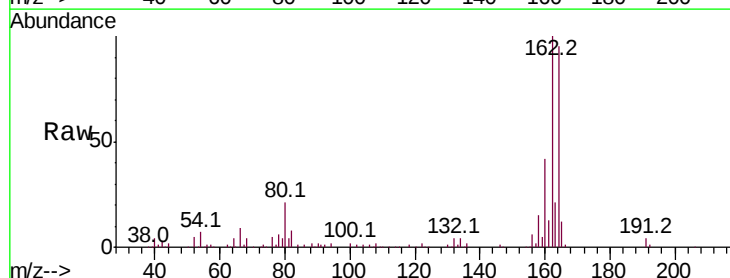

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

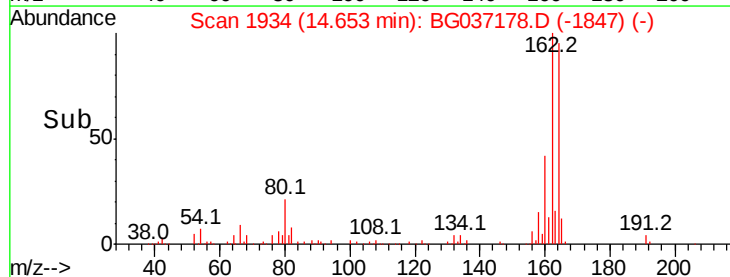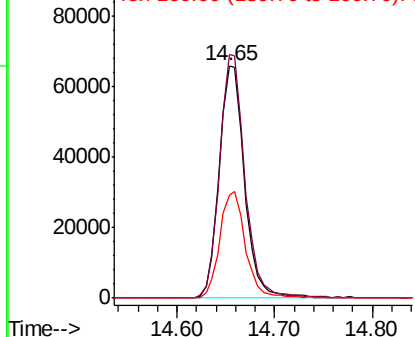




#41
 2,4,6-Tribromophenol
 Concen: 115.185 ng
 RT: 16.15 min Scan# 2188
 Delta R.T. -0.02 min
 Lab File: BG037178.D
 Acq: 5 Oct 2018 7:22

Instrument :
 BNA_G
 ClientSampleId :
 100218-DBRI-E-U-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	75.4	113.2
141	40.5	30.7	46.1


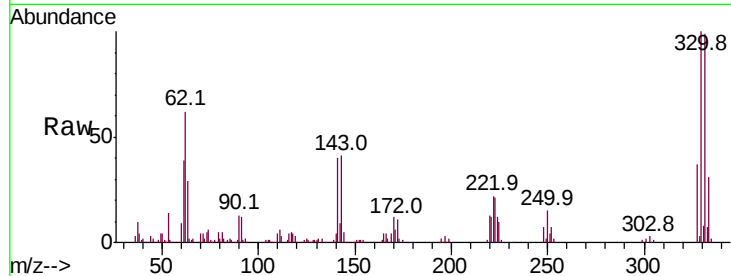


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

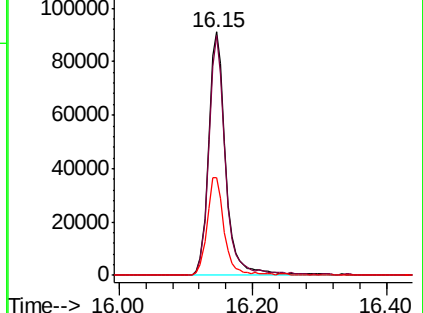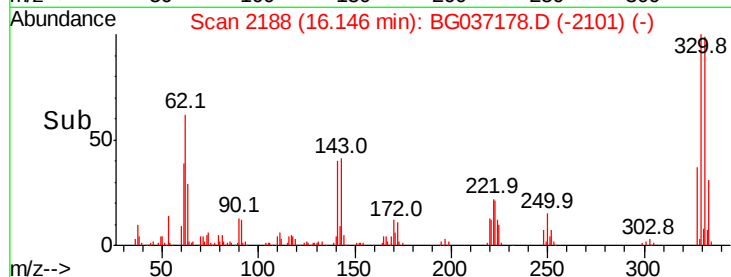

#44
 2-Fluorobiphenyl
 Concen: 99.400 ng
 RT: 13.28 min Scan# 1700
 Delta R.T. -0.02 min
 Lab File: BG037178.D
 Acq: 5 Oct 2018 7:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.8	31.3	46.9
170	25.1	21.0	31.6


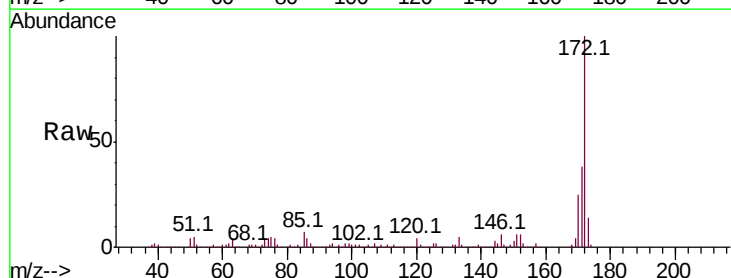



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



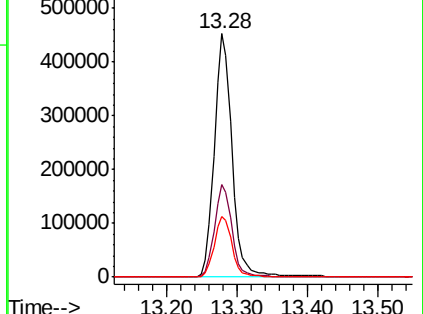
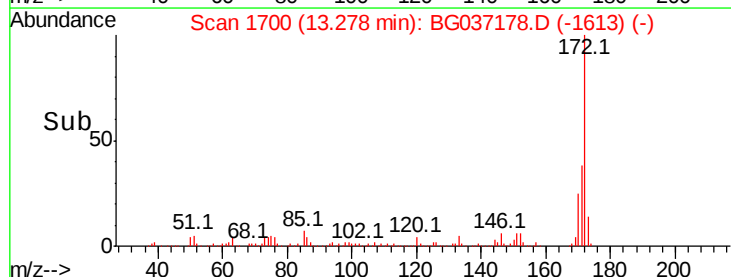


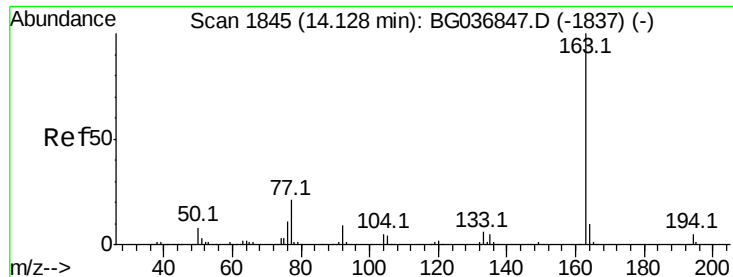

#49
Dimethylphthalate
Concen: 6.459 ng
RT: 14.11 min Scan# 1841
Delta R.T. -0.02 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22




Instrument :
BNA_G
ClientSampleId :
100218-DBRI-E-U-S


Tot Ion:163 Resp: 61856
Ion Ratio Lower Upper
163 100
194 3.9 4.0 6.0#
164 9.9 8.1 12.1

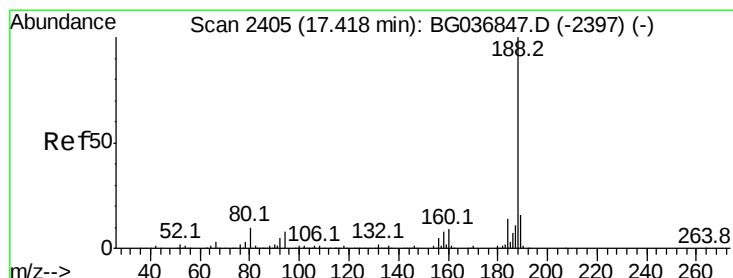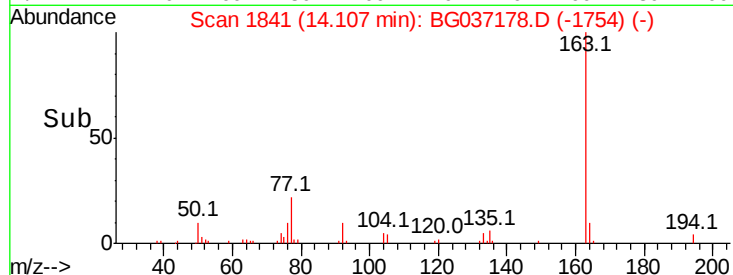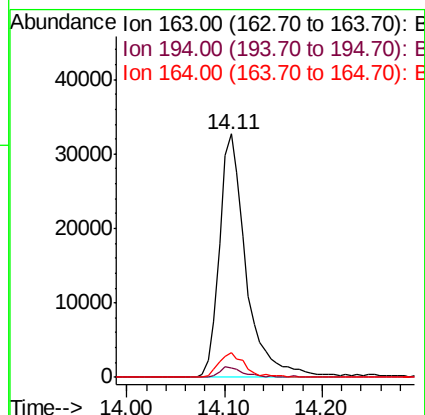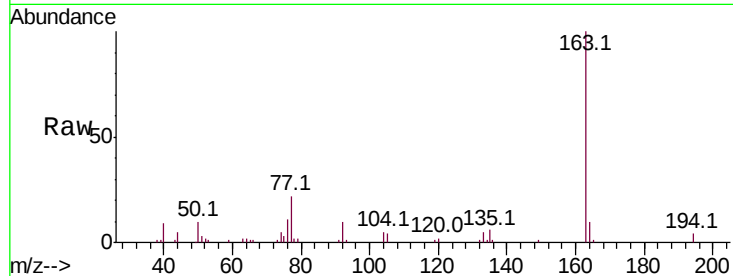

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.40 min Scan# 2402
Delta R.T. -0.02 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22

Tgt Ion:188 Resp: 315443
Ion Ratio Lower Upper
188 100
94 8.4 6.7 10.1
80 9.5 8.1 12.1

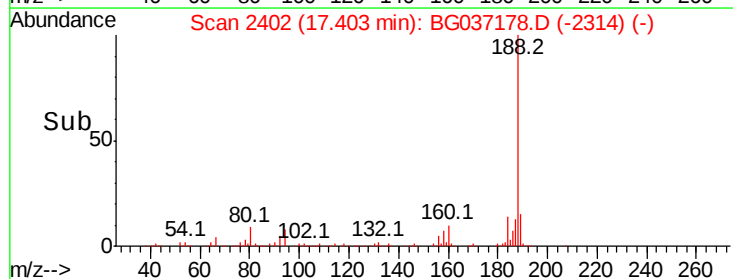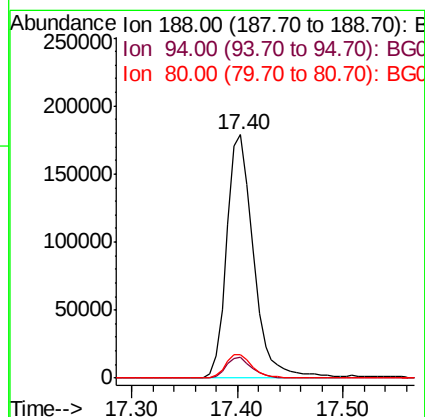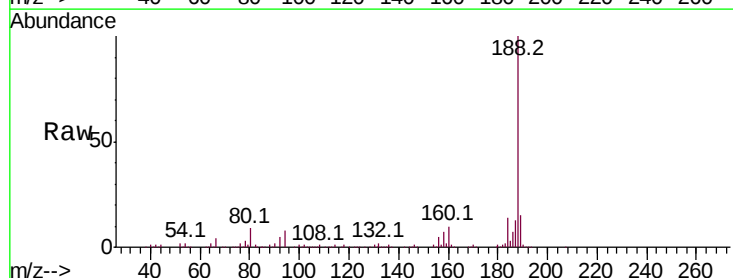

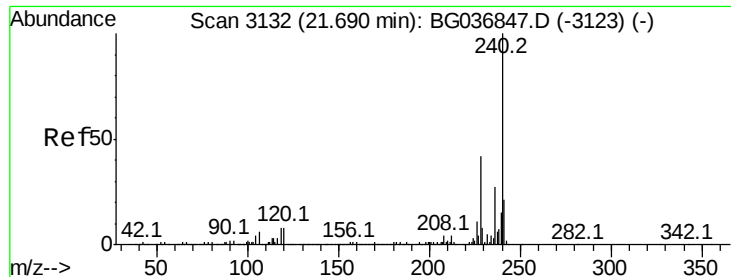

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3128

Delta R.T. -0.02 min

Lab File: BG037178.D

Acq: 5 Oct 2018 7:22

Instrument :

BNA_G

ClientSampleId :

100218-DBRI-E-U-S


Tot Ion:240 Resp: 327593

Ion Ratio Lower Upper

240 100

120 8.5 6.9 10.3




236 26.5 21.2 31.8

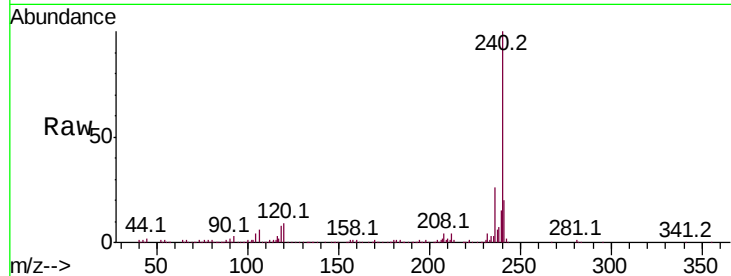

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

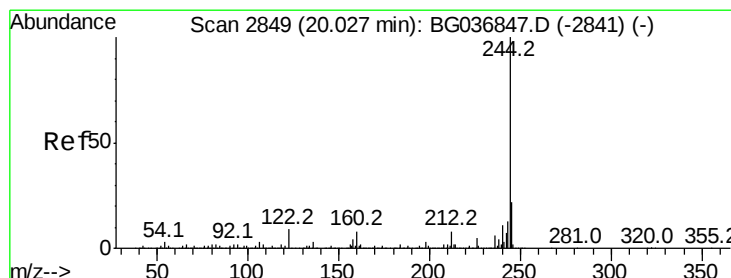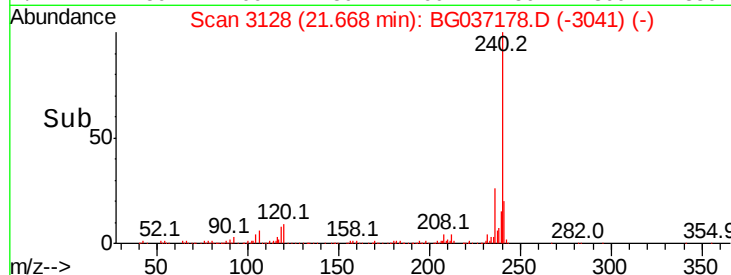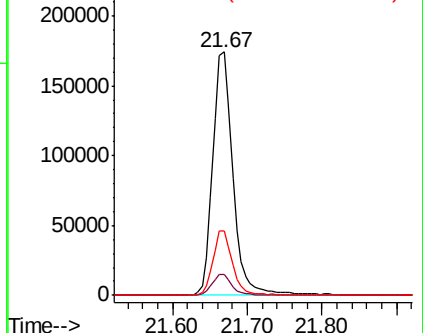

#78

Terphenyl-d14

Concen: 117.792 ng

RT: 20.01 min Scan# 2846

Delta R.T. -0.02 min

Lab File: BG037178.D

Acq: 5 Oct 2018 7:22


Tgt Ion:244 Resp: 1467505

Ion Ratio Lower Upper

244 100

212 9.3 7.0 10.6



122 9.8 7.1 10.7

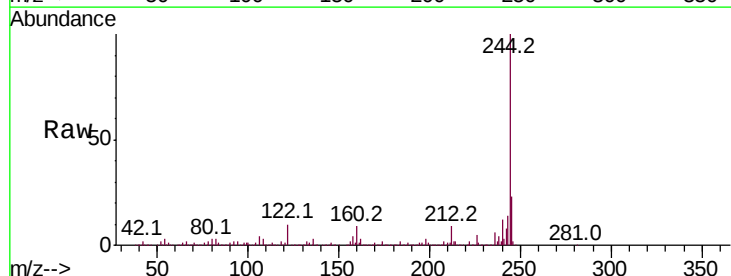


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

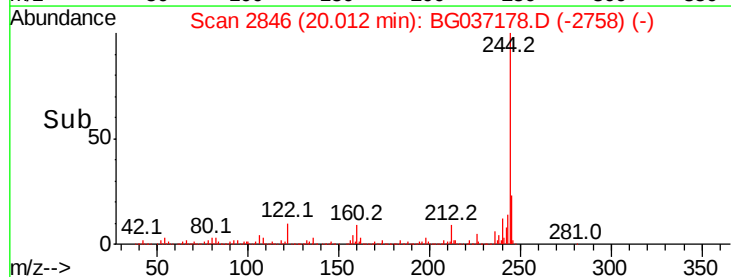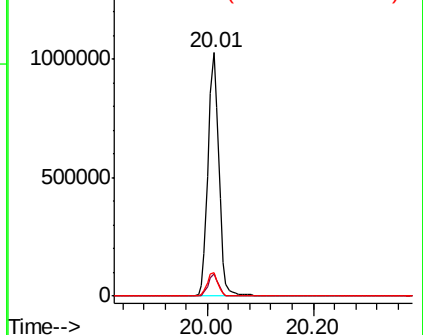


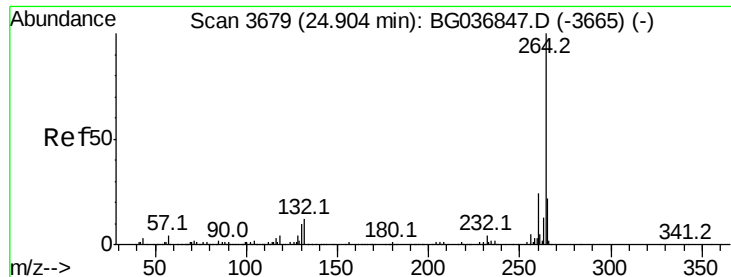

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.86 min Scan# 3671
Delta R.T. -0.04 min
Lab File: BG037178.D
Acq: 5 Oct 2018 7:22

Instrument :
BNA_G
ClientSampleId :
100218-DBRI-E-U-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.6	29.4
265	21.6	17.4	26.0

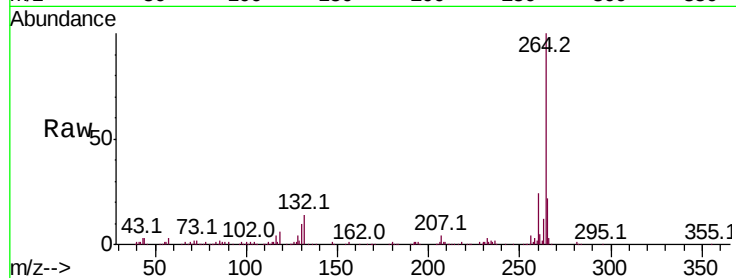

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

