

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100518\
 Data File : BG037182.D
 Acq On : 5 Oct 2018 9:58
 Operator : JU/SJ
 Sample : J5241-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 100218-JETT-E-D-S

Quant Time: Oct 05 11:11:44 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	43114	20.00	ng	-0.02
21) Naphthalene-d8	10.84	136	175358	20.00	ng	-0.02
38) Acenaphthene-d10	14.66	164	114729	20.00	ng	-0.02
63) Phenanthrene-d10	17.40	188	301103	20.00	ng	-0.02
75) Chrysene-d12	21.67	240	312445	20.00	ng	-0.02
86) Perylene-d12	24.86	264	314095	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	115600	51.42	ng	-0.01
7) Phenol-d6	7.19	99	96875	27.85	ng	-0.02
23) Nitrobenzene-d5	9.19	82	361241	110.32	ng	-0.02
41) 2,4,6-Tribromophenol	16.14	330	150354	109.53	ng	-0.02
44) 2-Fluorobiphenyl	13.28	172	728639	94.59	ng	-0.02
78) Terphenyl-d14	20.01	244	1360971	114.54	ng	-0.02
Target Compounds						
49) Dimethylphthalate	14.10	163	173973	18.839	ng	Qvalue # 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100518\
Data File : BG037182.D
Acq On : 5 Oct 2018 9:58
Operator : JU/SJ
Sample : J5241-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
100218-JETT-E-D-S

Quant Time: Oct 05 11:11:44 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

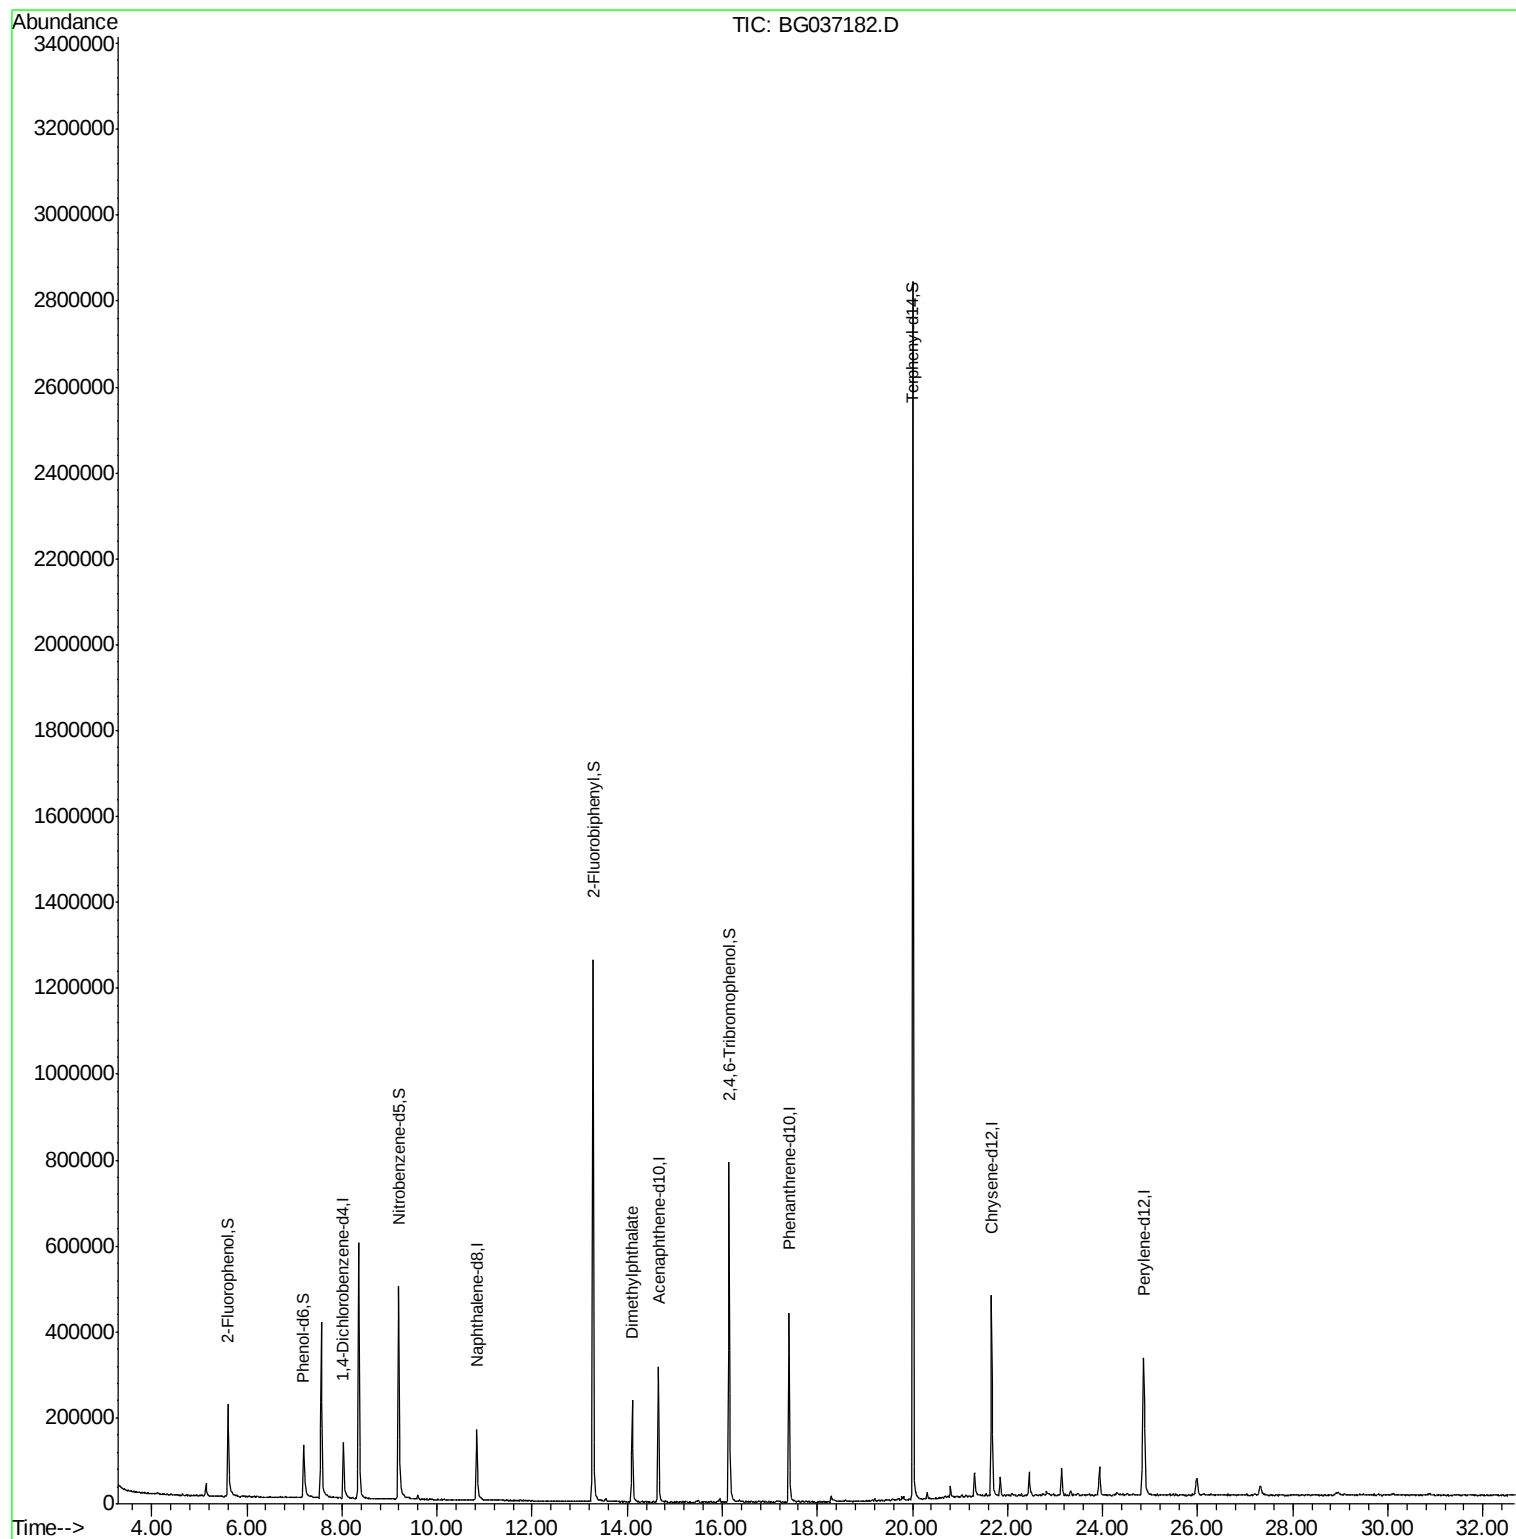

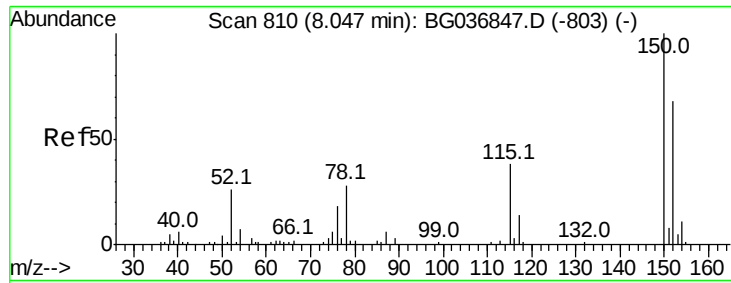


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.03 min Scan# 807
 Delta R.T. -0.02 min
 Lab File: BG037182.D
 Acq: 5 Oct 2018 9:58

Instrument :
 BNA_G
 ClientSampleId :
 100218-JETT-E-D-S

Tot Ion:152 Resp: 43114
 Ion Ratio Lower Upper
 152 100
 150 156.9 119.5 179.3
 115 65.9 44.5 66.7

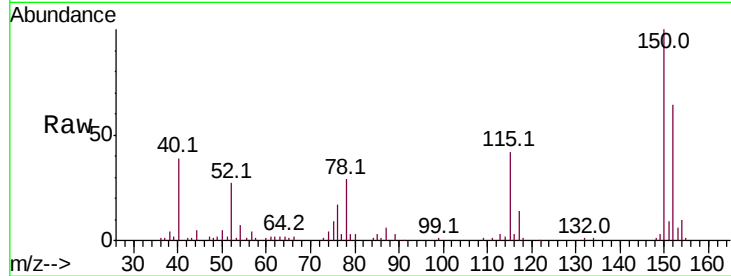


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

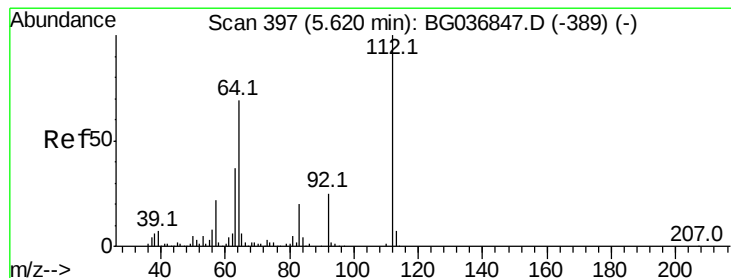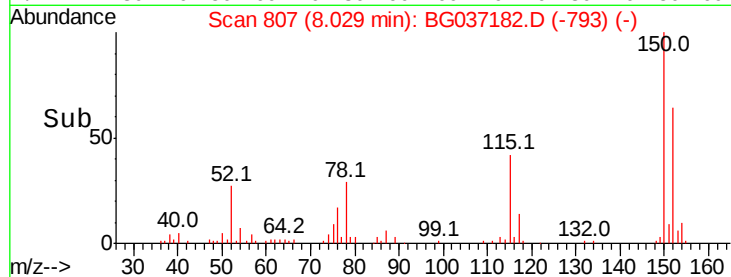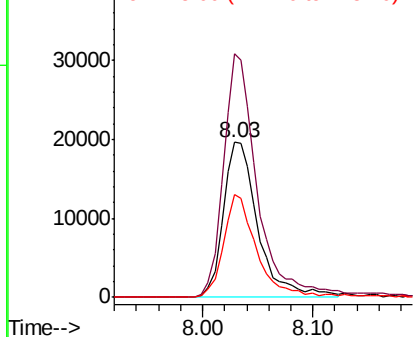



#5

2-Fluorophenol
 Concen: 51.421 ng
 RT: 5.61 min Scan# 395
 Delta R.T. -0.01 min
 Lab File: BG037182.D
 Acq: 5 Oct 2018 9:58

Tgt Ion:112 Resp: 115600
 Ion Ratio Lower Upper
 112 100
 64 72.6 57.2 85.8
 63 39.7 30.8 46.2

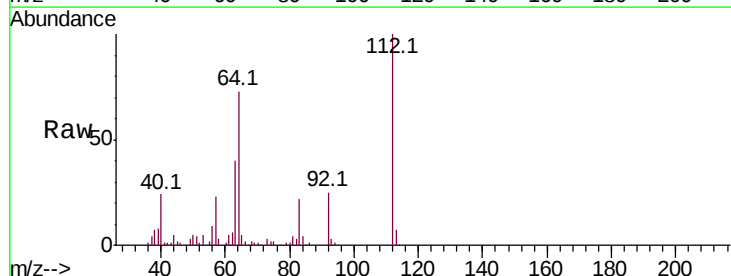

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BG
 Ion 63.00 (62.70 to 63.70): BG

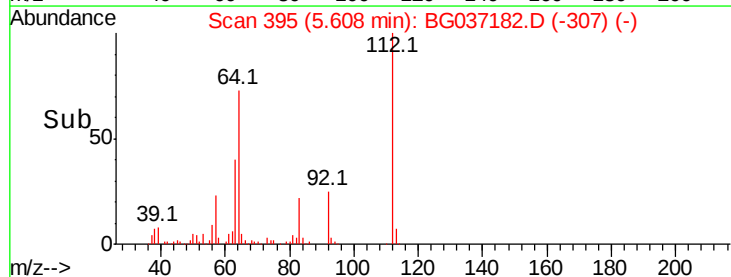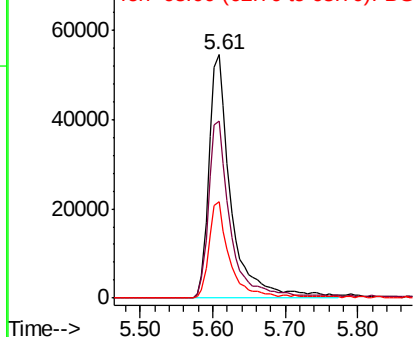



#7

Phenol-d6

Concen: 27.852 ng

RT: 7.19 min Scan# 665

Delta R.T. -0.02 min

Lab File: BG037182.D

Acq: 5 Oct 2018 9:58

Instrument :

BNA_G

ClientSampleId :

100218-JETT-E-D-S


Tot Ion: 99 Resp: 96875

Ion Ratio Lower Upper



99 100

42 21.5 16.5 24.7

71 35.5 29.4 44.2

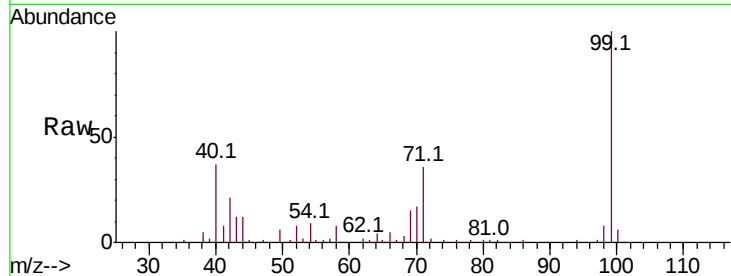

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

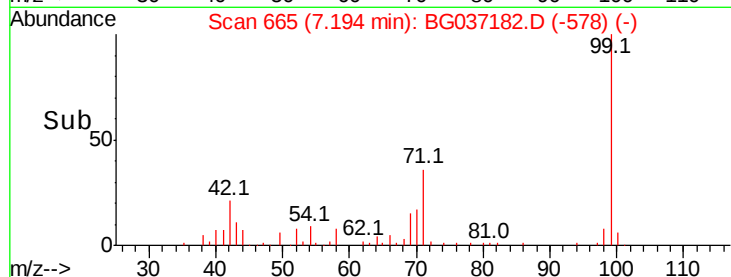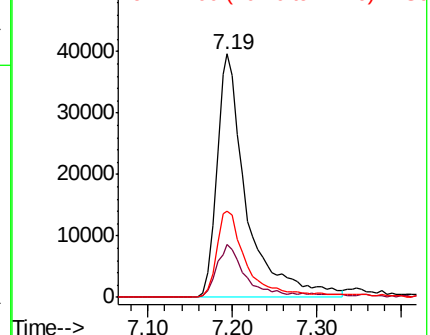

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.84 min Scan# 1285

Delta R.T. -0.02 min

Lab File: BG037182.D

Acq: 5 Oct 2018 9:58

Tgt Ion: 136 Resp: 175358


Ion Ratio Lower Upper

136 100



137 12.0 8.8 13.2

54 11.8 9.2 13.8

68 7.3 5.8 8.6

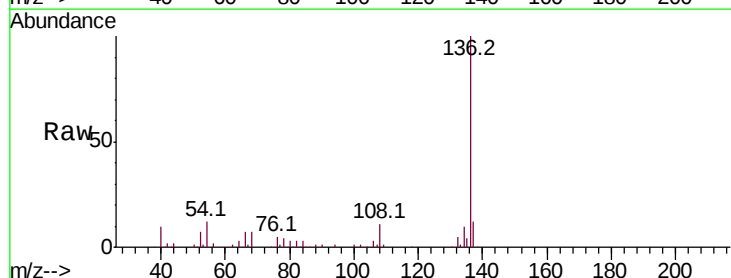

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


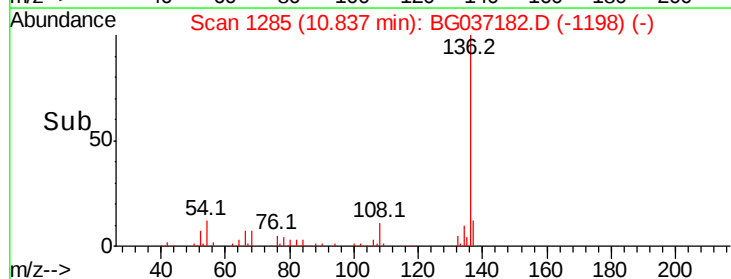
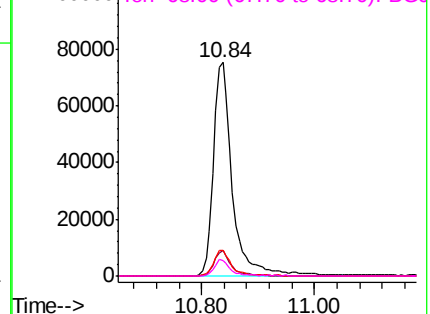




#23
 Nitrobenzene-d5
 Concen: 110.316 ng
 RT: 9.19 min Scan# 1005
 Delta R.T. -0.02 min
 Lab File: BG037182.D
 Acq: 5 Oct 2018 9:58




Instrument :
 BNA_G
 ClientSampleId :
 100218-JETT-E-D-S

Tot Ion	82	Resp	361241
Ion Ratio	Lower	Upper	
82	100		
128	40.6	33.3	49.9
54	60.1	45.1	67.7

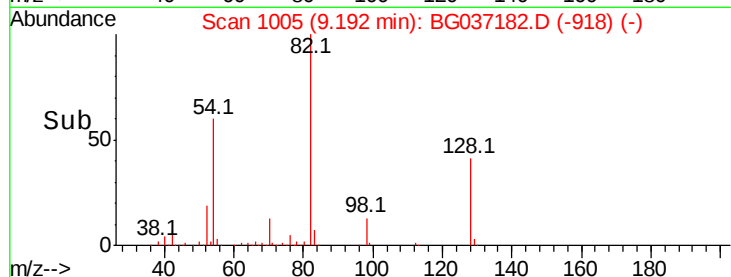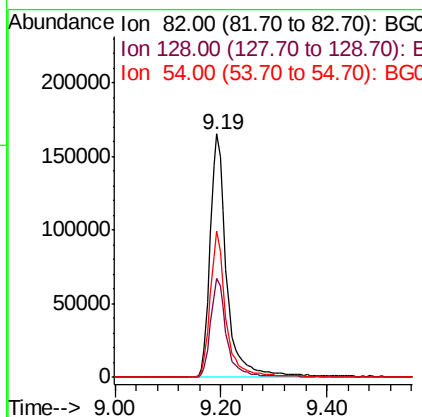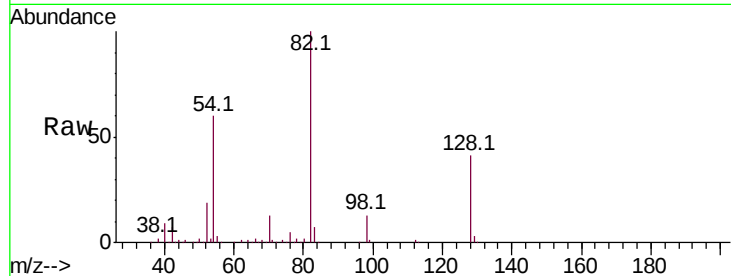

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1935
 Delta R.T. -0.02 min
 Lab File: BG037182.D
 Acq: 5 Oct 2018 9:58

Tgt Ion	164	Resp	114729
Ion Ratio	Lower	Upper	
164	100		
162	104.1	80.7	121.1
160	45.3	35.3	52.9

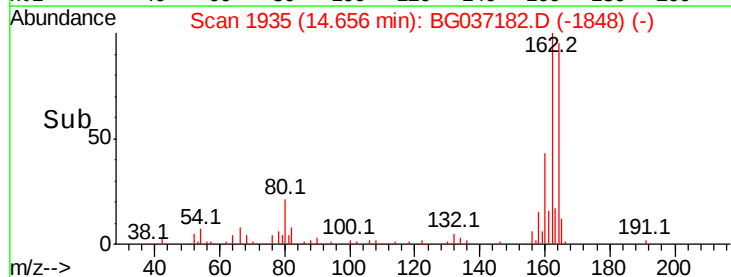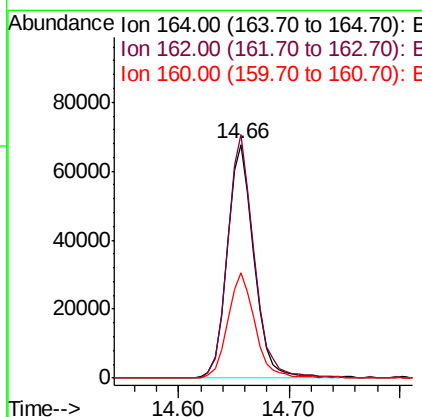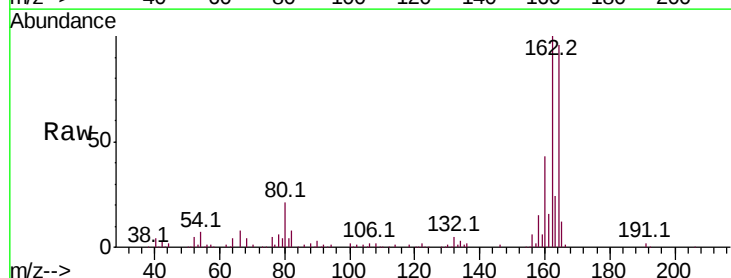




#41
 2,4,6-Tribromophenol
 Concen: 109.535 ng
 RT: 16.14 min Scan# 2188
 Delta R.T. -0.02 min
 Lab File: BG037182.D
 Acq: 5 Oct 2018 9:58

Instrument :
 BNA_G
 ClientSampleId :
 100218-JETT-E-D-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	75.4	113.2
141	41.7	30.7	46.1


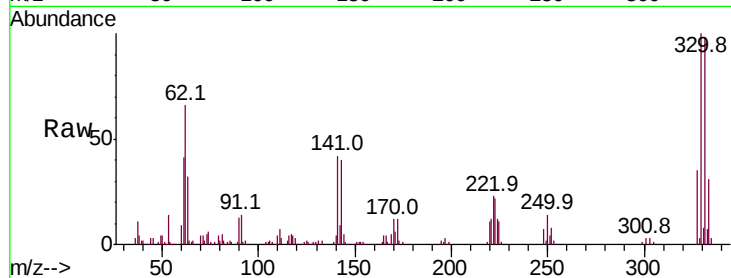


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

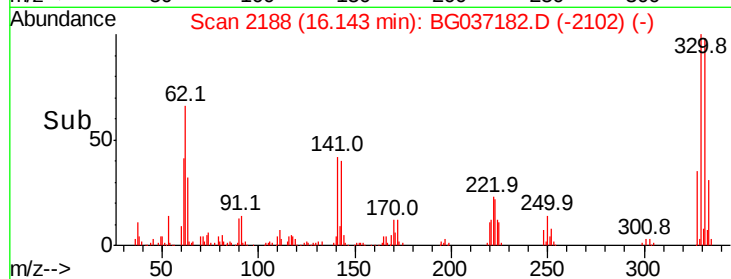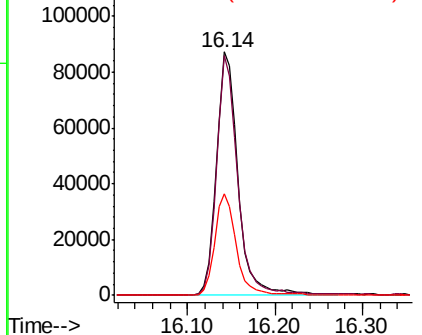

#44
 2-Fluorobiphenyl
 Concen: 94.591 ng
 RT: 13.28 min Scan# 1701
 Delta R.T. -0.02 min
 Lab File: BG037182.D
 Acq: 5 Oct 2018 9:58

Tgt Ion	Ratio	Lower	Upper
172	100		
171	38.5	31.3	46.9
170	25.4	21.0	31.6


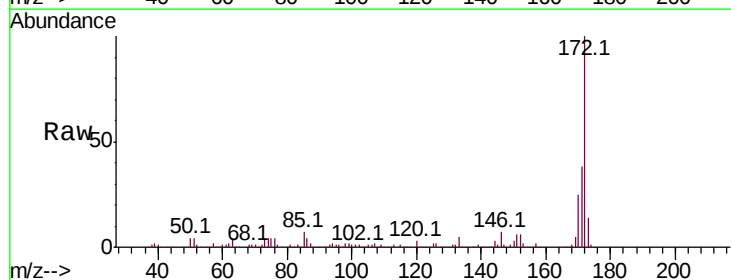



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

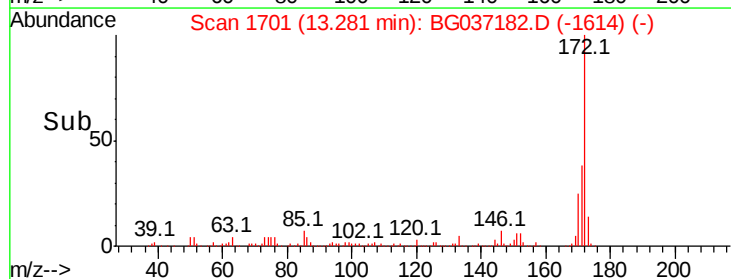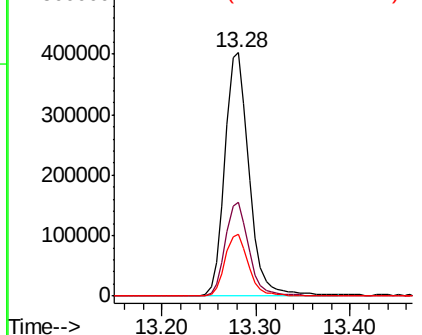

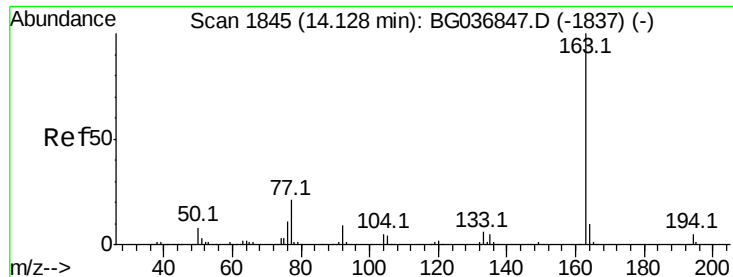

#49

Dimethylphthalate

Concen: 18.839 ng

RT: 14.10 min Scan# 1841

Delta R.T. -0.02 min

Lab File: BG037182.D

Acq: 5 Oct 2018 9:58

Instrument :

BNA_G

ClientSampleId :

100218-JETT-E-D-S


Tot Ion:163 Resp: 173973

Ion Ratio Lower Upper

163 100

194 3.9 4.0 6.0#




164 10.7 8.1 12.1

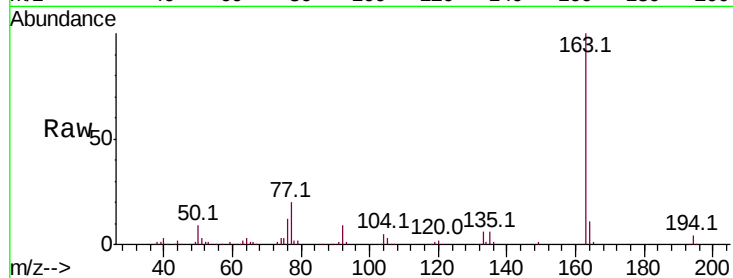

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

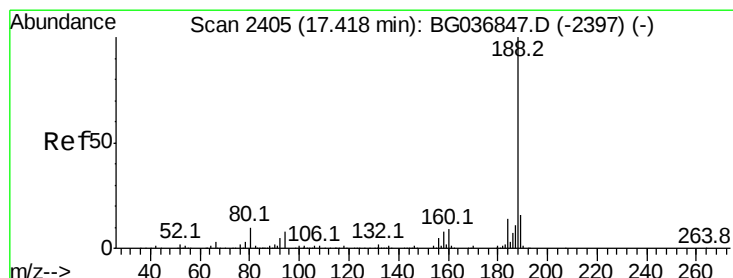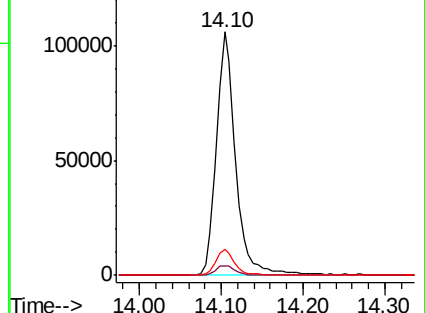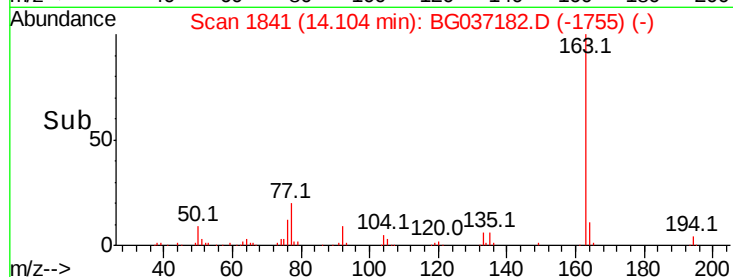

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2402

Delta R.T. -0.02 min

Lab File: BG037182.D

Acq: 5 Oct 2018 9:58


Tgt Ion:188 Resp: 301103

Ion Ratio Lower Upper

188 100

94 8.6 6.7 10.1



80 10.8 8.1 12.1

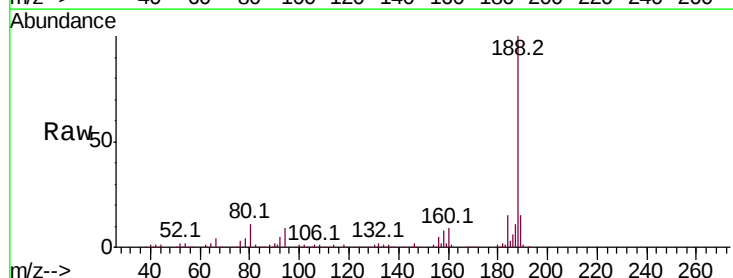


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

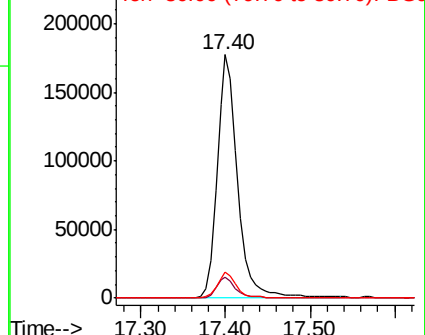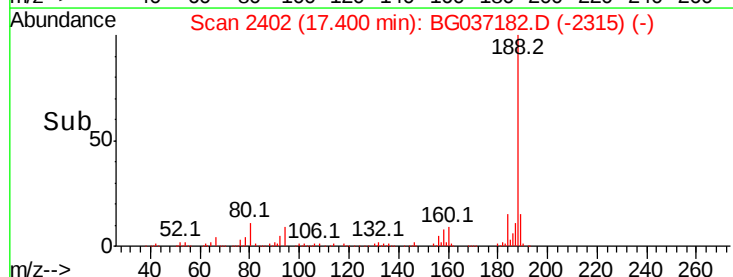

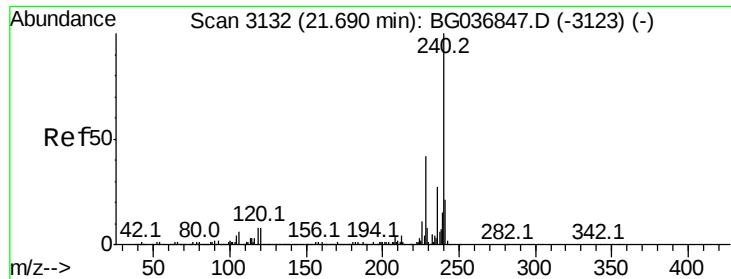

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3128

Delta R.T. -0.02 min

Lab File: BG037182.D

Acq: 5 Oct 2018 9:58

Instrument :

BNA_G

ClientSampleId :

100218-JETT-E-D-S


Tot Ion:240 Resp: 312445

Ion Ratio Lower Upper

240 100

120 8.7 6.9 10.3




236 26.7 21.2 31.8

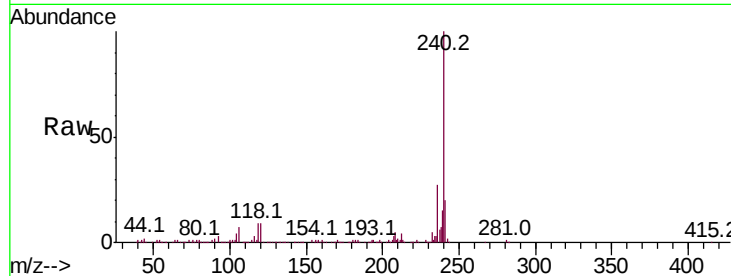

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

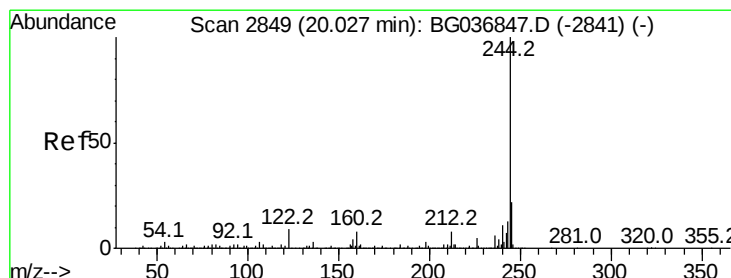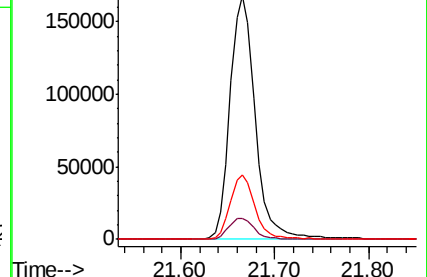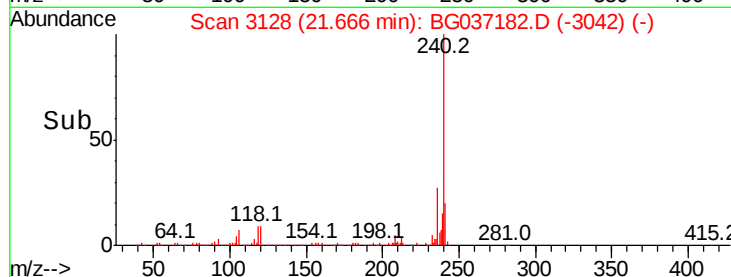

#78

Terphenyl-d14

Concen: 114.537 ng

RT: 20.01 min Scan# 2846

Delta R.T. -0.02 min

Lab File: BG037182.D

Acq: 5 Oct 2018 9:58


Tgt Ion:244 Resp: 1360971

Ion Ratio Lower Upper

244 100

212 9.2 7.0 10.6



122 10.3 7.1 10.7

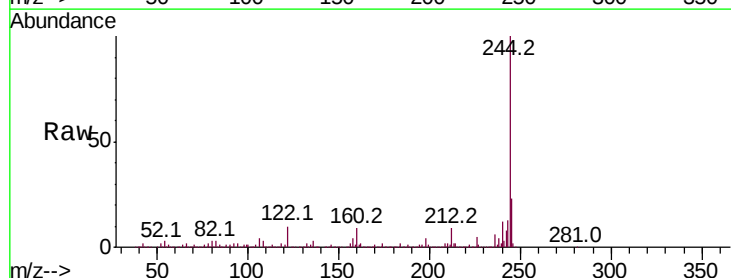


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

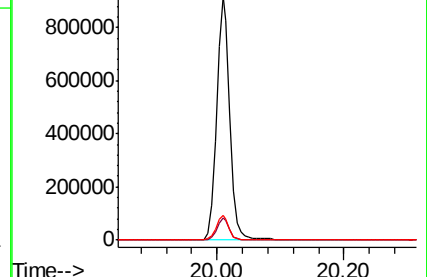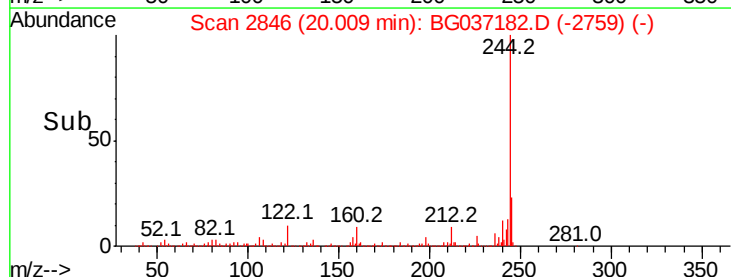


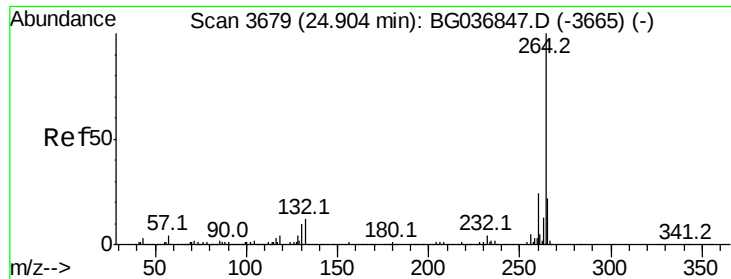

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.86 min Scan# 3672
Delta R.T. -0.04 min
Lab File: BG037182.D
Acq: 5 Oct 2018 9:58

Instrument :
BNA_G
ClientSampleId :
100218-JETT-E-D-S

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.6	29.4
265	21.7	17.4	26.0

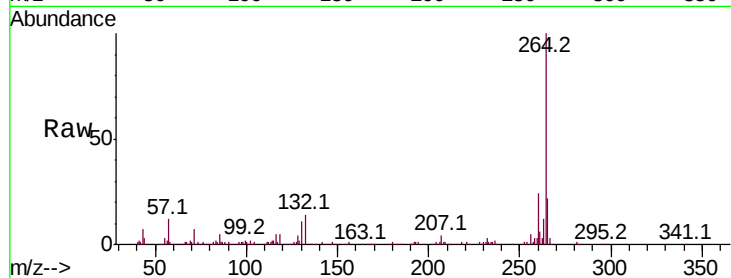

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

