

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100518\
 Data File : BG037185.D
 Acq On : 5 Oct 2018 11:55
 Operator : JU/SJ
 Sample : J5219-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FK-BPM-01-E10-F10-E10A-F10A

Quant Time: Oct 05 13:17:35 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	40243	20.00	ng	-0.02
21) Naphthalene-d8	10.84	136	162950	20.00	ng	-0.02
38) Acenaphthene-d10	14.66	164	104246	20.00	ng	-0.02
63) Phenanthrene-d10	17.40	188	265426	20.00	ng	-0.02
75) Chrysene-d12	21.67	240	276429	20.00	ng	-0.02
86) Perylene-d12	24.86	264	265899	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	213286	101.64	ng	-0.01
7) Phenol-d6	7.19	99	294790	90.80	ng	-0.02
23) Nitrobenzene-d5	9.19	82	196943	64.72	ng	-0.02
41) 2,4,6-Tribromophenol	16.14	330	114223	91.58	ng	-0.02
44) 2-Fluorobiphenyl	13.28	172	413419	59.07	ng	-0.02
78) Terphenyl-d14	20.01	244	709107	67.45	ng	-0.02
Target Compounds						Qvalue
49) Dimethylphthalate	14.10	163	176723	21.061	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100518\
Data File : BG037185.D
Acq On : 5 Oct 2018 11:55
Operator : JU/SJ
Sample : J5219-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FK-BPM-01-E10-F10-E10A-F10A

Quant Time: Oct 05 13:17:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

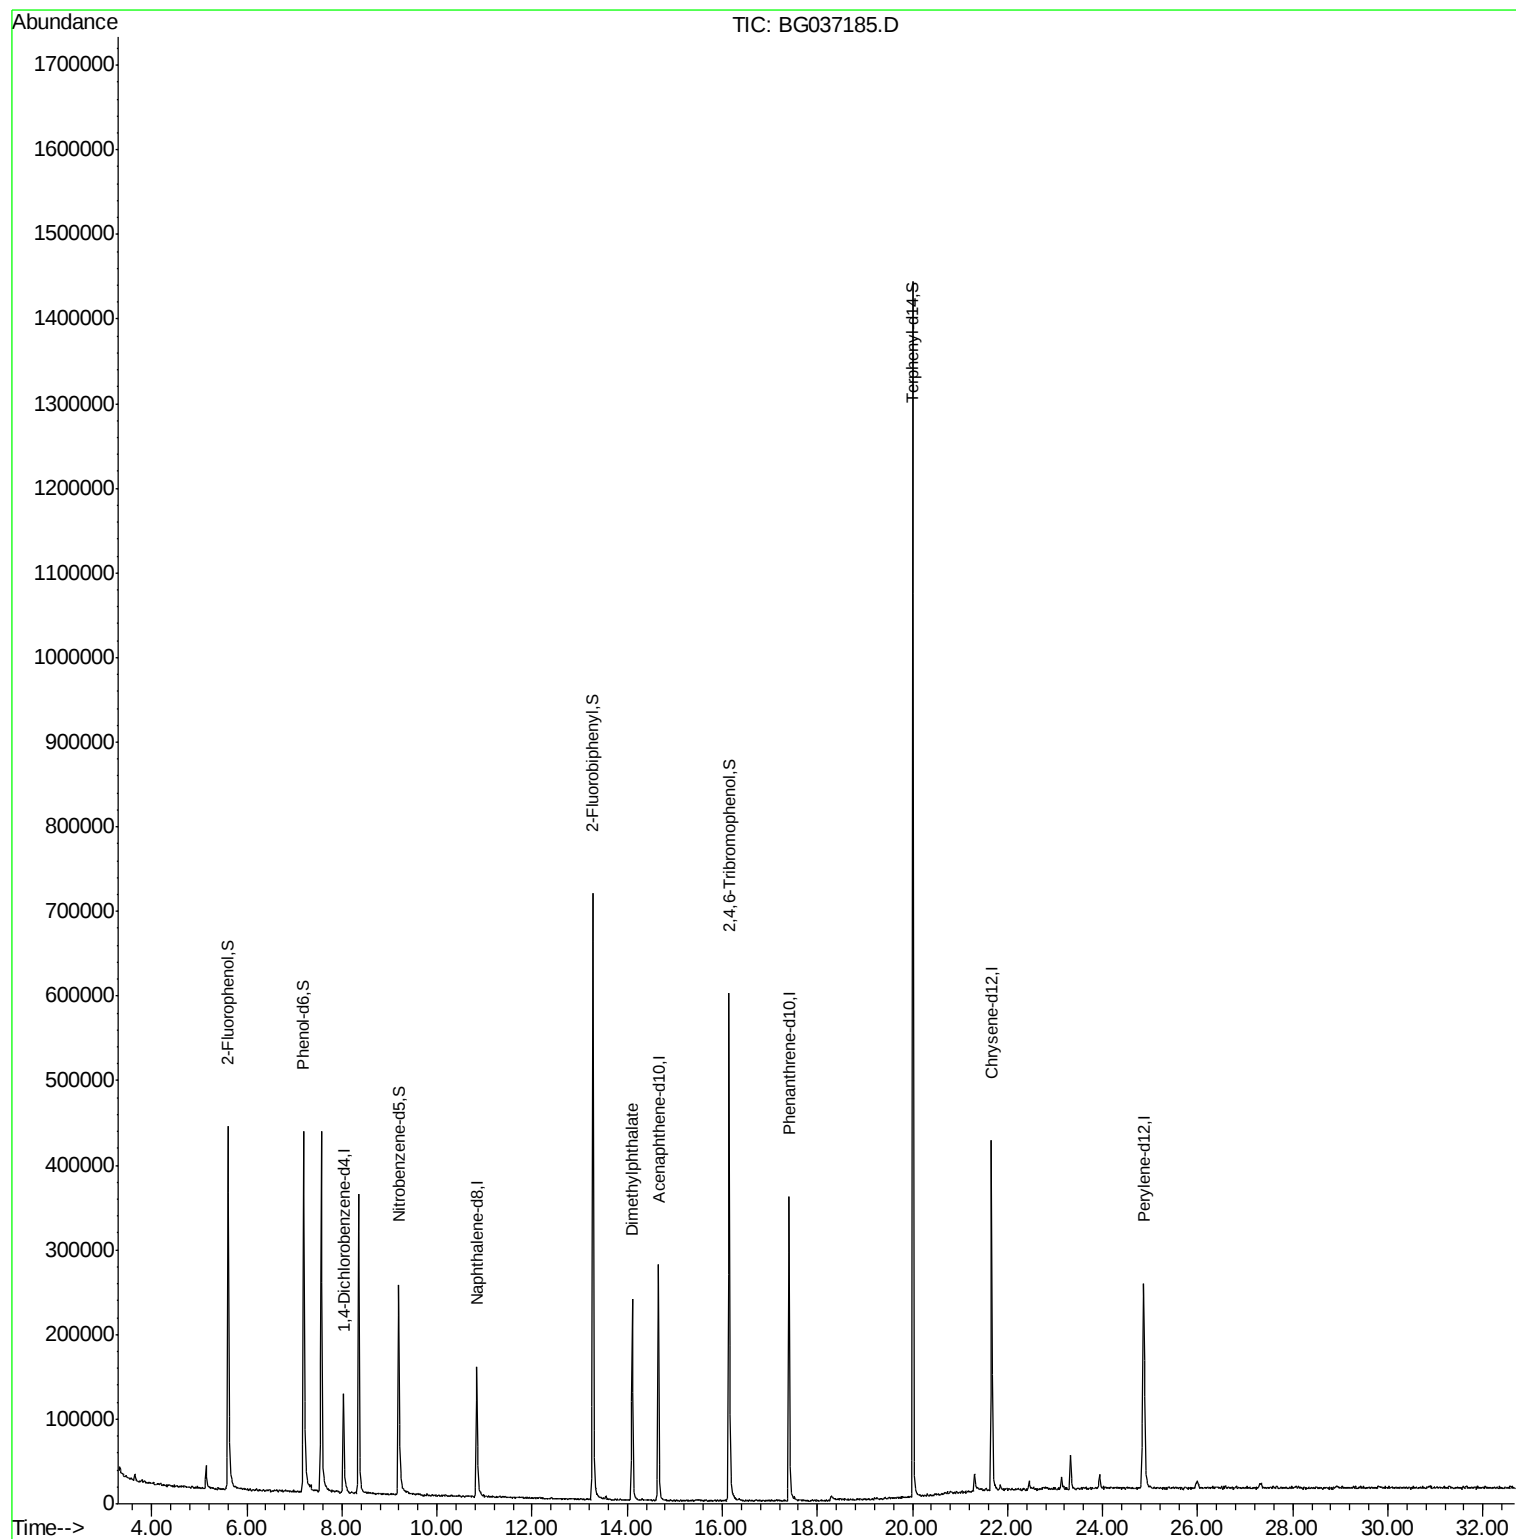

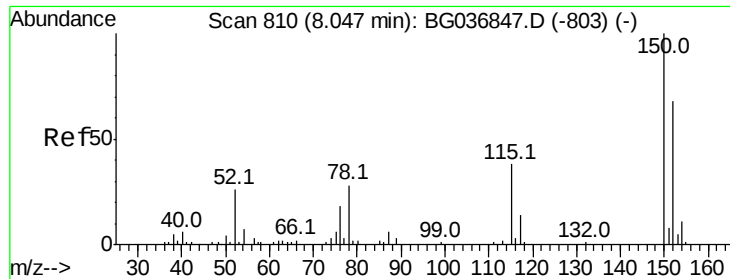


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.03 min Scan# 807
Delta R.T. -0.02 min
Lab File: BG037185.D
Acq: 5 Oct 2018 11:55

Instrument :
BNA_G
ClientSampleId :
FK-BPM-01-E10-F10-E10A-F10A

Tot Ion:152 Resp: 40243
Ion Ratio Lower Upper
152 100
150 150.3 119.5 179.3
115 59.7 44.5 66.7

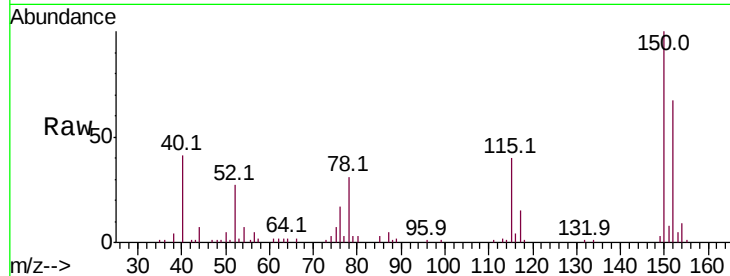


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

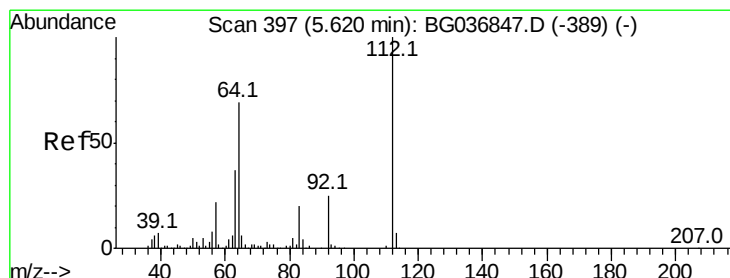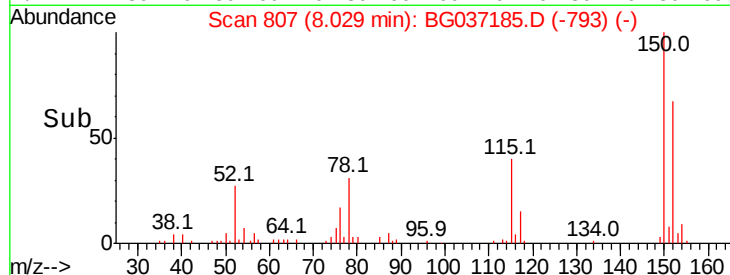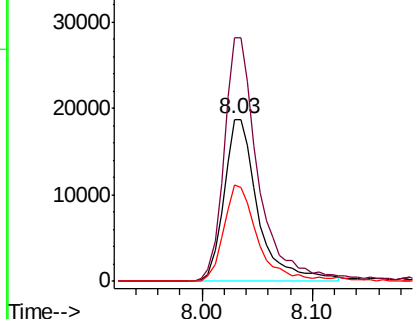



#5

2-Fluorophenol
Concen: 101.642 ng
RT: 5.61 min Scan# 395
Delta R.T. -0.01 min
Lab File: BG037185.D
Acq: 5 Oct 2018 11:55

Tgt Ion:112 Resp: 213286
Ion Ratio Lower Upper
112 100
64 72.1 57.2 85.8
63 37.5 30.8 46.2

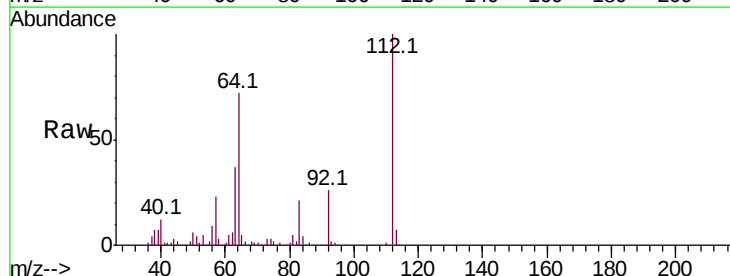

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG
Ion 63.00 (62.70 to 63.70): BG

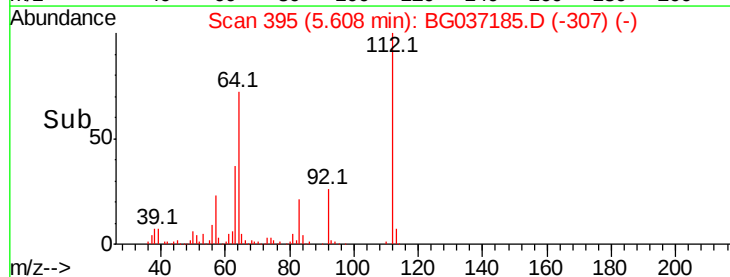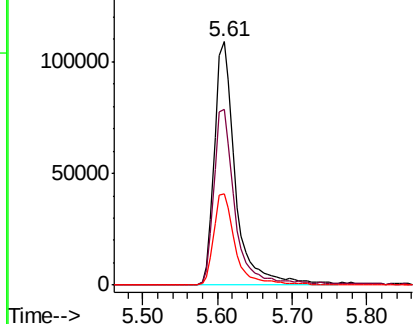



#7

Phenol-d6

Concen: 90.800 ng

RT: 7.19 min Scan# 665

Delta R.T. -0.02 min

Lab File: BG037185.D

Acq: 5 Oct 2018 11:55

Instrument :

BNA_G

ClientSampleId :

FK-BPM-01-E10-F10-E10A-F10A


Tot Ion: 99 Resp: 294790

Ion Ratio Lower Upper



99 100

42 21.7 16.5 24.7

71 38.1 29.4 44.2

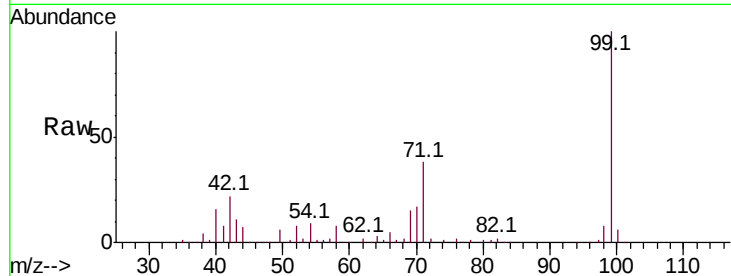

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

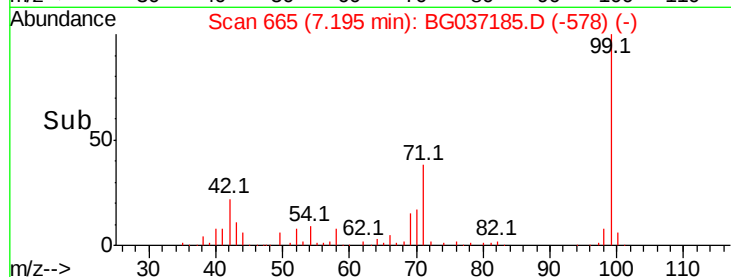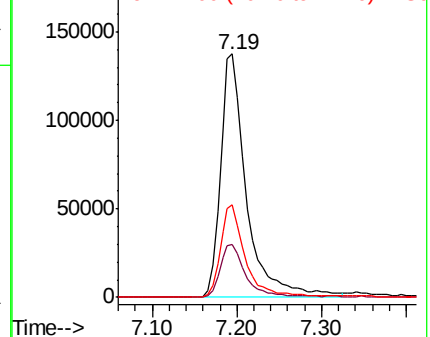

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.84 min Scan# 1285

Delta R.T. -0.02 min

Lab File: BG037185.D

Acq: 5 Oct 2018 11:55

Tgt Ion: 136 Resp: 162950


Ion Ratio Lower Upper

136 100



137 10.9 8.8 13.2


54 10.0 9.2 13.8

68 6.5 5.8 8.6

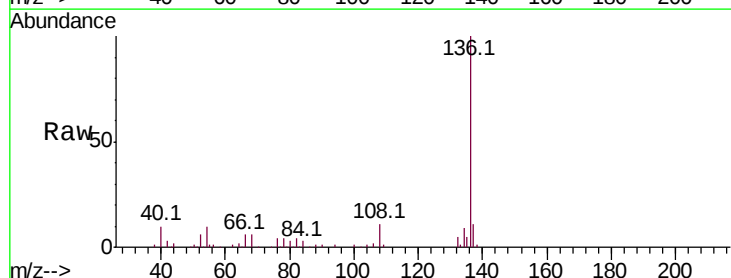

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC


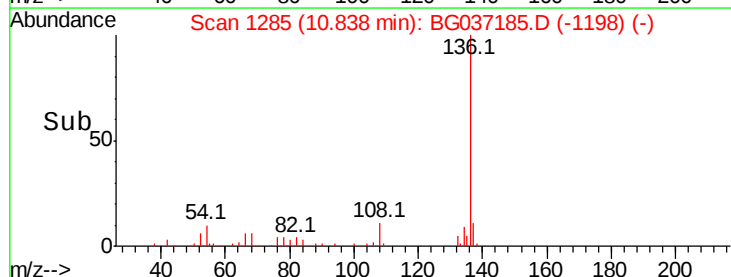
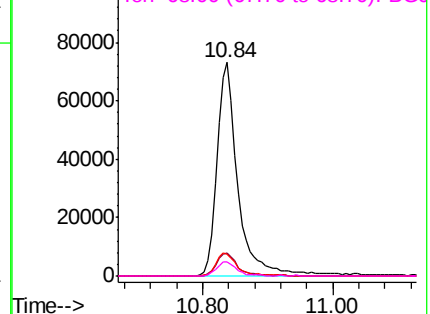


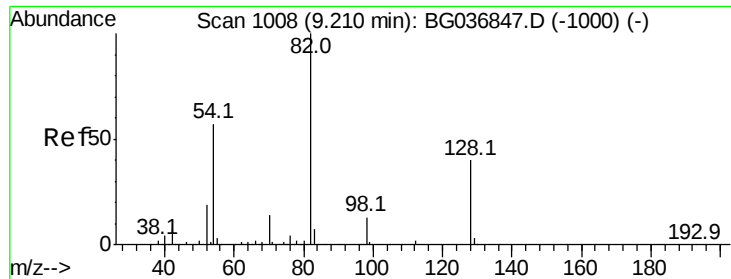

#23
 Nitrobenzene-d5
 Concen: 64.722 ng
 RT: 9.19 min Scan# 1005
 Delta R.T. -0.02 min
 Lab File: BG037185.D
 Acq: 5 Oct 2018 11:55




Instrument :
 BNA_G
 ClientSampleId :
 FK-BPM-01-E10-F10-E10A-F10A

Tot Ion: 82 Resp: 196943
 Ion Ratio Lower Upper
 82 100
 128 38.4 33.3 49.9
 54 56.5 45.1 67.7

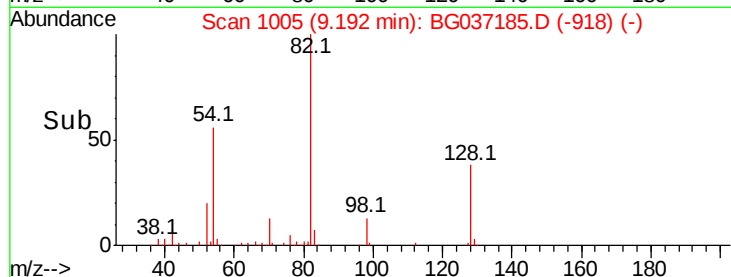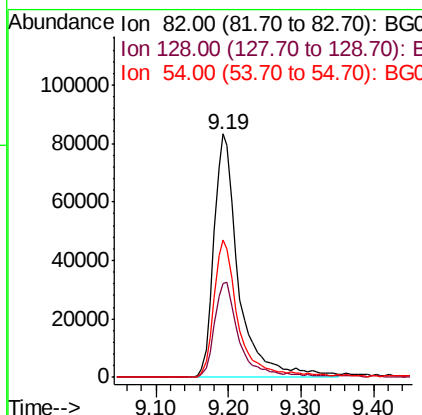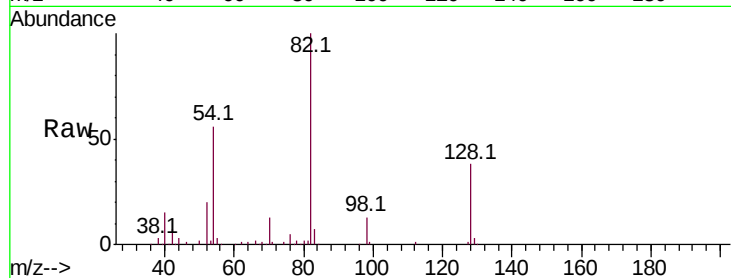

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.66 min Scan# 1935
 Delta R.T. -0.02 min
 Lab File: BG037185.D
 Acq: 5 Oct 2018 11:55

Tgt Ion: 164 Resp: 104246
 Ion Ratio Lower Upper
 164 100
 162 98.3 80.7 121.1
 160 46.2 35.3 52.9

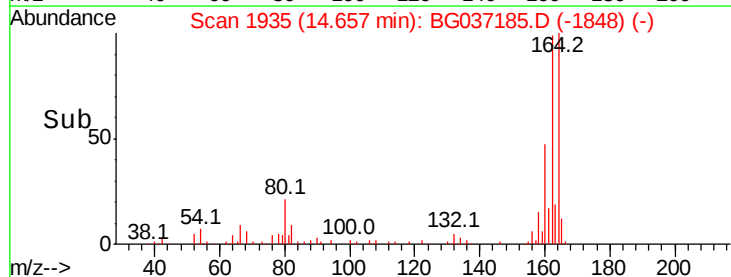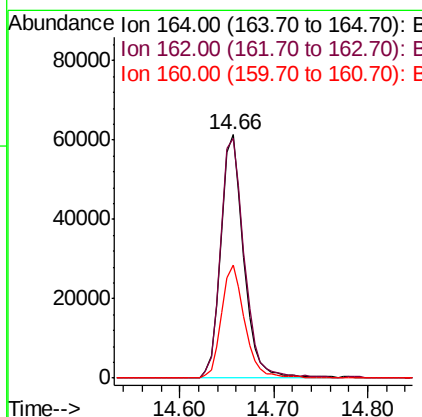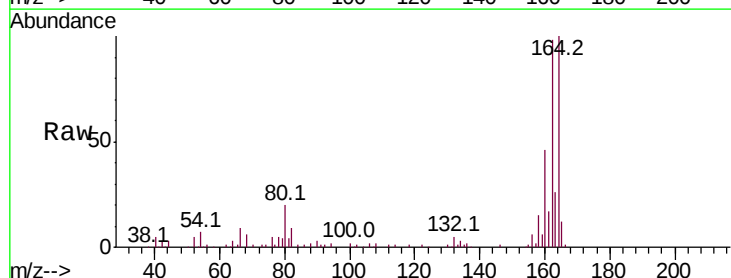






#41
 2,4,6-Tribromophenol
 Concen: 91.581 ng
 RT: 16.14 min Scan# 2188
 Delta R.T. -0.02 min
 Lab File: BG037185.D
 Acq: 5 Oct 2018 11:55

Instrument :
 BNA_G
 ClientSampleId :
 FK-BPM-01-E10-F10-E10A-F10A

Tot Ion:330 Resp: 114223
 Ion Ratio Lower Upper
 330 100
 332 96.7 75.4 113.2
 141 41.9 30.7 46.1

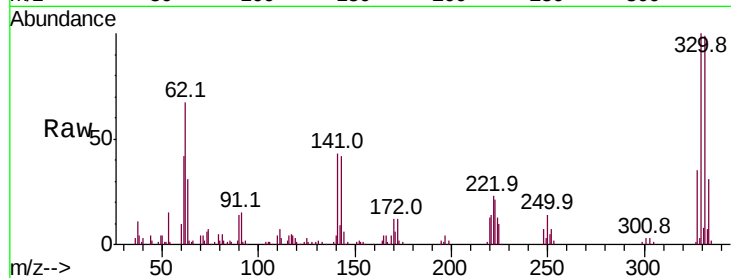


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

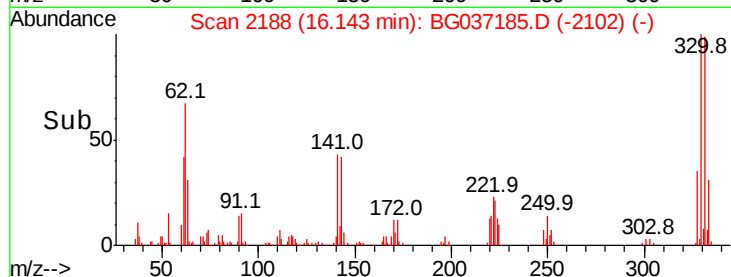
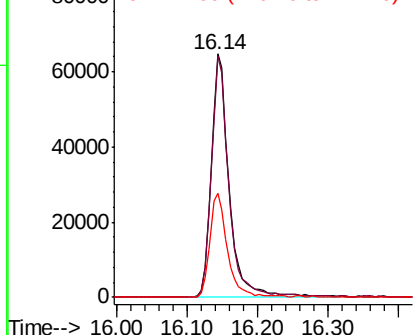



#44
 2-Fluorobiphenyl
 Concen: 59.066 ng
 RT: 13.28 min Scan# 1700
 Delta R.T. -0.02 min
 Lab File: BG037185.D
 Acq: 5 Oct 2018 11:55

Tgt Ion:172 Resp: 413419
 Ion Ratio Lower Upper
 172 100
 171 35.5 31.3 46.9
 170 23.9 21.0 31.6

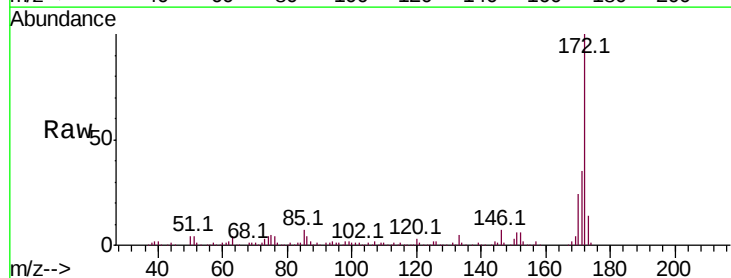

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

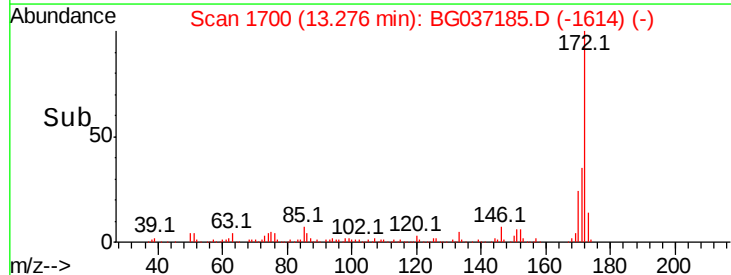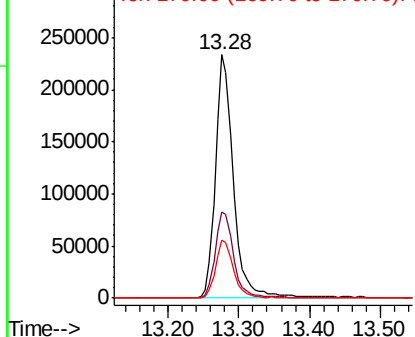

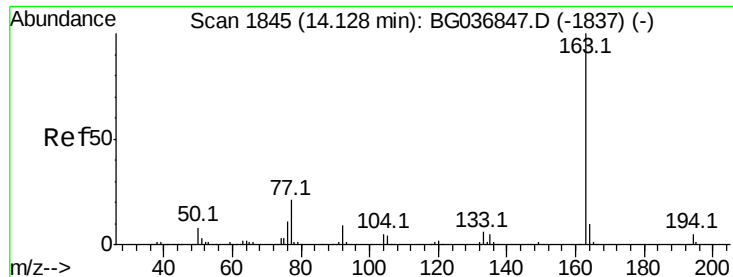

#49

Dimethylphthalate

Concen: 21.061 ng

RT: 14.10 min Scan# 1841

Delta R.T. -0.02 min

Lab File: BG037185.D

Acq: 5 Oct 2018 11:55

Instrument :

BNA_G

ClientSampleId :

FK-BPM-01-E10-F10-E10A-F10A


Tot Ion:163 Resp: 176723

Ion Ratio Lower Upper

163 100

194 4.5 4.0 6.0




164 10.7 8.1 12.1

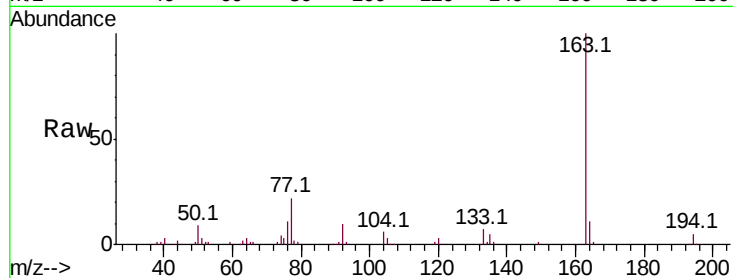

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

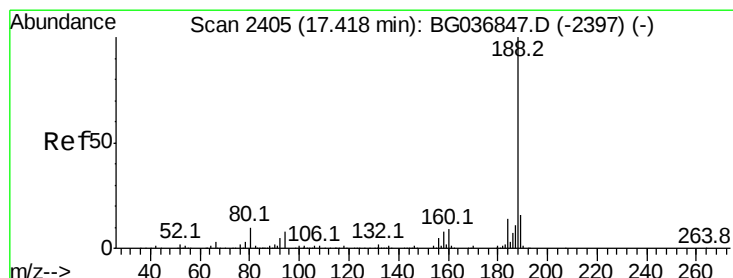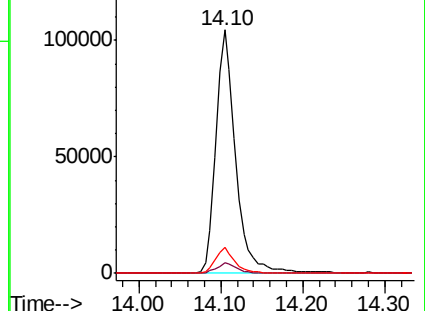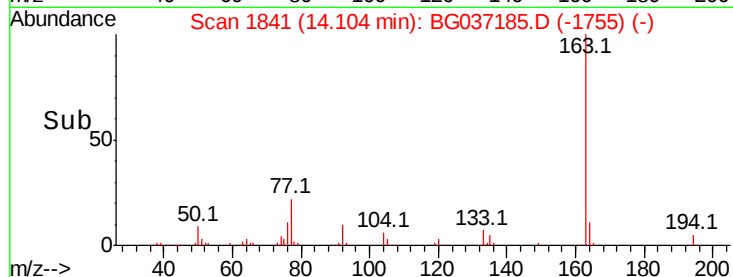

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.40 min Scan# 2402

Delta R.T. -0.02 min

Lab File: BG037185.D

Acq: 5 Oct 2018 11:55


Tgt Ion:188 Resp: 265426

Ion Ratio Lower Upper

188 100

94 8.2 6.7 10.1



80 10.5 8.1 12.1

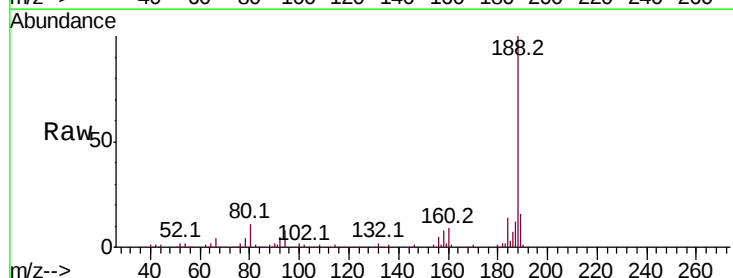


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

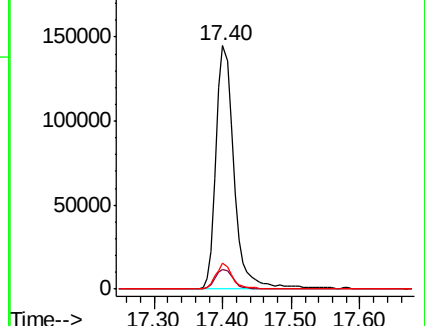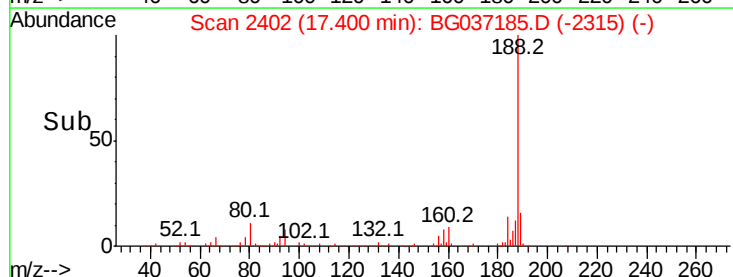

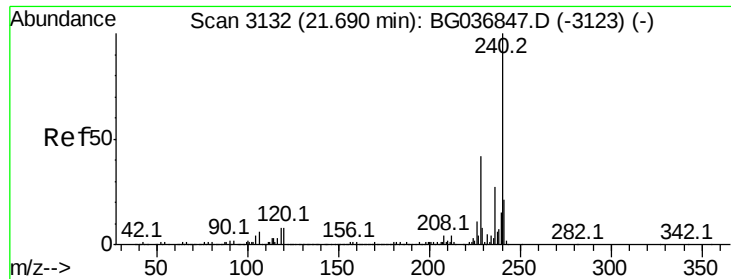

#75

Chrysene-d12

Concen: 20.000 ng

RT: 21.67 min Scan# 3128

Delta R.T. -0.02 min

Lab File: BG037185.D

Acq: 5 Oct 2018 11:55

Instrument :

BNA_G

ClientSampleId :

FK-BPM-01-E10-F10-E10A-F10A


Tot Ion:240 Resp: 276429

Ion Ratio Lower Upper

240 100

120 8.5 6.9 10.3




236 25.0 21.2 31.8

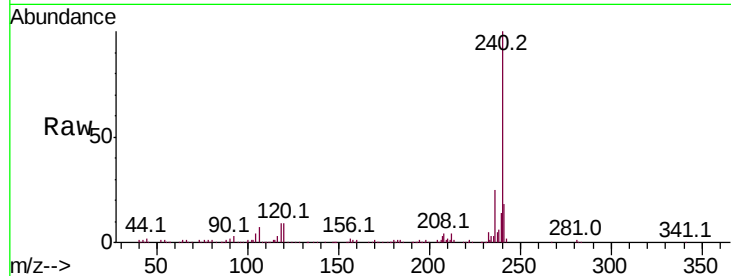

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

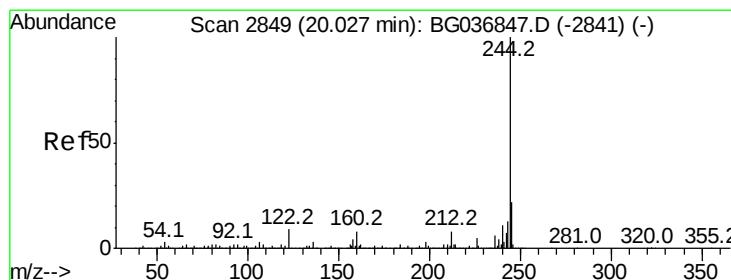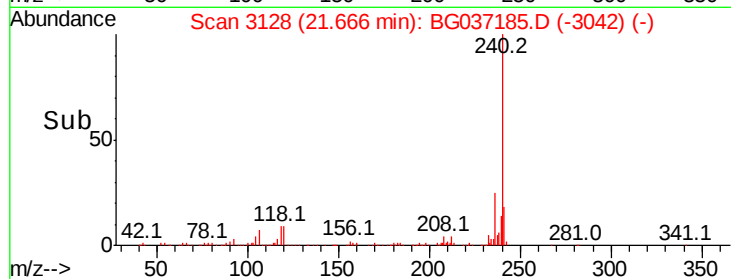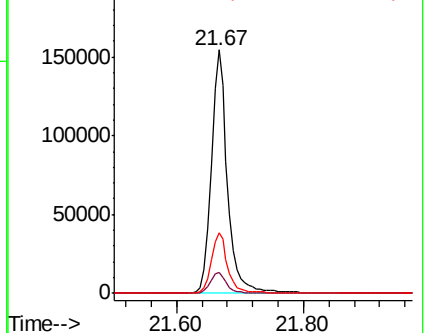

#78

Terphenyl-d14

Concen: 67.453 ng

RT: 20.01 min Scan# 2846

Delta R.T. -0.02 min

Lab File: BG037185.D

Acq: 5 Oct 2018 11:55


Tgt Ion:244 Resp: 709107

Ion Ratio Lower Upper

244 100

212 7.8 7.0 10.6



122 9.6 7.1 10.7

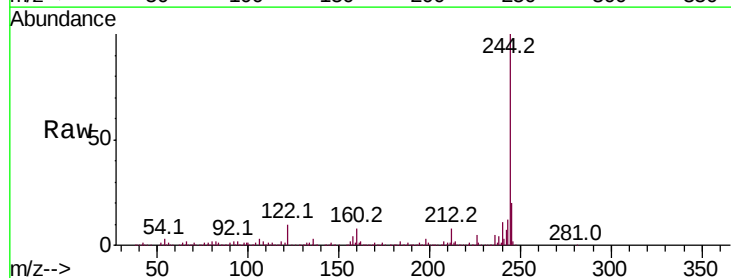


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

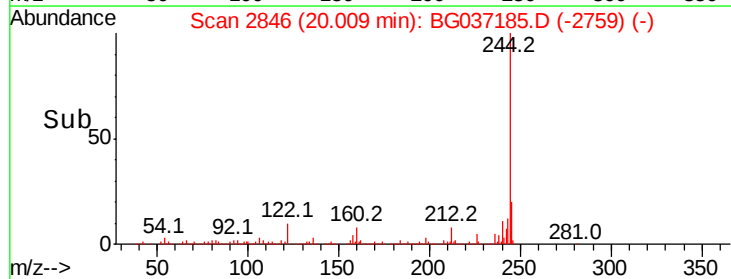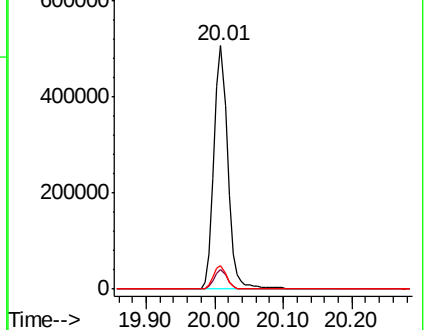

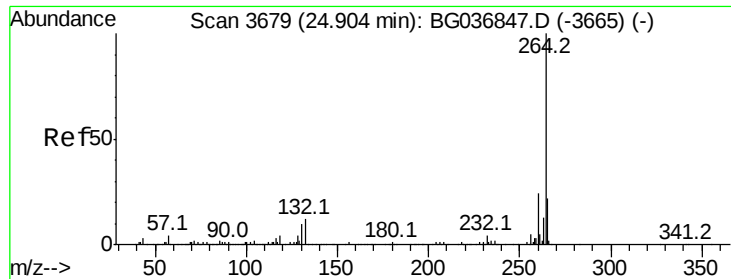

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.86 min Scan# 3672
Delta R.T. -0.04 min
Lab File: BG037185.D
Acq: 5 Oct 2018 11:55

Instrument :
BNA_G
ClientSampleId :
FK-BPM-01-E10-F10-E10A-F10A

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.3	19.6	29.4
265	20.5	17.4	26.0

