
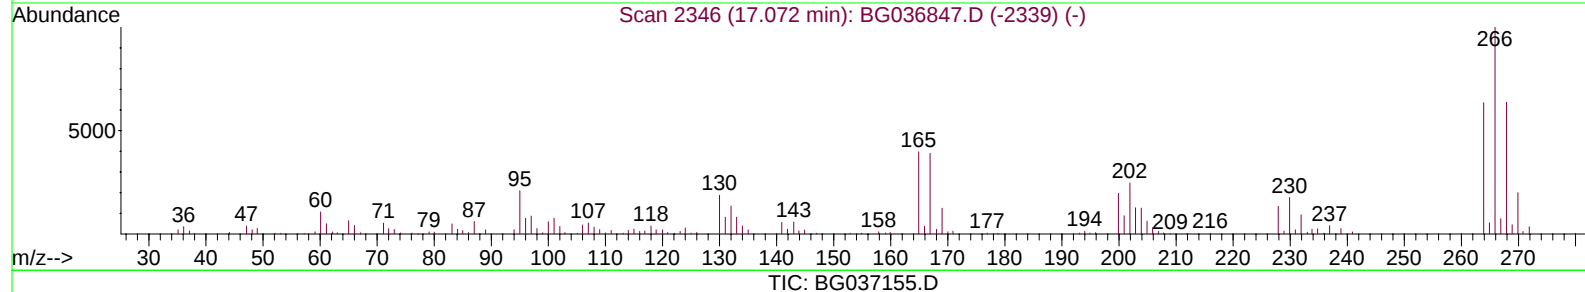
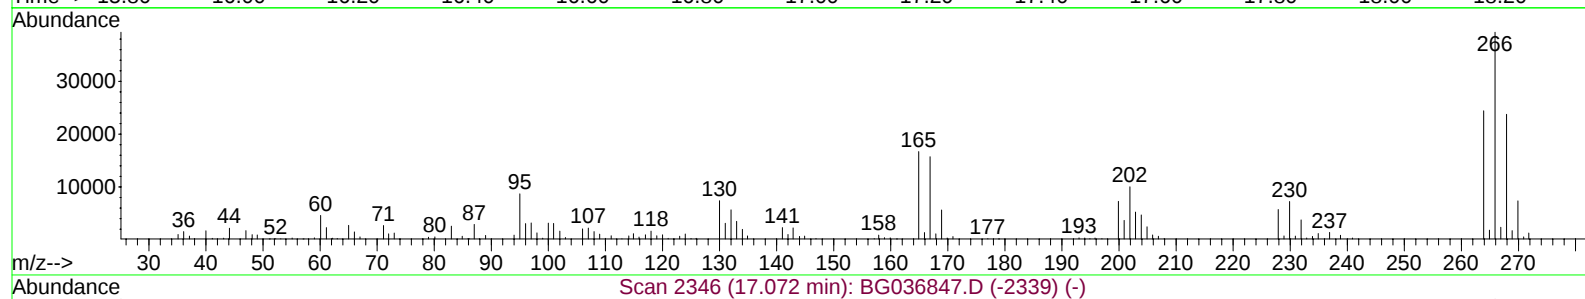


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100518\
Data File : BG037155.D
Acq On : 4 Oct 2018 14:56
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 11:29:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

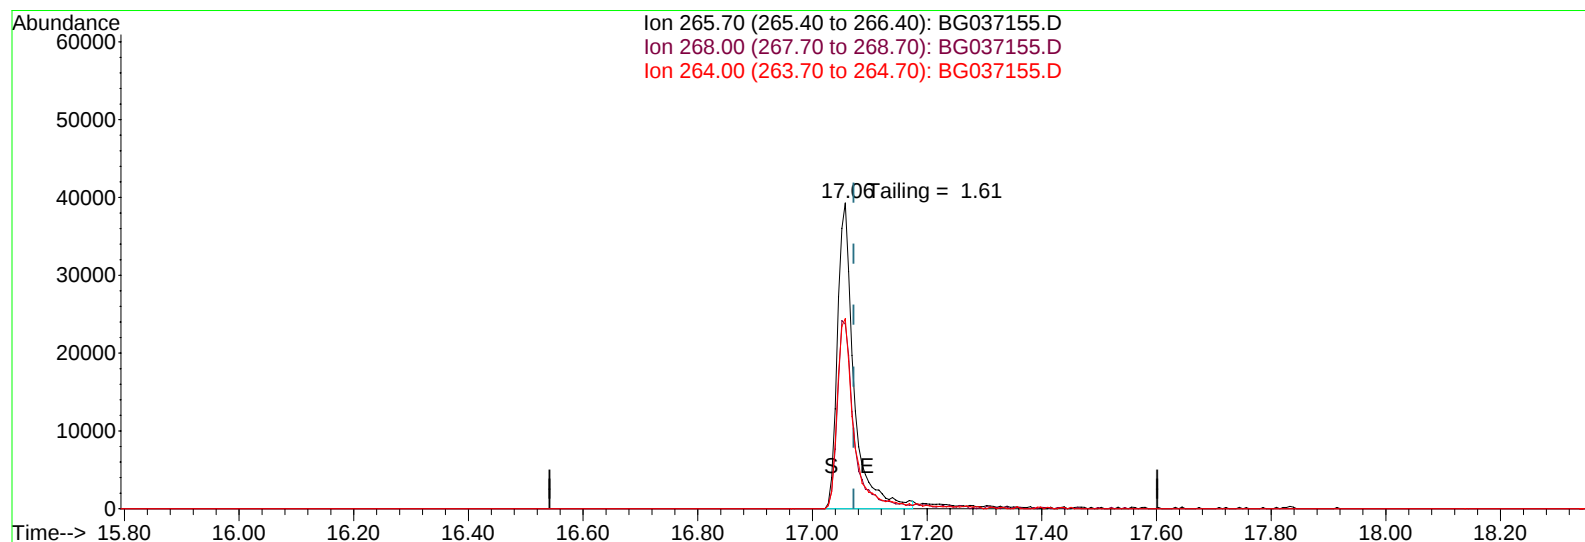

(69) Pentachlorophenol (C)




17.057min (-0.014) 27701.23ng

response 78049

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	60.46
264.00	61.10	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100518\
 Data File : BG037155.D
 Acq On : 4 Oct 2018 14:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 11:29:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Sep 24 10:41:23 2018
 Response via : Initial Calibration

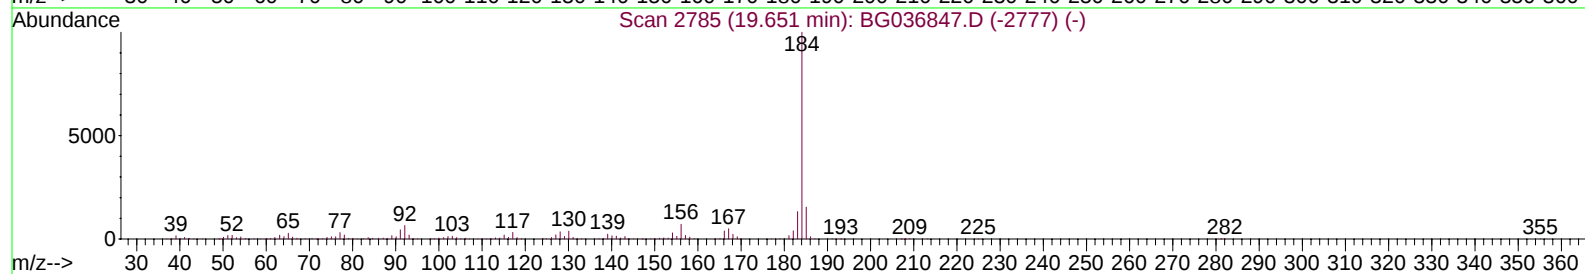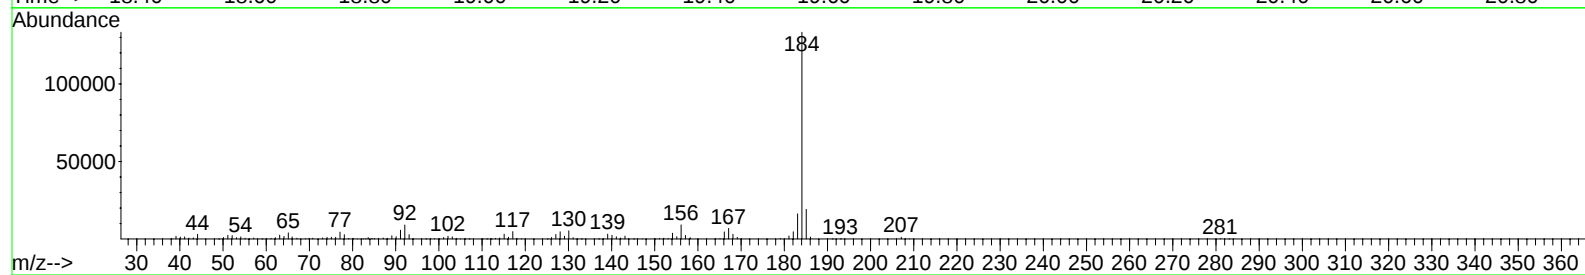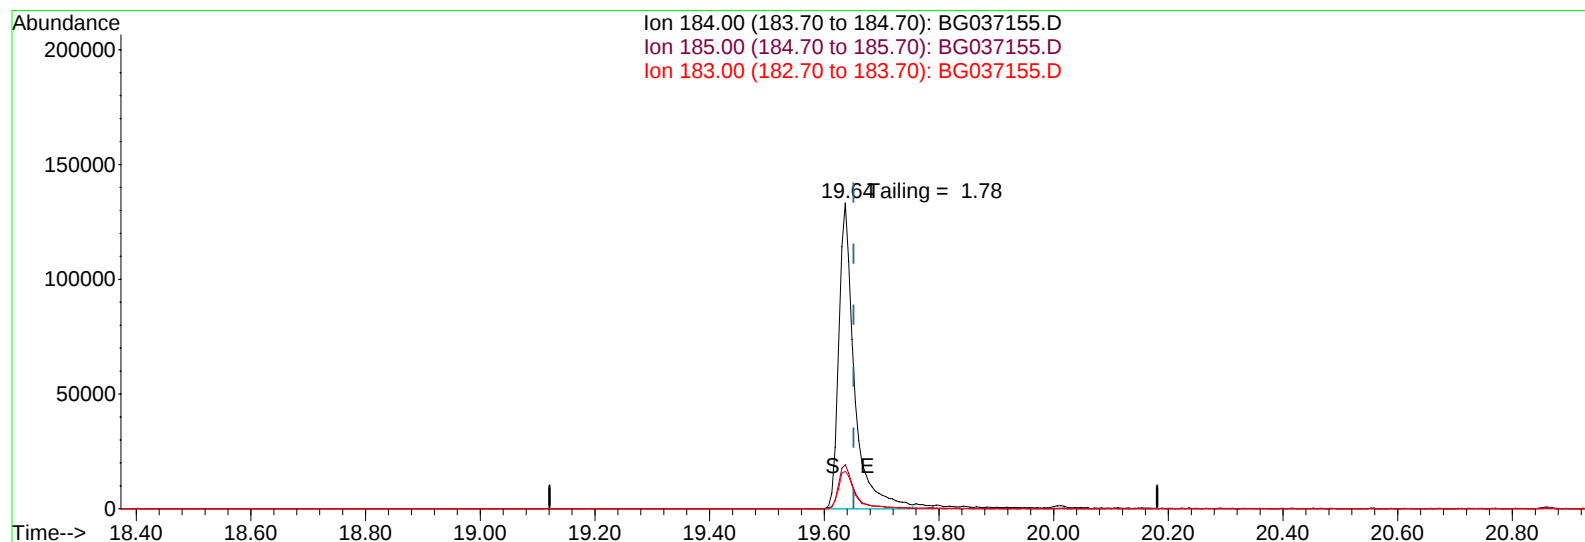

TIC: BG037155.D

(76) Benzidine

19.636min (-0.014) 399.94ng

response 252886

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.40
183.00	13.60	12.27
0.00	0.00	0.00