
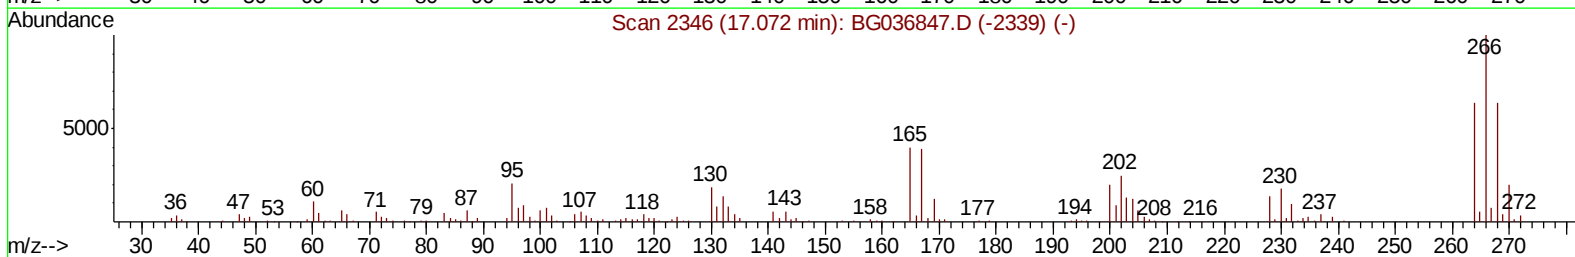
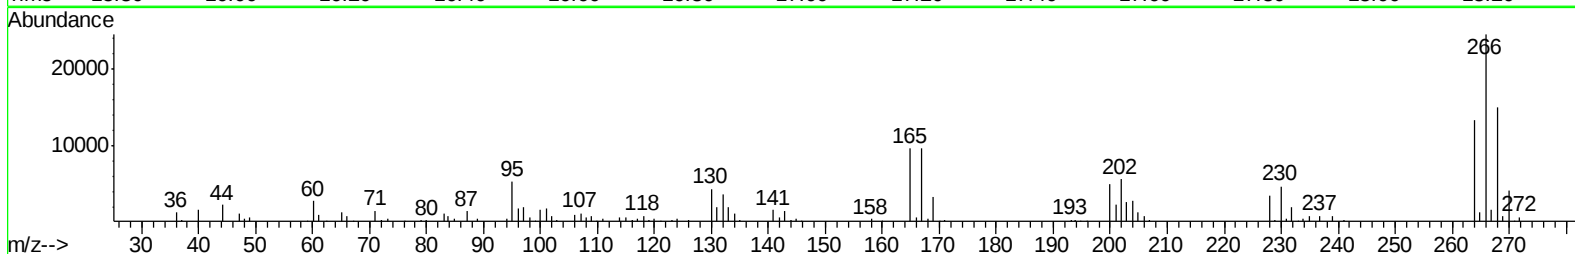


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100518\
Data File : BG037174.D
Acq On : 5 Oct 2018 4:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:36:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

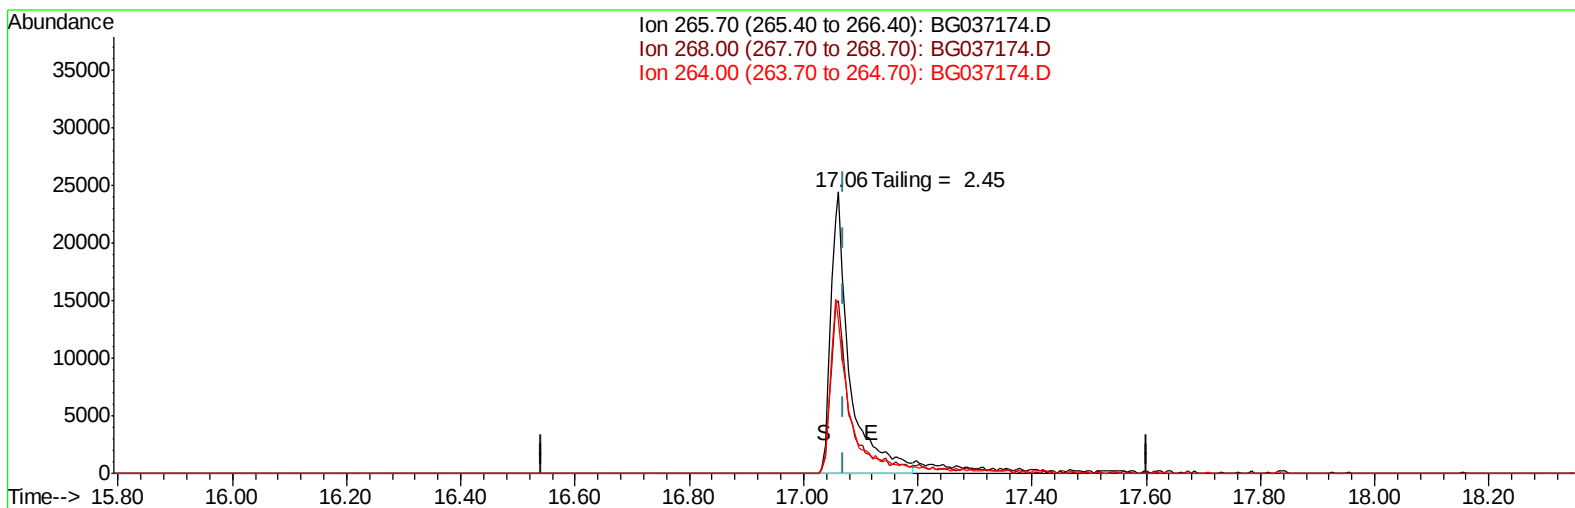

TIC: BG037174.D

(69) Pentachlorophenol (C)




17.061min (-0.010) 55454.14ng

response 55626

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.28
264.00	61.10	54.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100518\
Data File : BG037174.D
Acq On : 5 Oct 2018 4:46
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 05:36:43 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 24 10:41:23 2018
Response via : Initial Calibration

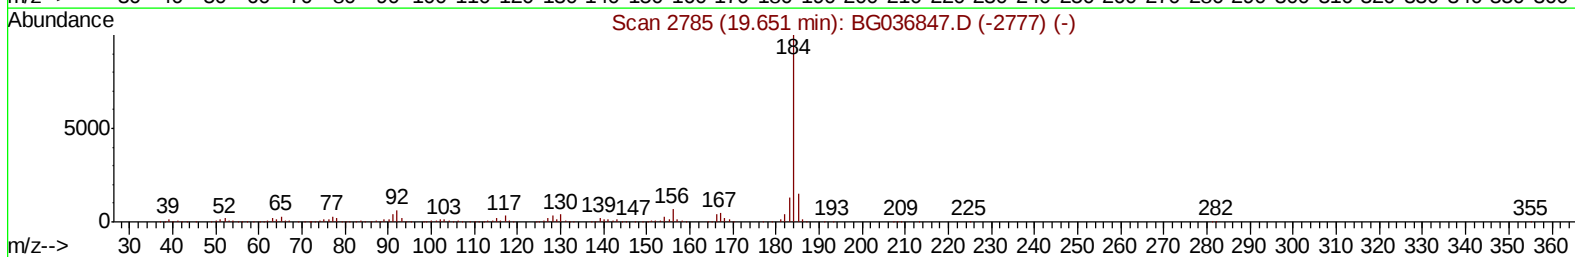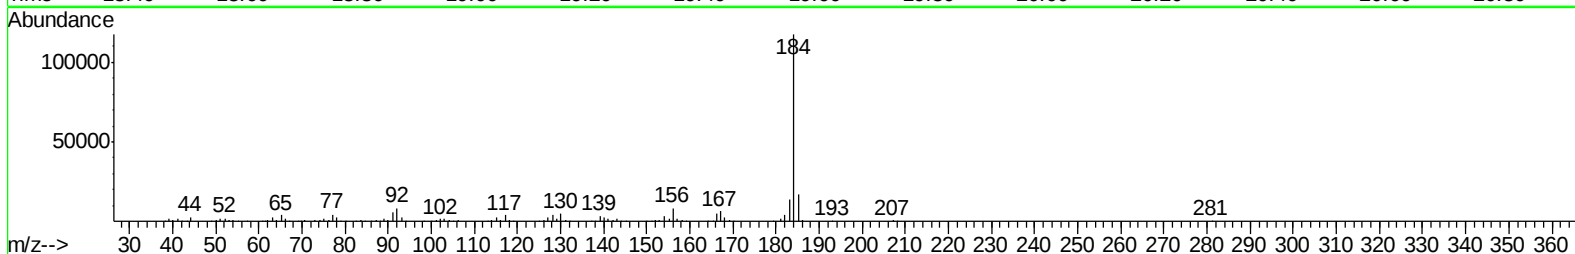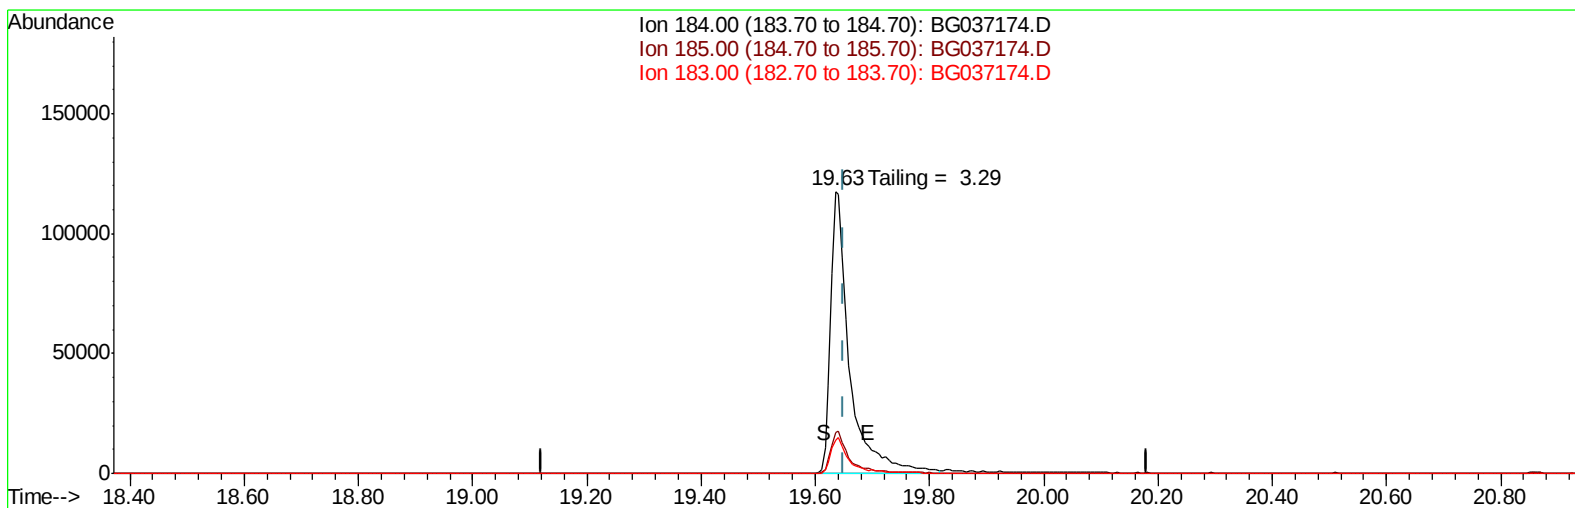

TIC: BG037174.D

(76) Benzidine

19.635min (-0.016) 6695.39ng

response 270001

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.68
183.00	13.60	11.92
0.00	0.00	0.00