

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100518\
 Data File : BG037167.D
 Acq On : 4 Oct 2018 22:42
 Operator : JU/SJ
 Sample : J5237-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 FBGW10318

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.609	389	395	415	rBV	194835	408045	13.20%	3.276%
2	7.196	659	665	674	rBV	106730	233946	7.57%	1.878%
3	7.566	721	728	747	rBV	417168	845312	27.36%	6.787%
4	8.036	801	808	822	rBV	100255	220541	7.14%	1.771%
5	8.353	855	862	878	rBV	425269	815615	26.39%	6.549%
6	9.193	998	1005	1027	rBV	331505	744830	24.10%	5.981%
7	10.838	1278	1285	1301	rBV	138093	298833	9.67%	2.399%
8	13.277	1694	1700	1720	rBV	956800	1740629	56.33%	13.976%
9	14.657	1929	1935	1946	rBV2	279570	488743	15.82%	3.924%
10	16.144	2180	2188	2209	rBV	646251	1219516	39.46%	9.792%
11	17.401	2396	2402	2415	rBV	388183	670504	21.70%	5.384%
12	20.010	2840	2846	2862	rBV	2181752	3090138	100.00%	24.812%
13	21.667	3122	3128	3141	rBV2	428328	769739	24.91%	6.181%
14	22.454	3257	3262	3267	rBV2	24254	36958	1.20%	0.297%
15	23.142	3374	3379	3386	rVB2	24278	45801	1.48%	0.368%
16	23.935	3508	3514	3521	rBV3	25399	57392	1.86%	0.461%
17	24.869	3662	3673	3685	rBV2	253326	767686	24.84%	6.164%


Sum of corrected areas: 12454228

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG100518\
Data File : BG037167.D
Acq On : 4 Oct 2018 22:42
Operator : JU/SJ
Sample : J5237-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FBGW10318

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

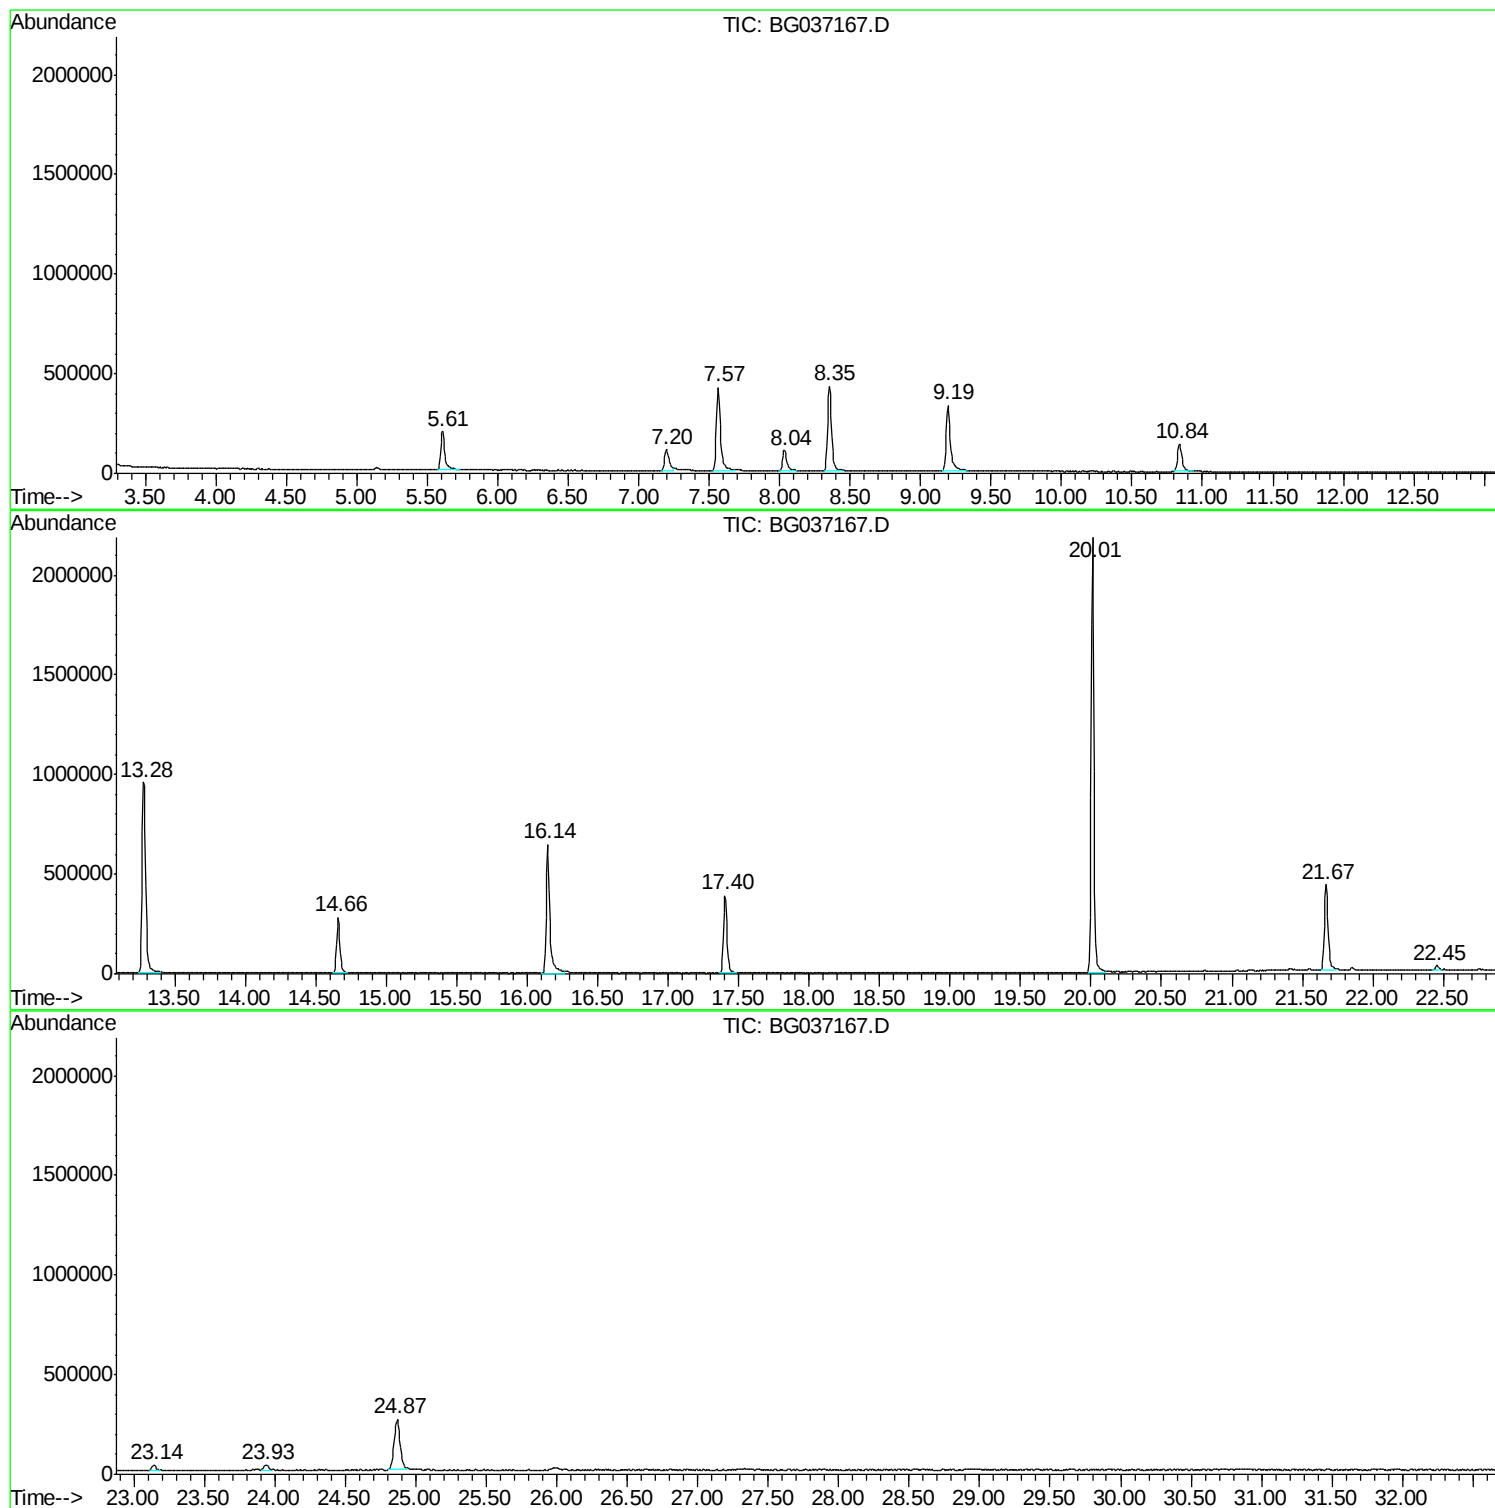

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100518\
Data File : BG037167.D
Acq On : 4 Oct 2018 22:42
Operator : JU/SJ
Sample : J5237-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FBGW10318

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100518\
Data File : BG037167.D
Acq On : 4 Oct 2018 22:42
Operator : JU/SJ
Sample : J5237-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FBGW10318

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc